

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102023\
 Data File : VV032511.D
 Acq On : 20 Oct 2023 09:45
 Operator : SY/MD
 Sample : VV1020WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK374

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032511.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.114	17	23	32	rVB	6262	8862	1.97%	0.281%
2	1.278	67	74	84	rBV	54410	57578	12.81%	1.826%
3	1.532	145	153	167	rVB	50176	58605	13.04%	1.859%
4	2.060	308	317	329	rBV	79593	115252	25.64%	3.655%
5	2.182	344	355	364	rVB2	9883	18368	4.09%	0.583%
6	2.452	431	439	447	rBV5	3825	6128	1.36%	0.194%
7	3.822	852	865	898	rBV2	34690	151772	33.76%	4.813%
8	4.252	983	999	1020	rBV	55341	146231	32.53%	4.638%
9	4.365	1024	1034	1035	rBV	6499	8114	1.81%	0.257%
10	4.960	1203	1219	1239	rBV2	137048	350327	77.94%	11.111%
11	5.047	1242	1246	1257	rVB6	7812	16283	3.62%	0.516%
12	5.539	1384	1399	1415	rBV	103864	221468	49.27%	7.024%
13	5.992	1525	1540	1555	rBV	83477	180068	40.06%	5.711%
14	6.918	1818	1828	1853	rBV	36910	78747	17.52%	2.497%
15	7.246	1917	1930	1955	rBV	140647	284404	63.27%	9.020%
16	7.561	2017	2028	2043	rBV2	22940	45023	10.02%	1.428%
17	8.030	2162	2174	2206	rBV	200896	449504	100.00%	14.256%
18	8.789	2398	2410	2429	rBV	171617	310332	69.04%	9.842%
19	10.156	2823	2835	2851	rBV2	69480	116279	25.87%	3.688%
20	11.188	3146	3156	3180	rBV	175979	282009	62.74%	8.944%
21	11.564	3262	3273	3292	rBV	154447	247756	55.12%	7.858%




Sum of corrected areas: 3153110

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102023\
Data File : VV032511.D
Acq On : 20 Oct 2023 09:45
Operator : SY/MD
Sample : VV1020WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK374

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

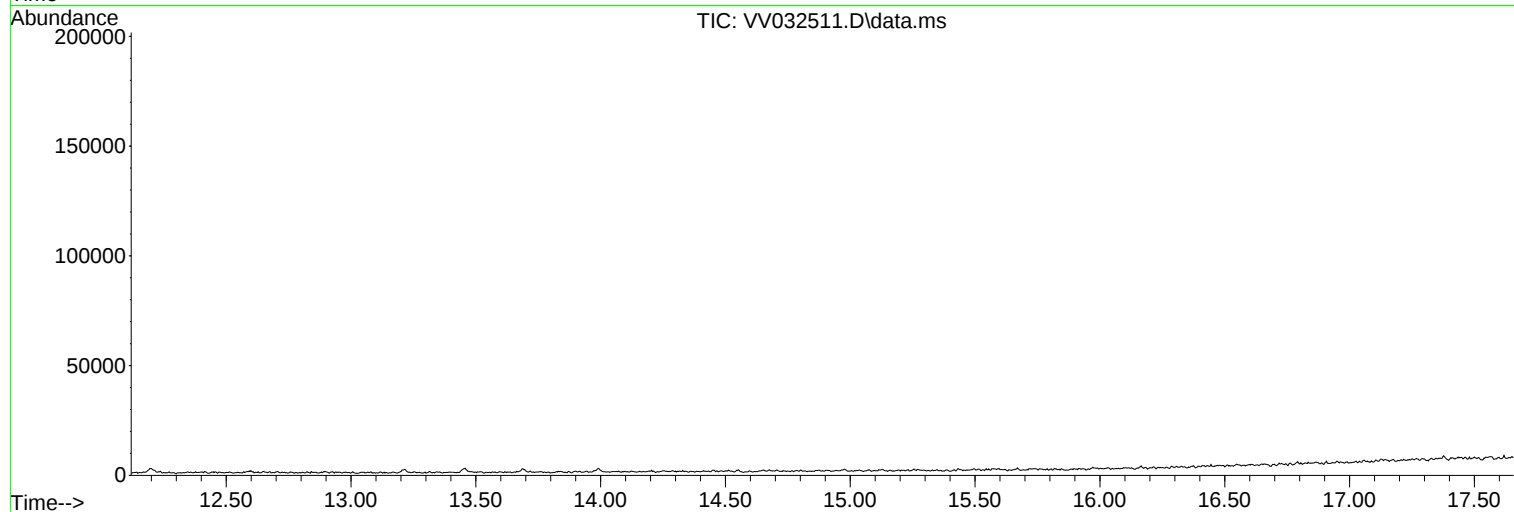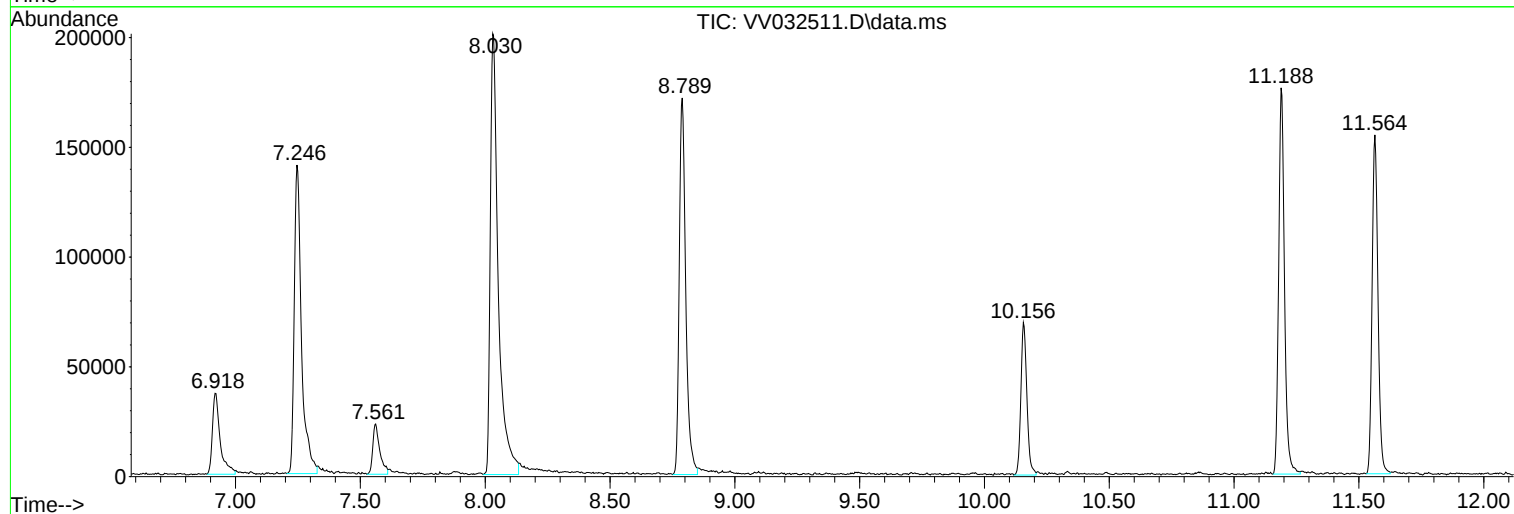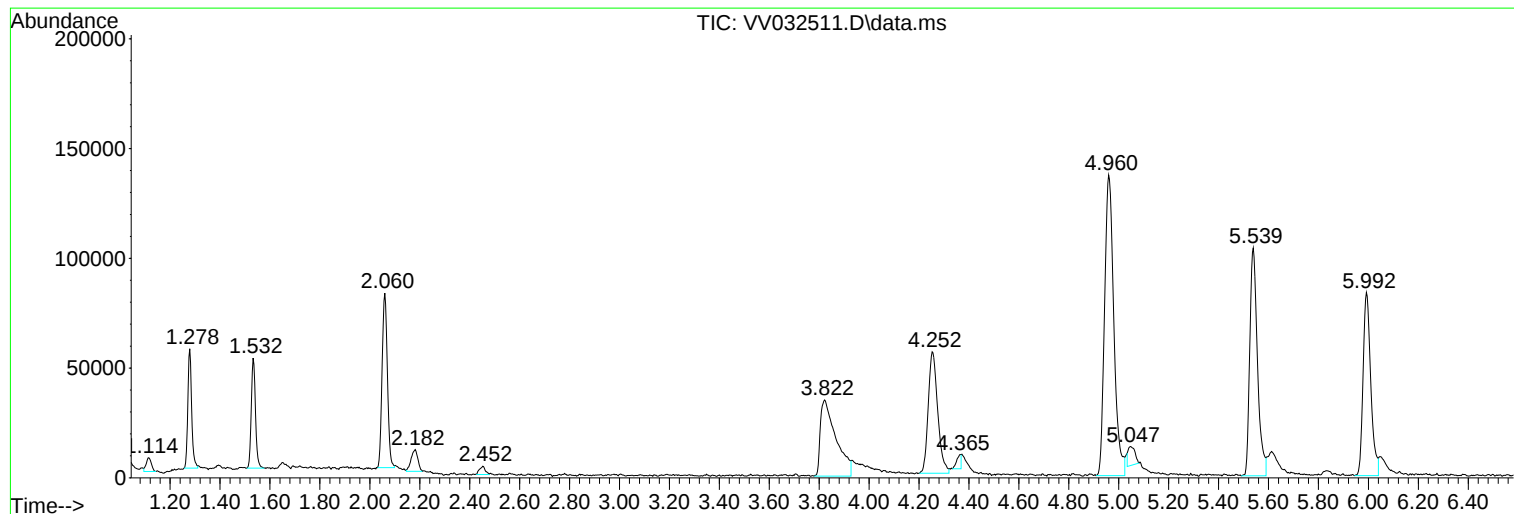

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102023\
Data File : VV032511.D
Acq On : 20 Oct 2023 09:45
Operator : SY/MD
Sample : VV1020WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK374

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102023\
Data File : VV032511.D
Acq On : 20 Oct 2023 09:45
Operator : SY/MD
Sample : VV1020WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK374

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc