

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102023\
 Data File : VV032514.D
 Acq On : 20 Oct 2023 11:04
 Operator : SY/MD
 Sample : 04950-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4A02

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032514.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	87	rVB	48811	52968	13.36%	1.742%
2	1.532	146	153	163	rBV	44103	52145	13.15%	1.715%
3	2.060	306	317	329	rBV	73215	107734	27.17%	3.543%
4	2.175	347	353	367	rVB4	6186	12111	3.05%	0.398%
5	3.812	848	862	891	rBV2	39426	144994	36.56%	4.769%
6	4.256	982	1000	1024	rBV2	53007	153412	38.69%	5.046%
7	4.960	1204	1219	1240	rBV3	127518	326718	82.39%	10.746%
8	5.539	1385	1399	1415	rBV2	109183	232339	58.59%	7.642%
9	5.992	1524	1540	1574	rBV	78447	181699	45.82%	5.976%
10	6.918	1818	1828	1844	rBV2	33191	68273	17.22%	2.246%
11	7.249	1920	1931	1952	rBV	130445	254507	64.18%	8.371%
12	7.561	2018	2028	2047	rBV	19782	41559	10.48%	1.367%
13	7.879	2115	2127	2135	rBV2	8318	14649	3.69%	0.482%
14	8.030	2163	2174	2206	rBV	186176	396558	100.00%	13.043%
15	8.789	2398	2410	2431	rBV	177766	319038	80.45%	10.493%
16	10.156	2824	2835	2851	rBV	62795	103337	26.06%	3.399%
17	10.326	2878	2888	2902	rVB3	18247	31715	8.00%	1.043%
18	11.188	3143	3156	3177	rBV	188117	300602	75.80%	9.887%
19	11.503	3243	3254	3260	rBV6	2928	5502	1.39%	0.181%
20	11.564	3263	3273	3289	rVV	144298	229604	57.90%	7.552%
21	12.197	3455	3470	3479	rBV	6574	10921	2.75%	0.359%




Sum of corrected areas: 3040385

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102023\
Data File : VV032514.D
Acq On : 20 Oct 2023 11:04
Operator : SY/MD
Sample : 04950-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4A02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

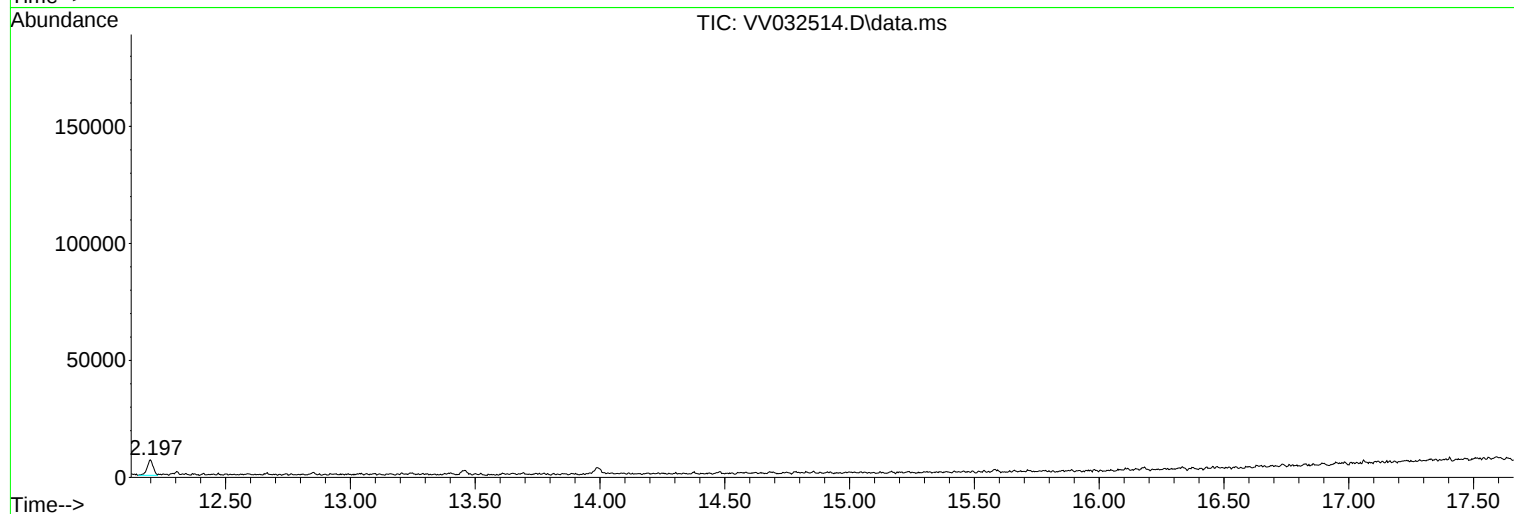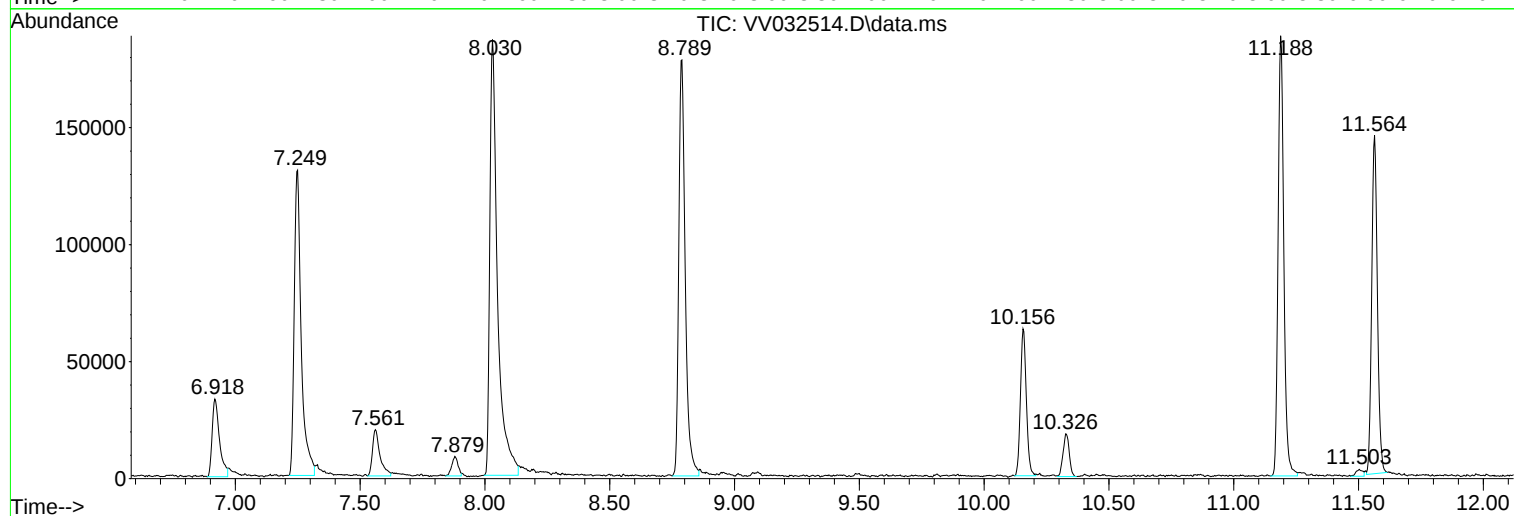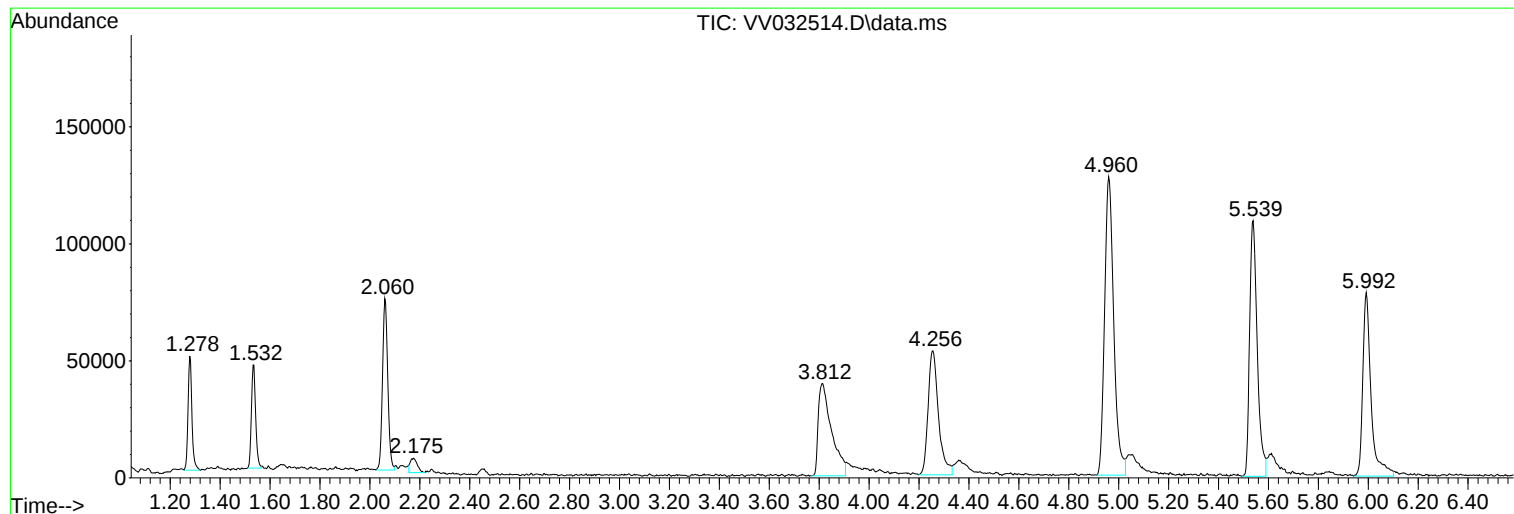

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102023\
Data File : VV032514.D
Acq On : 20 Oct 2023 11:04
Operator : SY/MD
Sample : 04950-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4A02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102023\
Data File : VV032514.D
Acq On : 20 Oct 2023 11:04
Operator : SY/MD
Sample : 04950-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4A02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc