

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102023\
 Data File : VV032519.D
 Acq On : 20 Oct 2023 13:05
 Operator : SY/MD
 Sample : 04950-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A49D1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032519.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.111	19	22	29	rVB	4967	6112	1.19%	0.167%
2	1.278	67	74	87	rVV	59669	64875	12.59%	1.777%
3	1.532	145	153	163	rBV	56809	67170	13.03%	1.840%
4	2.059	307	317	331	rBV	88550	130150	25.25%	3.565%
5	2.178	344	354	364	rVB	9441	18965	3.68%	0.519%
6	3.799	847	858	889	rBV	61820	197048	38.23%	5.397%
7	4.252	982	999	1019	rBV2	63974	171772	33.33%	4.705%
8	4.365	1021	1034	1056	rVB3	9328	30425	5.90%	0.833%
9	4.960	1202	1219	1236	rBV2	157023	399858	77.58%	10.951%
10	5.535	1386	1398	1415	rBV	104619	226712	43.98%	6.209%
11	5.847	1488	1495	1505	rVB10	3009	5926	1.15%	0.162%
12	5.992	1527	1540	1555	rBV	95738	205345	39.84%	5.624%
13	6.918	1818	1828	1854	rBV2	42042	89418	17.35%	2.449%
14	7.246	1919	1930	1949	rBV	164066	325258	63.10%	8.908%
15	7.326	1950	1955	1974	rVB2	13923	27753	5.38%	0.760%
16	7.561	2016	2028	2049	rBV	26120	55965	10.86%	1.533%
17	7.879	2115	2127	2139	rBV7	3742	10053	1.95%	0.275%
18	8.027	2163	2173	2206	rBV	244027	515441	100.00%	14.117%
19	8.789	2399	2410	2435	rBV	177085	319383	61.96%	8.747%
20	8.956	2451	2462	2471	rBV5	3862	6774	1.31%	0.186%
21	9.079	2493	2500	2515	rVB3	11408	20361	3.95%	0.558%
22	9.487	2618	2627	2637	rBV3	5352	9160	1.78%	0.251%
23	10.156	2824	2835	2853	rBV	82004	133454	25.89%	3.655%
24	10.326	2881	2888	2897	rVB3	5658	8674	1.68%	0.238%
25	10.863	3044	3055	3066	rBV4	5380	9300	1.80%	0.255%
26	11.188	3146	3156	3176	rBV	185139	295411	57.31%	8.091%
27	11.496	3236	3252	3254	rBV9	3880	5691	1.10%	0.156%
28	11.564	3262	3273	3290	rVB	182985	294744	57.18%	8.073%




Sum of corrected areas: 3651198

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102023\
Data File : VV032519.D
Acq On : 20 Oct 2023 13:05
Operator : SY/MD
Sample : 04950-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49D1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

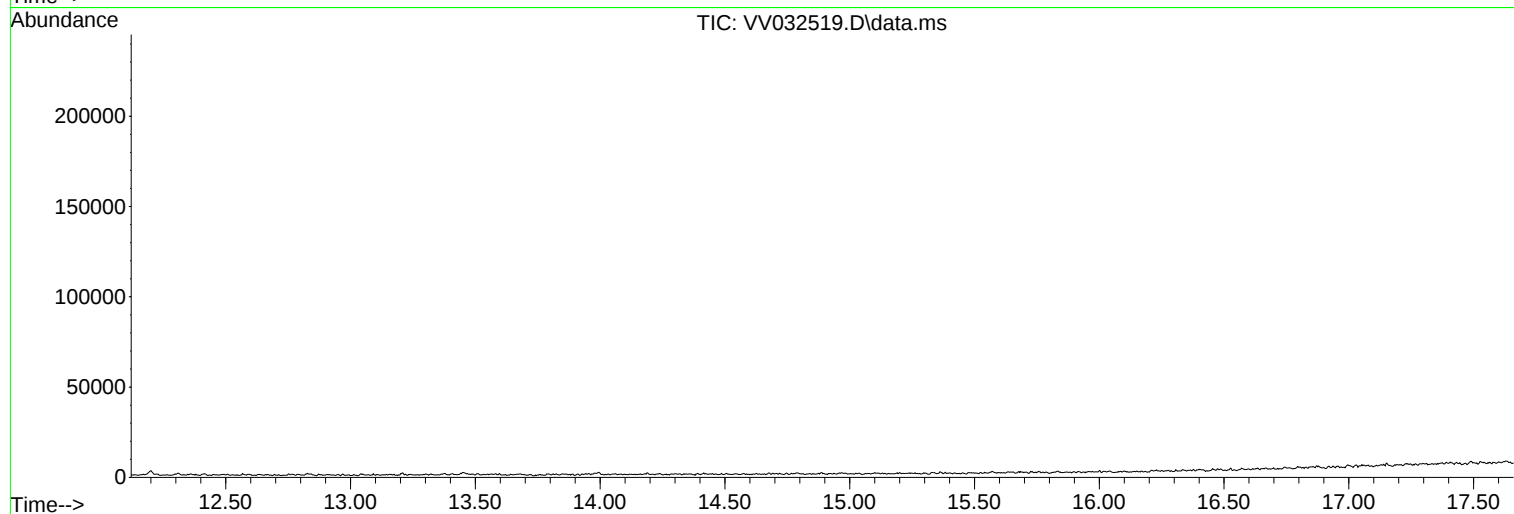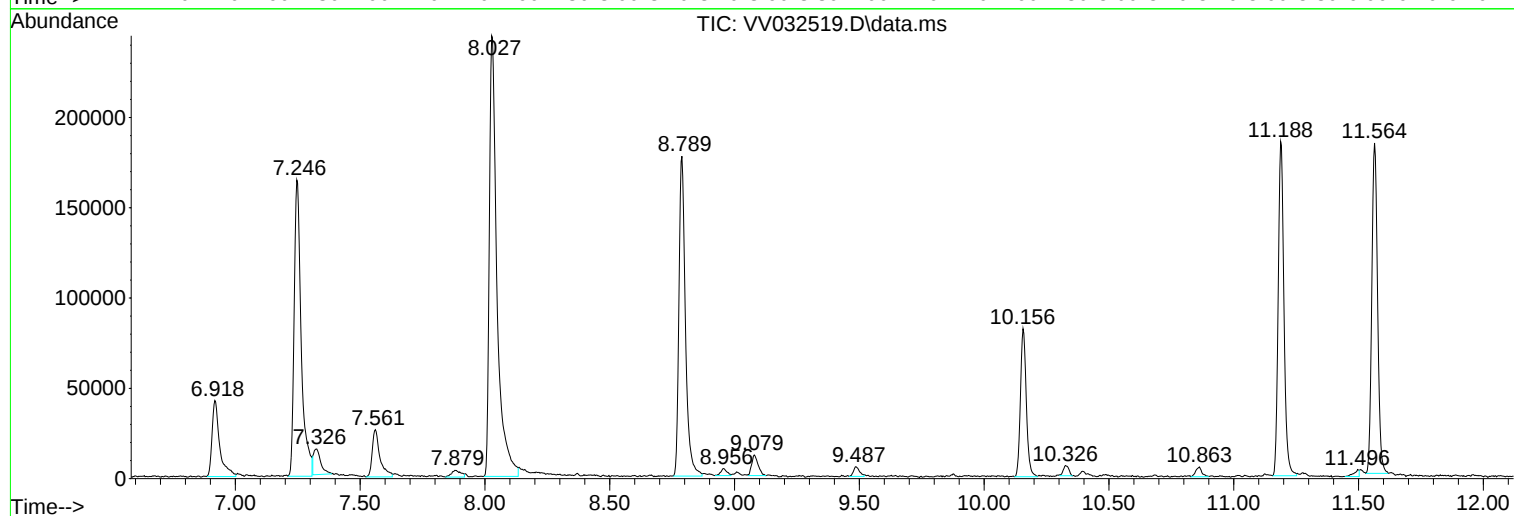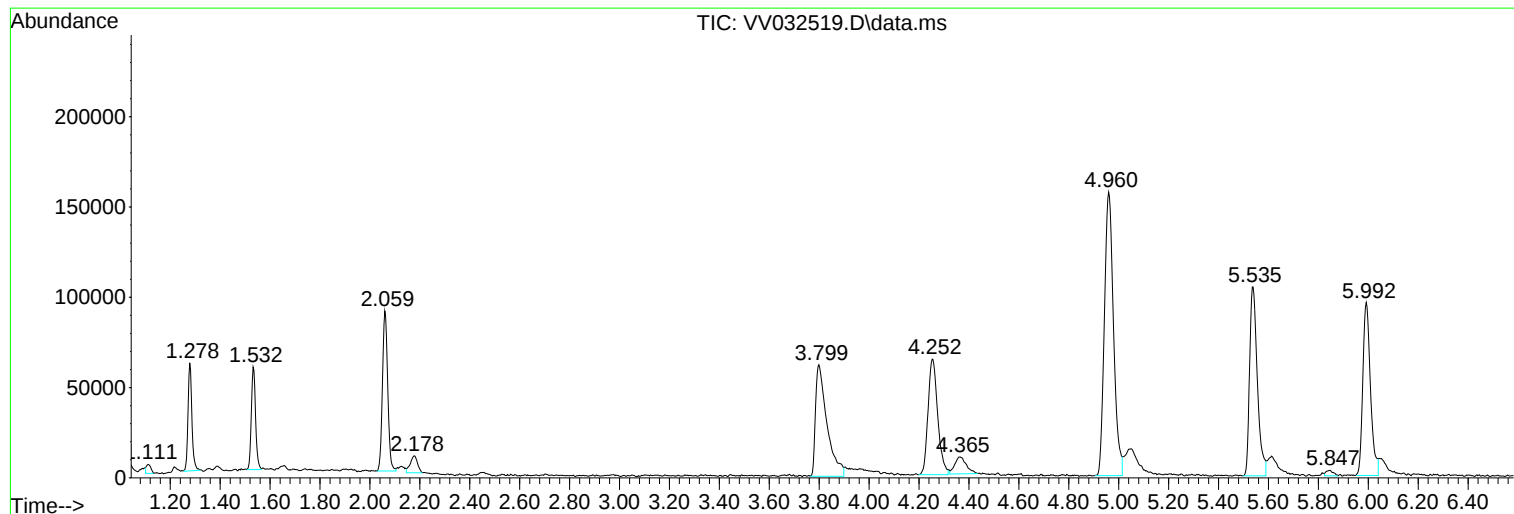

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102023\
Data File : VV032519.D
Acq On : 20 Oct 2023 13:05
Operator : SY/MD
Sample : 04950-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49D1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102023\
Data File : VV032519.D
Acq On : 20 Oct 2023 13:05
Operator : SY/MD
Sample : 04950-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49D1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
