

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102023\
 Data File : VV032521.D
 Acq On : 20 Oct 2023 13:53
 Operator : SY/MD
 Sample : 04950-11
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A49D3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV032521.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.114	17	23	36	rVB2	5313	9276	2.16%	0.302%
2	1.217	46	55	64	rBV	8845	12277	2.86%	0.399%
3	1.278	67	74	86	rVV	48534	52931	12.32%	1.722%
4	1.532	146	153	166	rBV	46383	56500	13.16%	1.838%
5	2.060	307	317	331	rBV	73674	109725	25.55%	3.570%
6	2.182	347	355	367	rVB2	8071	15020	3.50%	0.489%
7	3.802	850	859	899	rBV	47108	160854	37.45%	5.233%
8	4.256	984	1000	1022	rBV	54087	142930	33.28%	4.650%
9	4.960	1205	1219	1238	rBV2	129924	332329	77.38%	10.811%
10	5.539	1388	1399	1415	rBV	101091	216461	50.40%	7.042%
11	5.992	1525	1540	1554	rBV	81224	169156	39.39%	5.503%
12	6.918	1816	1828	1851	rBV	34524	75889	17.67%	2.469%
13	7.246	1919	1930	1950	rBV	135861	268276	62.47%	8.727%
14	7.561	2017	2028	2048	rBV2	22094	45730	10.65%	1.488%
15	8.030	2163	2174	2211	rBV	199552	429482	100.00%	13.972%
16	8.789	2396	2410	2436	rBV	170716	312151	72.68%	10.155%
17	9.082	2491	2501	2514	rVB7	5442	10735	2.50%	0.349%
18	9.493	2616	2629	2636	rBV9	3334	5524	1.29%	0.180%
19	10.156	2822	2835	2854	rBV	66961	109983	25.61%	3.578%
20	10.329	2878	2889	2897	rBV3	4582	7864	1.83%	0.256%
21	11.188	3145	3156	3176	rBV	181681	286802	66.78%	9.330%
22	11.564	3260	3273	3289	rVV	153224	244027	56.82%	7.939%




Sum of corrected areas: 3073922

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102023\
Data File : VV032521.D
Acq On : 20 Oct 2023 13:53
Operator : SY/MD
Sample : 04950-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49D3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

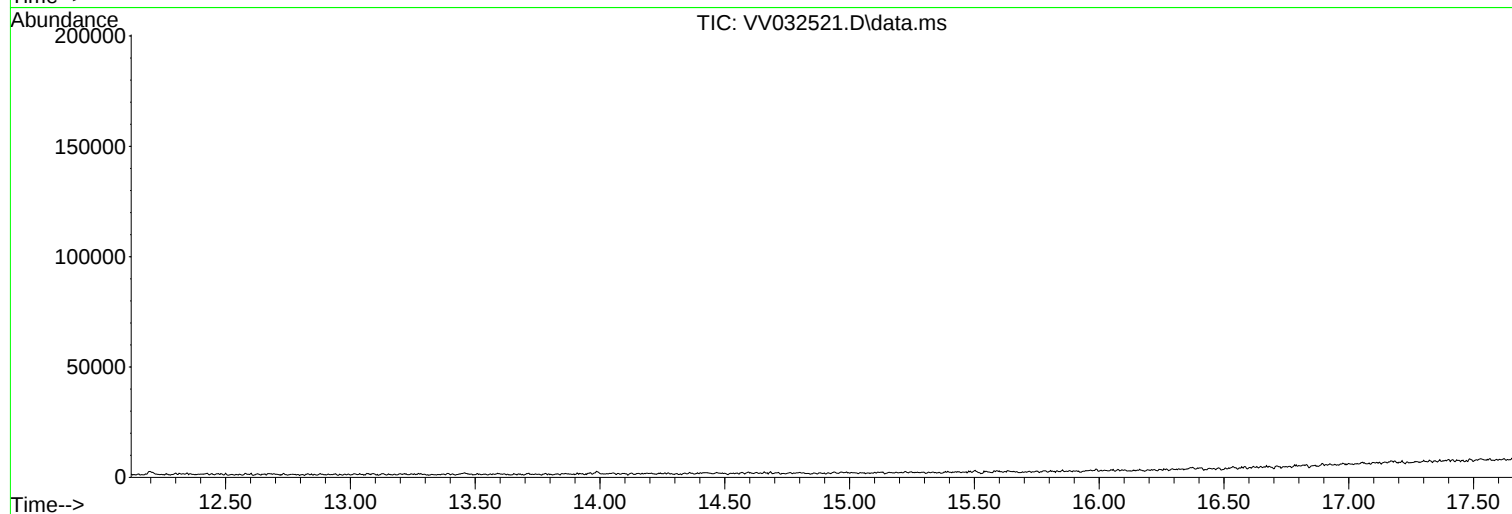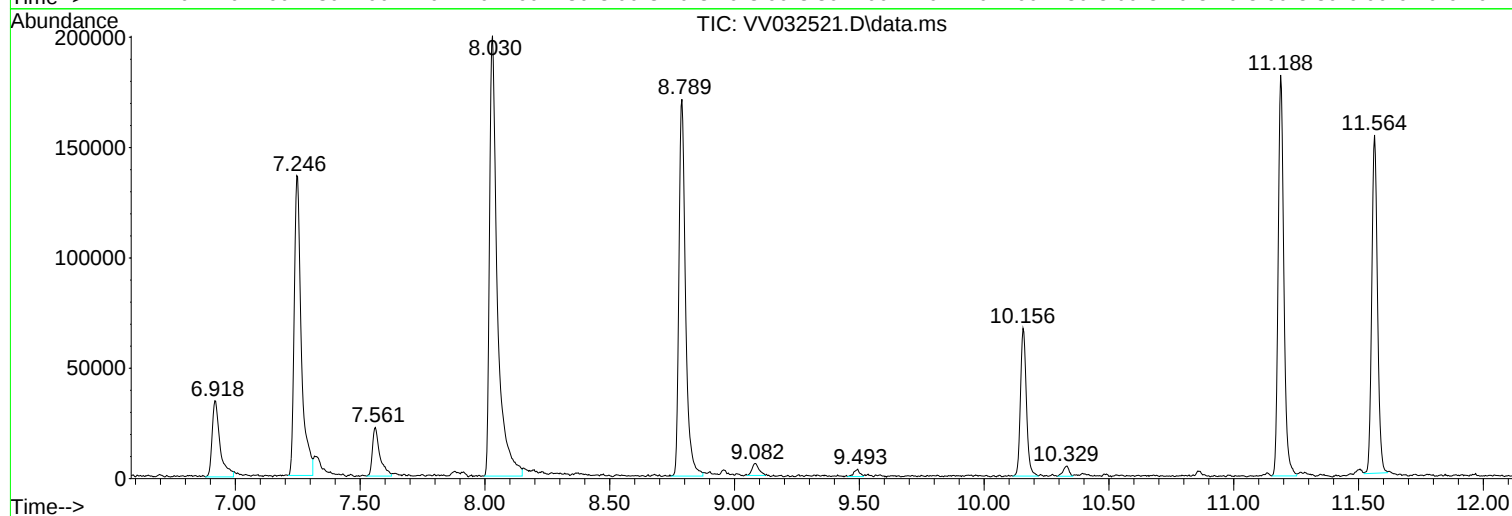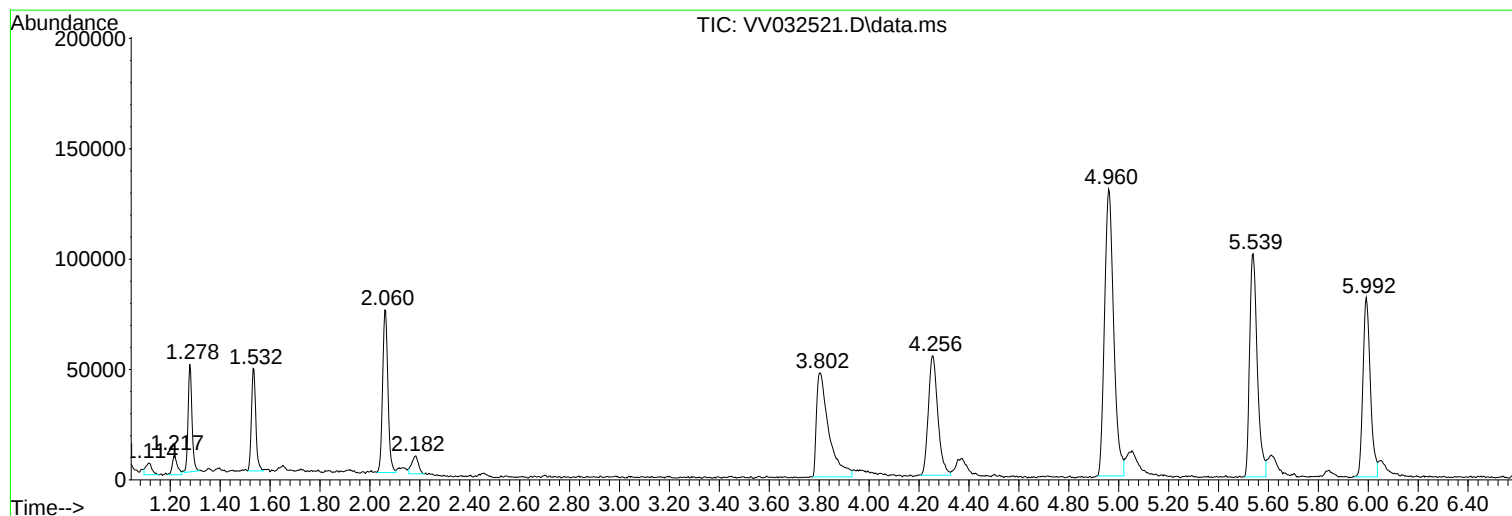

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102023\
Data File : VV032521.D
Acq On : 20 Oct 2023 13:53
Operator : SY/MD
Sample : 04950-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49D3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102023\
Data File : VV032521.D
Acq On : 20 Oct 2023 13:53
Operator : SY/MD
Sample : 04950-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49D3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------