

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102023\
 Data File : VV032523.D
 Acq On : 20 Oct 2023 14:42
 Operator : SY/MD
 Sample : 04950-13
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A49D7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032523.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.118	17	24	33	rVB2	5006	8265	2.09%	0.274%
2	1.217	50	55	62	rBV	7516	9146	2.32%	0.303%
3	1.278	67	74	85	rVB	46966	50468	12.79%	1.671%
4	1.394	104	110	117	rVB8	2731	4054	1.03%	0.134%
5	1.536	146	154	167	rVB	45471	55276	14.00%	1.830%
6	2.063	308	318	329	rBV	68340	101481	25.71%	3.359%
7	2.182	347	355	368	rVB4	8263	15895	4.03%	0.526%
8	3.802	847	859	894	rBV	45470	155725	39.45%	5.155%
9	4.256	982	1000	1025	rBV2	50062	138119	34.99%	4.572%
10	4.371	1025	1036	1050	rVB4	6869	18654	4.73%	0.618%
11	4.960	1203	1219	1238	rBV3	121116	315411	79.91%	10.441%
12	5.539	1385	1399	1414	rBV	106512	224312	56.83%	7.426%
13	5.838	1483	1492	1503	rBV	2979	6513	1.65%	0.216%
14	5.992	1528	1540	1555	rBV	75767	161954	41.03%	5.361%
15	6.918	1819	1828	1854	rBV2	32570	67216	17.03%	2.225%
16	7.249	1918	1931	1953	rBV	125323	251249	63.65%	8.317%
17	7.561	2016	2028	2050	rBV2	19992	43917	11.13%	1.454%
18	8.030	2165	2174	2206	rBV	184532	394709	100.00%	13.067%
19	8.789	2398	2410	2432	rBV	182958	323344	81.92%	10.704%
20	9.082	2493	2501	2514	rBV10	4469	7618	1.93%	0.252%
21	9.490	2621	2628	2637	rBV7	2533	4564	1.16%	0.151%
22	10.156	2823	2835	2851	rBV	62754	103402	26.20%	3.423%
23	10.326	2882	2888	2900	rVB4	4580	6862	1.74%	0.227%
24	11.188	3146	3156	3178	rBV	184514	296063	75.01%	9.801%
25	11.493	3240	3251	3262	rBV4	9361	21530	5.45%	0.713%
26	11.564	3263	3273	3292	rVB	146619	235017	59.54%	7.780%




Sum of corrected areas: 3020764

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102023\
Data File : VV032523.D
Acq On : 20 Oct 2023 14:42
Operator : SY/MD
Sample : 04950-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49D7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

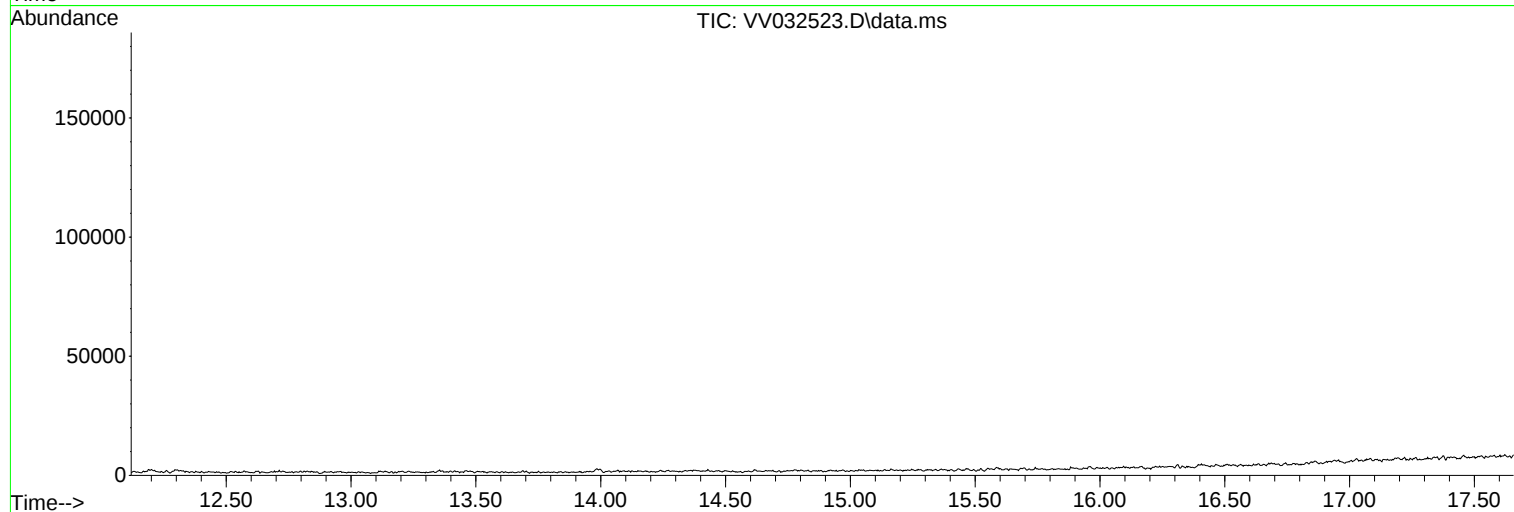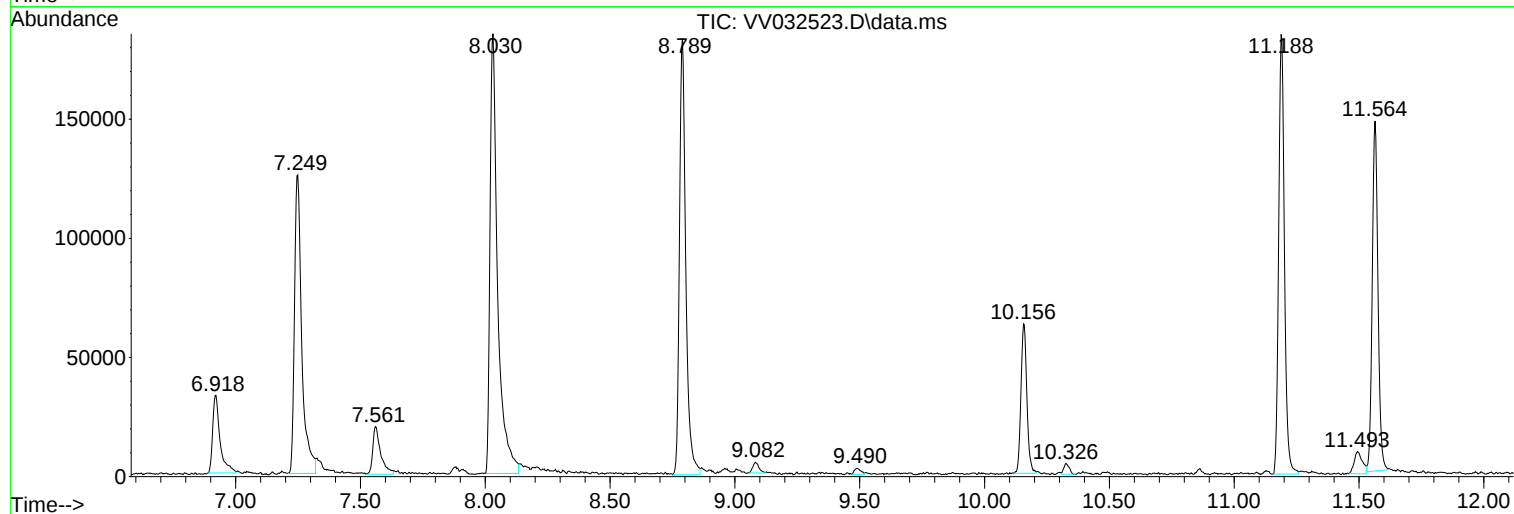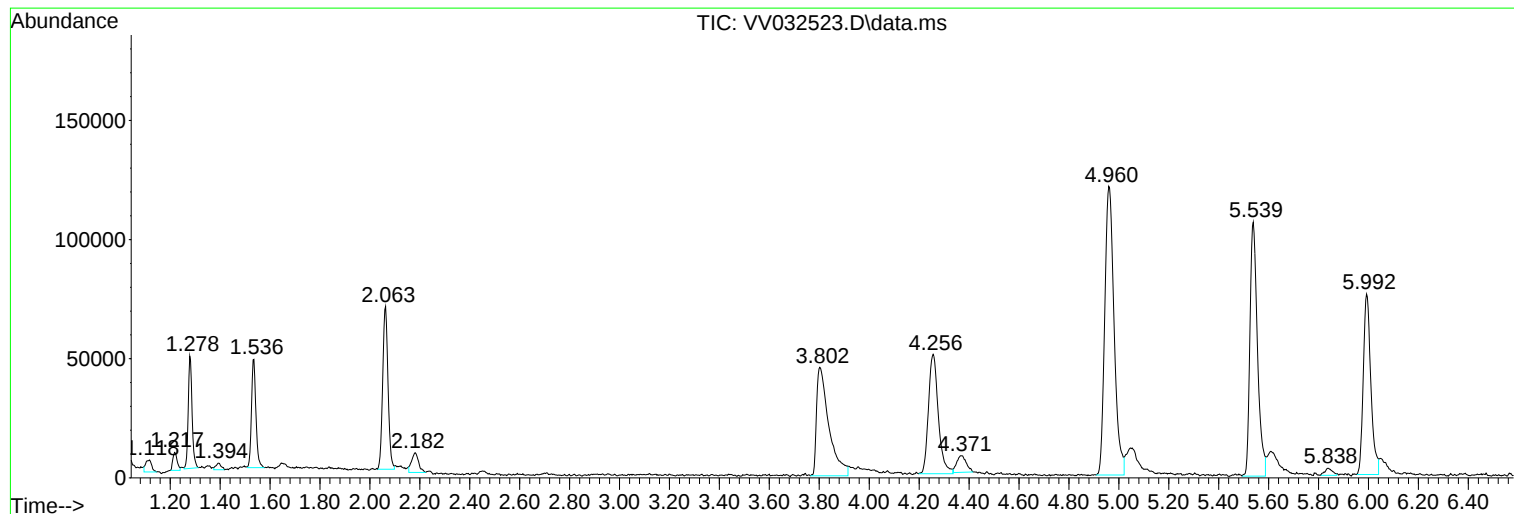

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102023\
Data File : VV032523.D
Acq On : 20 Oct 2023 14:42
Operator : SY/MD
Sample : 04950-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49D7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102023\
Data File : VV032523.D
Acq On : 20 Oct 2023 14:42
Operator : SY/MD
Sample : 04950-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49D7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc