

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102023\
 Data File : VV032527.D
 Acq On : 20 Oct 2023 16:39
 Operator : SY/MD
 Sample : 04994-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B05

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032527.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.085	10	14	17	rBV2	7213	6454	1.51%	0.206%
2	1.278	64	74	86	rBV	51711	58720	13.78%	1.871%
3	1.388	103	108	115	rVB3	4337	5021	1.18%	0.160%
4	1.535	146	154	164	rVB	44245	51866	12.17%	1.653%
5	2.059	307	317	328	rBV	69557	103895	24.37%	3.311%
6	2.175	345	353	365	rVB2	6659	13705	3.22%	0.437%
7	3.815	852	863	902	rBV2	42941	178712	41.93%	5.696%
8	4.252	984	999	1019	rBV2	50707	136674	32.06%	4.356%
9	4.368	1025	1035	1049	rVB3	5215	13222	3.10%	0.421%
10	4.960	1202	1219	1237	rBV3	122247	316667	74.29%	10.093%
11	5.538	1387	1399	1415	rBV	105535	224617	52.70%	7.159%
12	5.992	1527	1540	1556	rBV	74780	161001	37.77%	5.131%
13	6.918	1816	1828	1853	rBV	32853	70141	16.46%	2.235%
14	7.246	1920	1930	1955	rBV	126973	247896	58.16%	7.901%
15	7.561	2017	2028	2045	rBV	20691	42537	9.98%	1.356%
16	7.879	2115	2127	2131	rBV2	11678	20305	4.76%	0.647%
17	7.908	2131	2136	2153	rVB4	15627	29899	7.01%	0.953%
18	8.030	2163	2174	2213	rBV	195413	426253	100.00%	13.585%
19	8.789	2399	2410	2435	rBV	175256	313236	73.49%	9.983%
20	10.156	2823	2835	2847	rBV	64002	105112	24.66%	3.350%
21	10.329	2880	2889	2900	rVB2	20905	32781	7.69%	1.045%
22	11.188	3146	3156	3178	rBV	185492	295392	69.30%	9.415%
23	11.564	3261	3273	3295	rBV	141825	235587	55.27%	7.508%
24	12.197	3460	3470	3481	rVB2	7237	12253	2.87%	0.391%
25	12.593	3582	3593	3601	rBV9	3318	5192	1.22%	0.165%
26	13.207	3776	3784	3796	rBV5	5246	7448	1.75%	0.237%
27	13.445	3850	3858	3871	rBV3	7663	13127	3.08%	0.418%
28	13.686	3925	3933	3944	rBV10	6240	9913	2.33%	0.316%




Sum of corrected areas: 3137626

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102023\
Data File : VV032527.D
Acq On : 20 Oct 2023 16:39
Operator : SY/MD
Sample : 04994-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B05

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

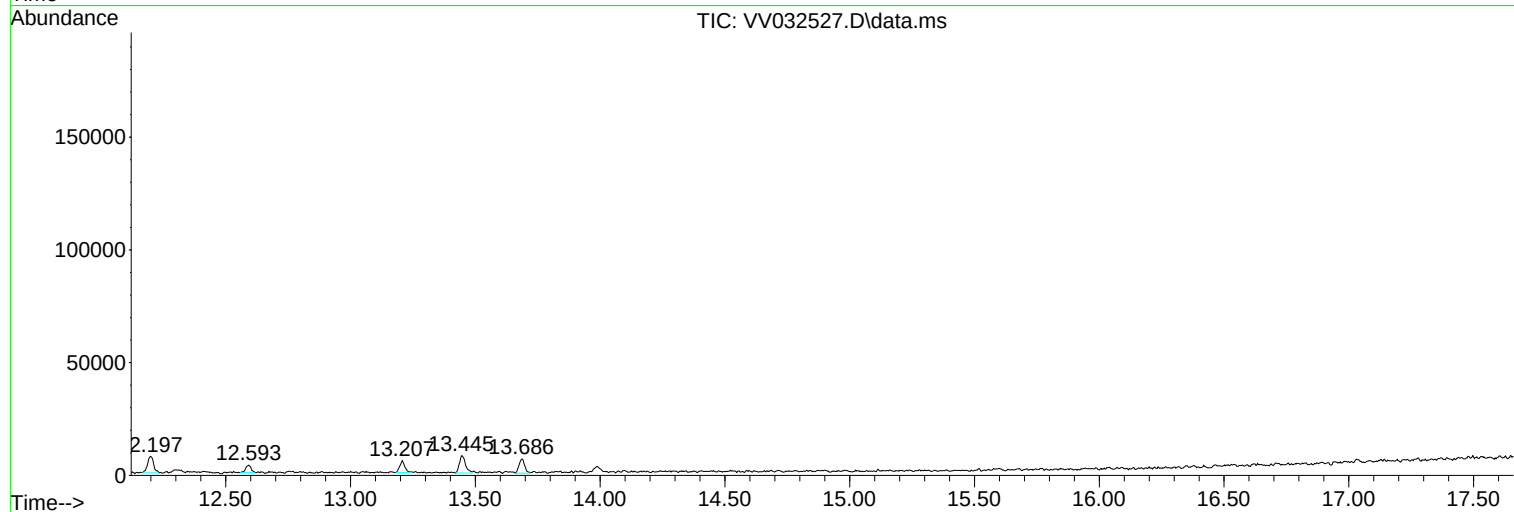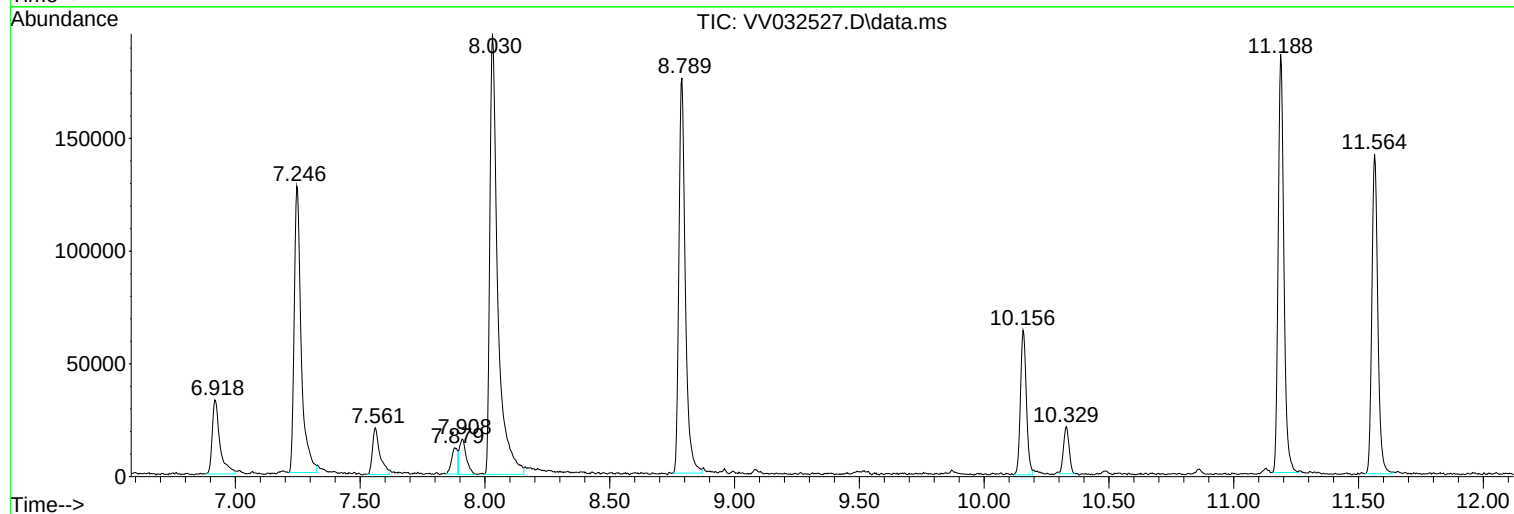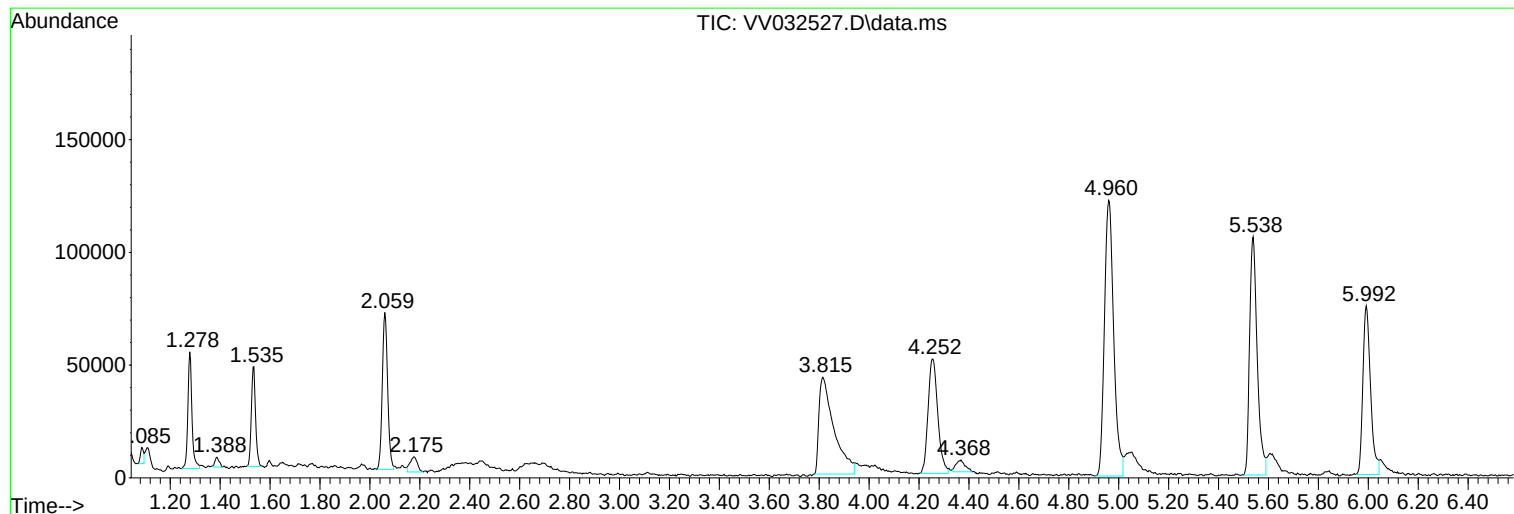

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102023\
Data File : VV032527.D
Acq On : 20 Oct 2023 16:39
Operator : SY/MD
Sample : 04994-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B05

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102023\
Data File : VV032527.D
Acq On : 20 Oct 2023 16:39
Operator : SY/MD
Sample : 04994-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B05

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc