

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102023\
 Data File : VV032534.D
 Acq On : 20 Oct 2023 19:30
 Operator : SY/MD
 Sample : 04994-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B35

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV032534.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	64	74	92	rBV	43187	50783	11.35%	1.518%
2	1.359	92	99	105	rBV	4602	6980	1.56%	0.209%
3	1.532	146	153	167	rBV	40885	48294	10.80%	1.444%
4	2.060	307	317	332	rBV	67504	100271	22.42%	2.998%
5	2.452	433	439	446	rVB5	3386	5223	1.17%	0.156%
6	3.822	849	865	886	rBV3	45520	178957	40.01%	5.351%
7	4.275	983	1006	1027	rBV4	137648	447234	100.00%	13.373%
8	4.960	1204	1219	1237	rBV3	115758	296614	66.32%	8.869%
9	5.535	1387	1398	1416	rBV	99489	213797	47.80%	6.393%
10	5.992	1524	1540	1556	rBV	73298	157716	35.26%	4.716%
11	6.439	1664	1679	1695	rBV2	37453	79430	17.76%	2.375%
12	6.918	1816	1828	1842	rBV2	29472	60288	13.48%	1.803%
13	7.246	1920	1930	1950	rBV	116372	228065	50.99%	6.819%
14	7.561	2020	2028	2049	rBV	18075	36892	8.25%	1.103%
15	7.879	2112	2127	2143	rBV	13411	27065	6.05%	0.809%
16	8.031	2164	2174	2209	rBV	184829	408002	91.23%	12.200%
17	8.185	2212	2222	2238	rVB3	9635	22639	5.06%	0.677%
18	8.789	2398	2410	2433	rBV	164976	299349	66.93%	8.951%
19	10.156	2823	2835	2851	rBV	61604	100911	22.56%	3.017%
20	10.326	2876	2888	2903	rVB3	26600	44454	9.94%	1.329%
21	11.188	3145	3156	3178	rBV	173201	280111	62.63%	8.376%
22	11.564	3259	3273	3290	rBV	134820	222360	49.72%	6.649%
23	12.194	3460	3469	3480	rVB2	8023	13619	3.05%	0.407%
24	12.291	3491	3499	3510	rBV9	8342	15311	3.42%	0.458%




Sum of corrected areas: 3344365

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102023\
Data File : VV032534.D
Acq On : 20 Oct 2023 19:30
Operator : SY/MD
Sample : 04994-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B35

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

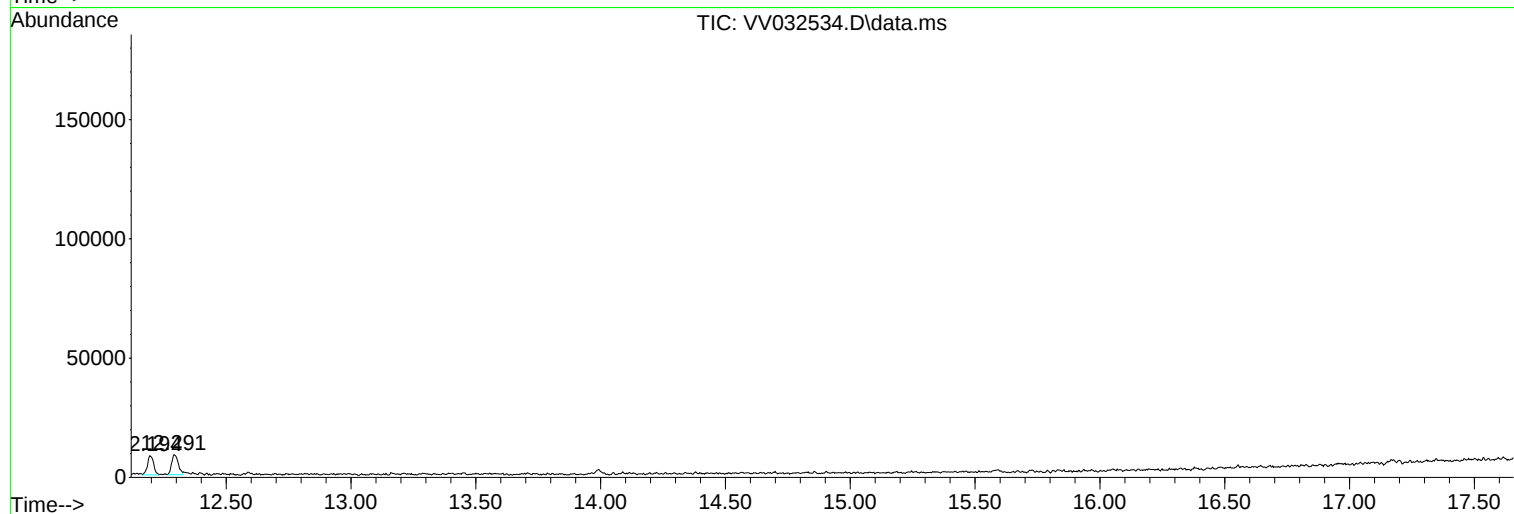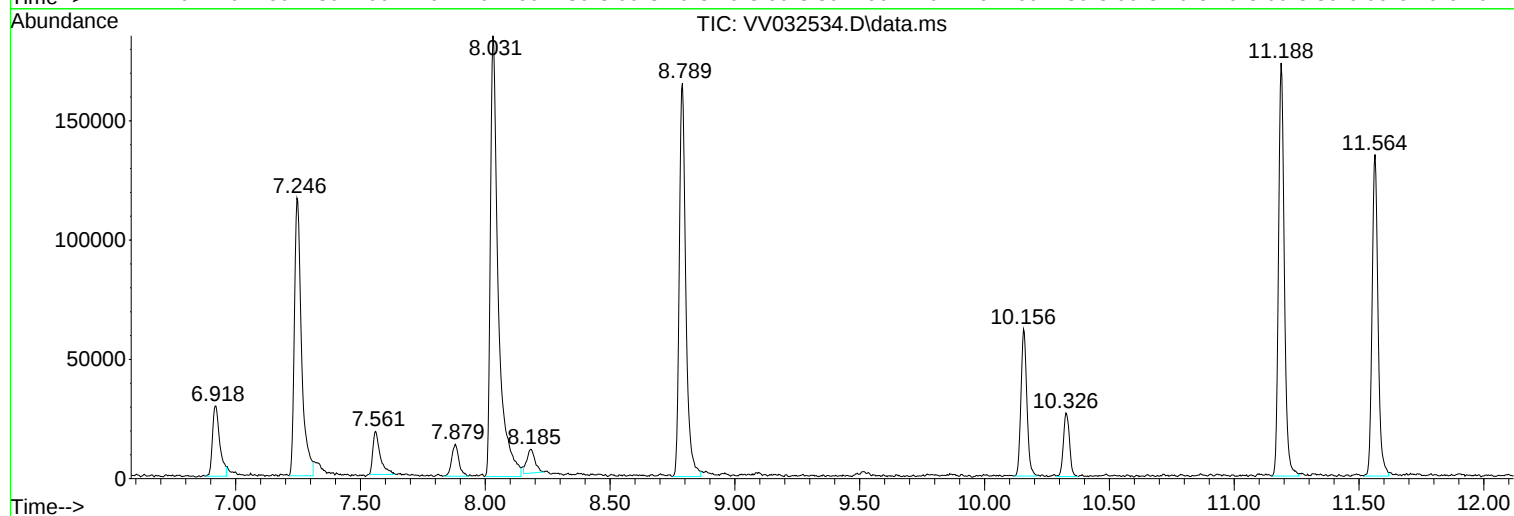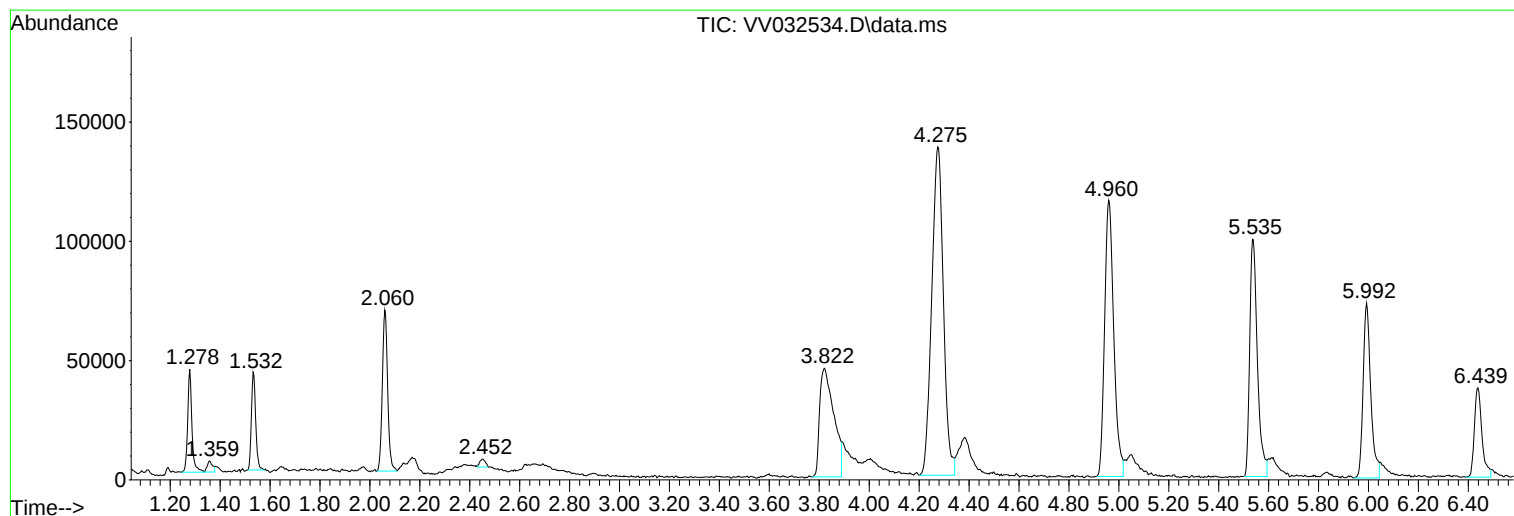

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102023\
Data File : VV032534.D
Acq On : 20 Oct 2023 19:30
Operator : SY/MD
Sample : 04994-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B35

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102023\
Data File : VV032534.D
Acq On : 20 Oct 2023 19:30
Operator : SY/MD
Sample : 04994-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B35

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc