

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102023\
 Data File : VV032536.D
 Acq On : 20 Oct 2023 20:40
 Operator : SY/MD
 Sample : VV1020WBL02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK375

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV032536.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.108	16	21	31	rVB	4980	7355	1.87%	0.265%
2	1.278	67	74	86	rBV	47084	51580	13.14%	1.860%
3	1.532	146	153	164	rBV	43826	51148	13.03%	1.844%
4	2.059	307	317	329	rBV	71737	103935	26.48%	3.747%
5	2.172	346	352	368	rVB3	8043	14824	3.78%	0.534%
6	2.449	429	438	449	rBV6	3370	6449	1.64%	0.233%
7	3.825	855	866	903	rBV2	27223	132790	33.83%	4.788%
8	4.252	983	999	1021	rBV3	49851	134068	34.16%	4.834%
9	4.362	1023	1033	1056	rVB4	5656	17436	4.44%	0.629%
10	4.960	1202	1219	1237	rBV3	120793	310508	79.11%	11.195%
11	5.538	1383	1399	1414	rBV	92950	196123	49.97%	7.071%
12	5.992	1527	1540	1556	rBV	71239	157346	40.09%	5.673%
13	6.921	1819	1829	1844	rBV2	29748	60587	15.44%	2.184%
14	7.246	1919	1930	1954	rBV	124129	243663	62.08%	8.785%
15	7.561	2018	2028	2042	rBV2	18658	37808	9.63%	1.363%
16	8.034	2165	2175	2205	rBV	173473	392488	100.00%	14.151%
17	8.789	2398	2410	2432	rBV	155397	282830	72.06%	10.198%
18	10.156	2825	2835	2853	rBV	61311	101385	25.83%	3.655%
19	11.188	3144	3156	3178	rBV	154579	253573	64.61%	9.143%
20	11.564	3259	3273	3287	rBV	137123	217614	55.44%	7.846%




Sum of corrected areas: 2773510

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102023\
Data File : VV032536.D
Acq On : 20 Oct 2023 20:40
Operator : SY/MD
Sample : VV1020WBL02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK375

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

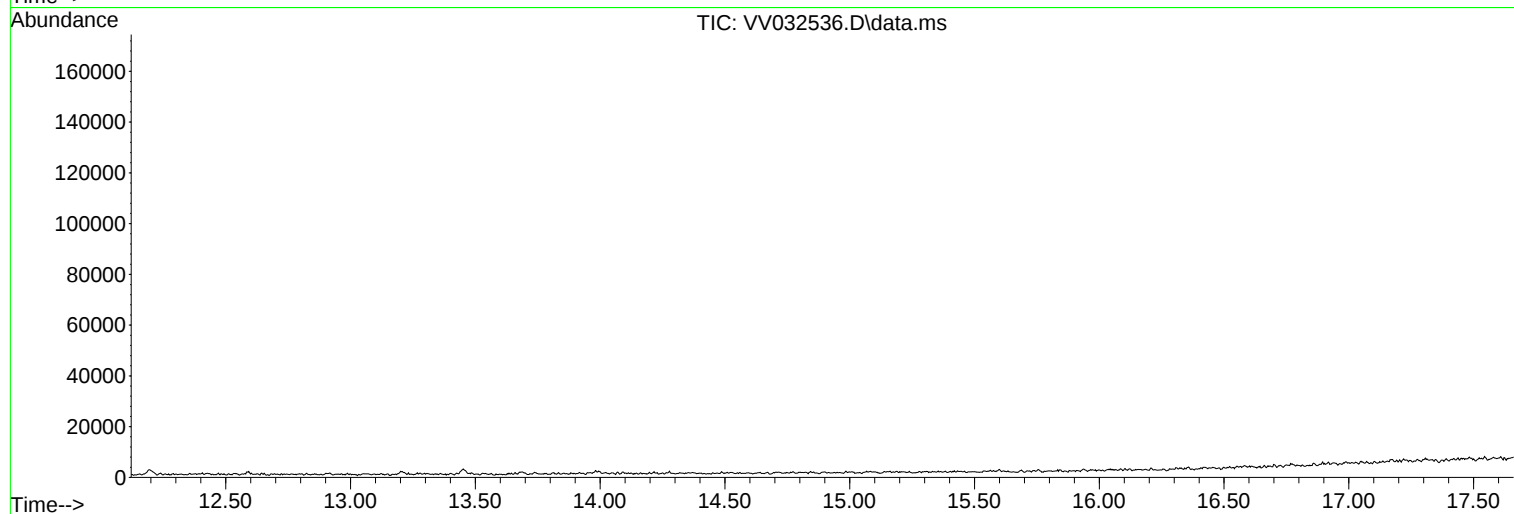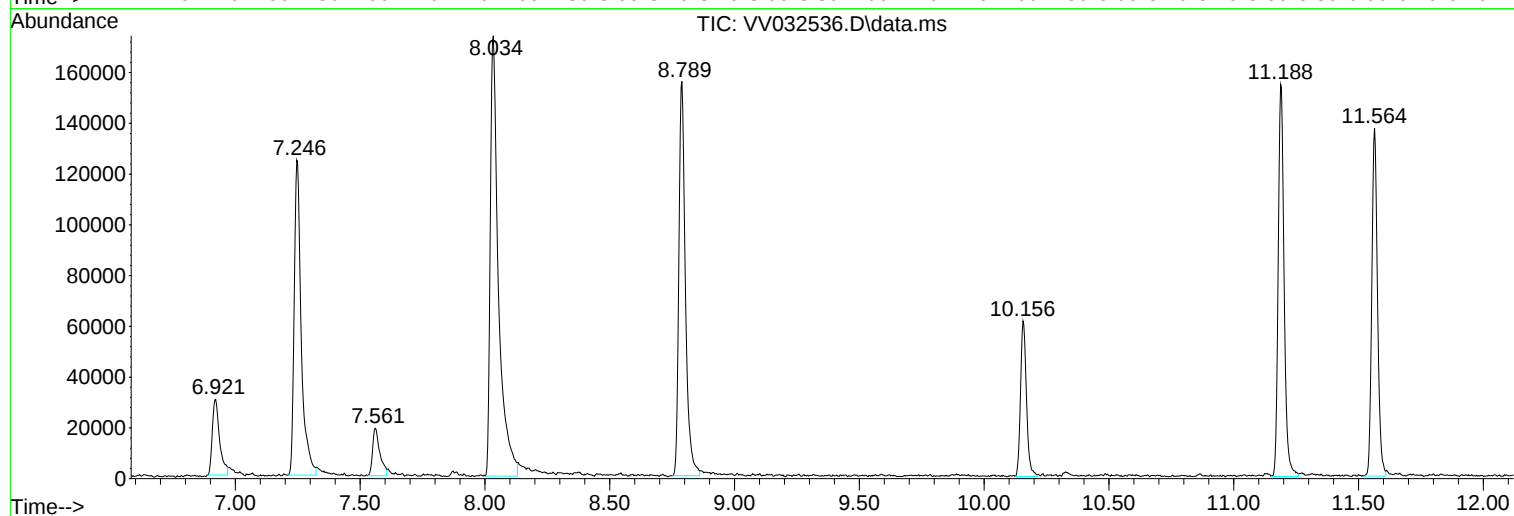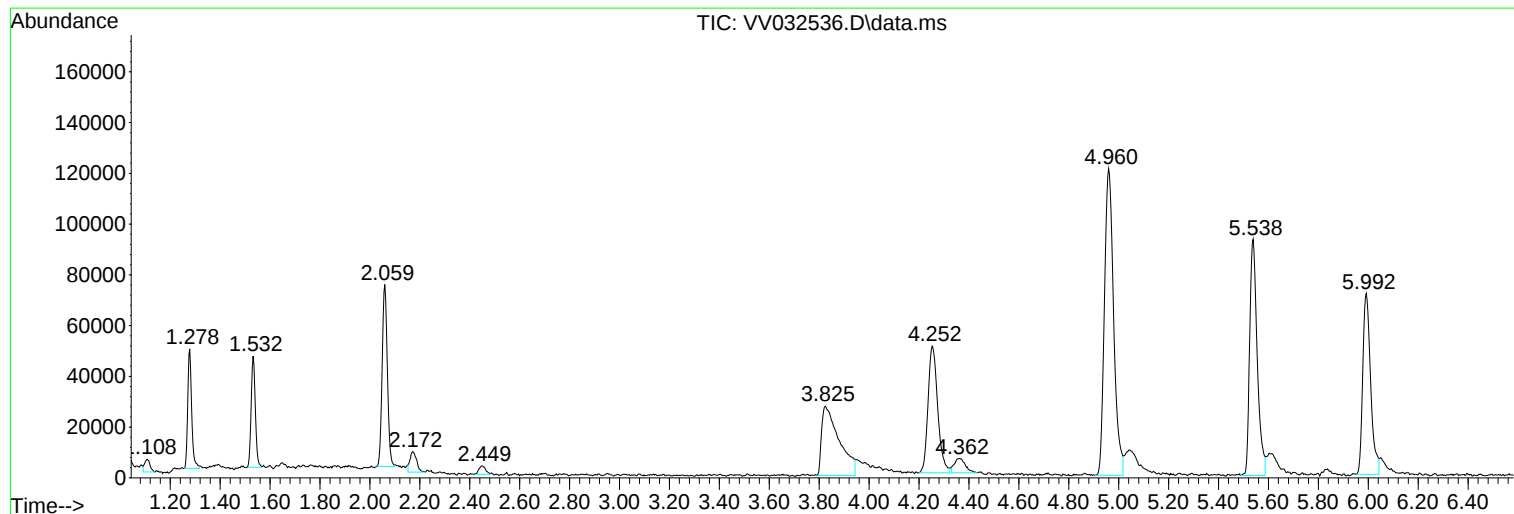

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102023\
Data File : VV032536.D
Acq On : 20 Oct 2023 20:40
Operator : SY/MD
Sample : VV1020WBL02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK375

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102023\
Data File : VV032536.D
Acq On : 20 Oct 2023 20:40
Operator : SY/MD
Sample : VV1020WBL02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK375

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------