

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102023\
 Data File : VV032538.D
 Acq On : 20 Oct 2023 21:29
 Operator : SY/MD
 Sample : 04950-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4955

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032538.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.105	11	20	29	rVB2	3889	7993	2.10%	0.282%
2	1.217	48	55	63	rBV	10211	12628	3.31%	0.445%
3	1.278	67	74	87	rVV	43125	47747	12.53%	1.683%
4	1.388	102	108	115	rVB4	4062	5469	1.44%	0.193%
5	1.532	146	153	166	rBV	41299	49679	13.04%	1.751%
6	2.060	307	317	331	rBV	64019	93378	24.51%	3.292%
7	2.169	347	351	366	rVB6	5902	10664	2.80%	0.376%
8	3.805	849	860	886	rBV2	45148	150266	39.44%	5.297%
9	4.256	982	1000	1020	rBV	50523	133782	35.11%	4.716%
10	4.960	1203	1219	1238	rBV4	112509	295732	77.62%	10.425%
11	5.539	1384	1399	1414	rBV	100347	210760	55.32%	7.430%
12	5.992	1528	1540	1555	rBV	70033	151010	39.63%	5.324%
13	6.918	1816	1828	1852	rBV2	29419	63788	16.74%	2.249%
14	7.246	1917	1930	1948	rBV	115078	224921	59.03%	7.929%
15	7.323	1949	1954	1968	rVB	11593	21294	5.59%	0.751%
16	7.561	2016	2028	2038	rBV	18570	34806	9.14%	1.227%
17	7.882	2119	2128	2133	rBV4	3891	6028	1.58%	0.213%
18	8.030	2164	2174	2203	rBV	179583	381004	100.00%	13.431%
19	8.789	2398	2410	2431	rBV	165401	295935	77.67%	10.433%
20	9.079	2492	2500	2515	rBV2	8375	16065	4.22%	0.566%
21	9.487	2618	2627	2633	rBV6	4442	6444	1.69%	0.227%
22	10.156	2825	2835	2851	rBV	59643	98215	25.78%	3.462%
23	10.329	2880	2889	2896	rVB6	5475	8994	2.36%	0.317%
24	10.853	3045	3052	3066	rBV7	2980	5491	1.44%	0.194%
25	11.188	3146	3156	3175	rBV	177175	278128	73.00%	9.805%
26	11.496	3241	3252	3262	rBV6	6502	14485	3.80%	0.511%
27	11.564	3263	3273	3286	rVB	132678	211954	55.63%	7.472%




Sum of corrected areas: 2836660

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102023\
Data File : VV032538.D
Acq On : 20 Oct 2023 21:29
Operator : SY/MD
Sample : 04950-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4955

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

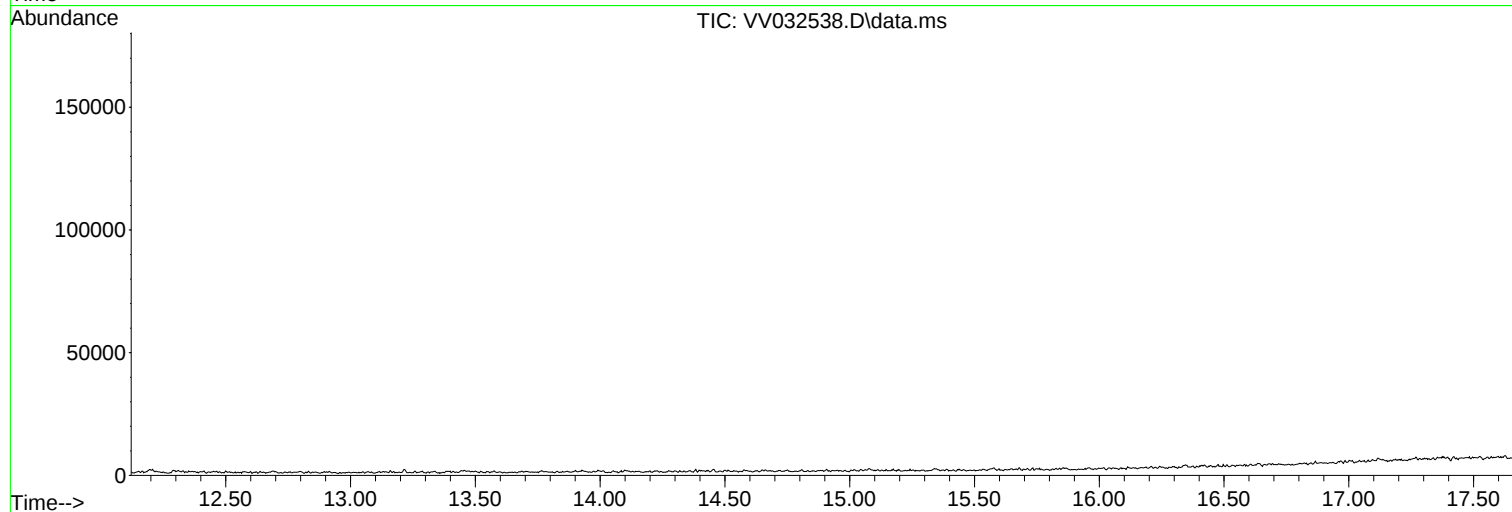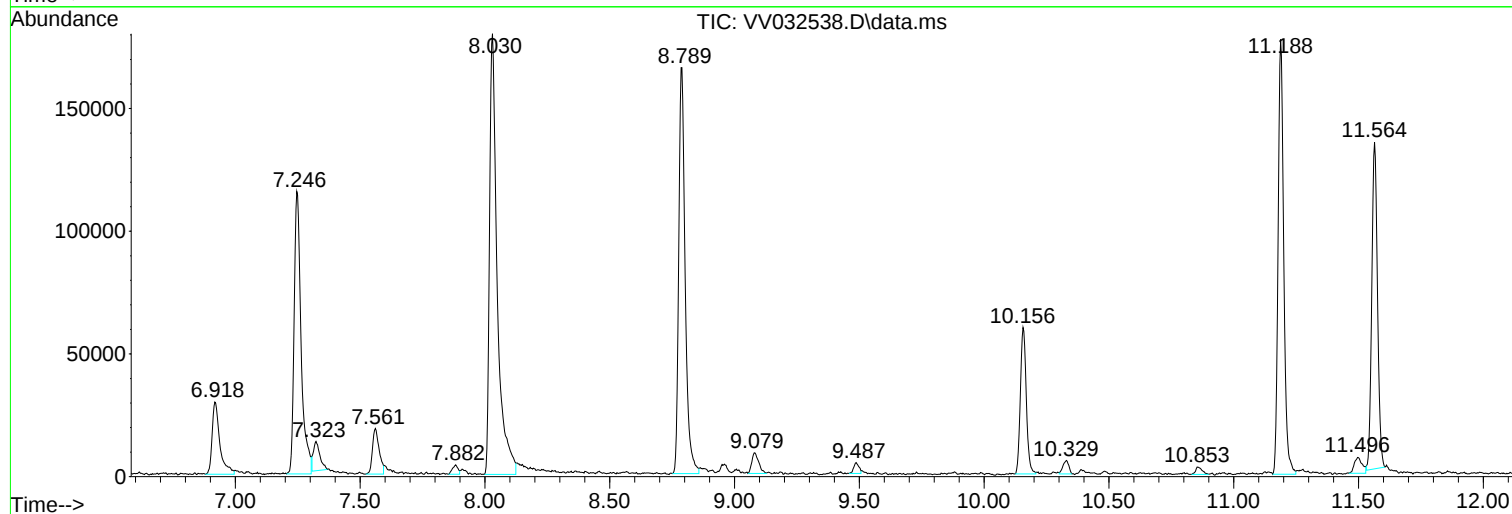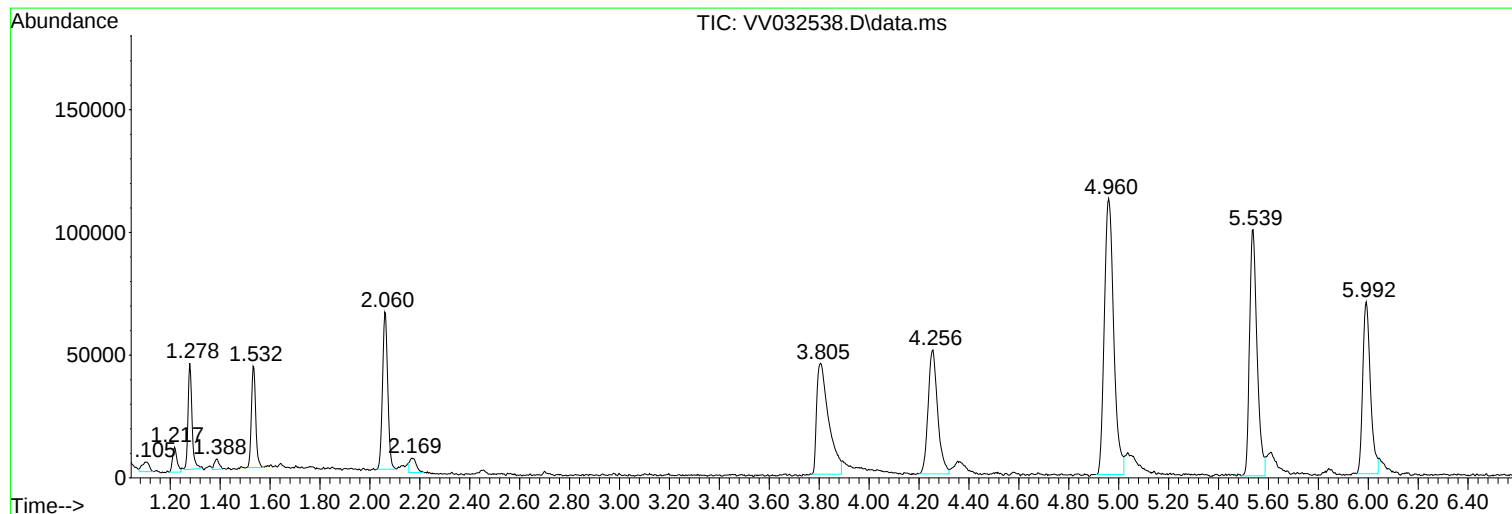

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102023\
Data File : VV032538.D
Acq On : 20 Oct 2023 21:29
Operator : SY/MD
Sample : 04950-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4955

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102023\
Data File : VV032538.D
Acq On : 20 Oct 2023 21:29
Operator : SY/MD
Sample : 04950-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4955

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc