

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102023\
 Data File : VV032540.D
 Acq On : 20 Oct 2023 22:17
 Operator : SY/MD
 Sample : 04950-16
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A49E8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032540.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.108	9	21	30	rVB2	4686	9962	2.66%	0.351%
2	1.217	41	55	61	rBV3	4438	7317	1.96%	0.258%
3	1.278	67	74	82	rBV	41778	44024	11.77%	1.551%
4	1.388	103	108	116	rVB2	4230	5612	1.50%	0.198%
5	1.532	146	153	163	rBV	40782	47356	12.66%	1.668%
6	2.060	307	317	328	rBV	60877	90683	24.24%	3.195%
7	3.809	848	861	892	rBV2	45837	161846	43.27%	5.702%
8	4.252	983	999	1023	rBV	48674	130088	34.78%	4.583%
9	4.362	1023	1033	1046	rVB3	4845	11878	3.18%	0.418%
10	4.960	1202	1219	1239	rBV4	108825	288091	77.02%	10.150%
11	5.538	1386	1399	1415	rBV	98382	209761	56.08%	7.390%
12	5.992	1524	1540	1554	rBV2	68311	145479	38.89%	5.125%
13	6.918	1818	1828	1855	rBV2	28803	64067	17.13%	2.257%
14	7.246	1920	1930	1947	rBV	107619	212152	56.72%	7.474%
15	7.323	1947	1954	1966	rVB2	13568	27145	7.26%	0.956%
16	7.561	2018	2028	2051	rBV2	17079	37304	9.97%	1.314%
17	8.030	2162	2174	2212	rBV	173896	374057	100.00%	13.178%
18	8.789	2399	2410	2429	rBV	167820	296168	79.18%	10.434%
19	8.956	2452	2462	2470	rBV5	4966	8340	2.23%	0.294%
20	9.079	2489	2500	2511	rBV2	11693	21966	5.87%	0.774%
21	9.484	2617	2626	2643	rVB7	5844	11202	2.99%	0.395%
22	10.156	2822	2835	2851	rBV2	59950	99388	26.57%	3.501%
23	10.332	2882	2890	2899	rVB5	2790	4627	1.24%	0.163%
24	10.394	2902	2909	2913	rBV5	3314	4487	1.20%	0.158%
25	10.860	3045	3054	3065	rVB6	5776	9035	2.42%	0.318%
26	11.188	3145	3156	3175	rBV	175042	280253	74.92%	9.873%
27	11.490	3238	3250	3263	rBV6	8513	22785	6.09%	0.803%
28	11.564	3263	3273	3293	rVB	128318	213400	57.05%	7.518%




Sum of corrected areas: 2838473

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102023\
Data File : VV032540.D
Acq On : 20 Oct 2023 22:17
Operator : SY/MD
Sample : 04950-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49E8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

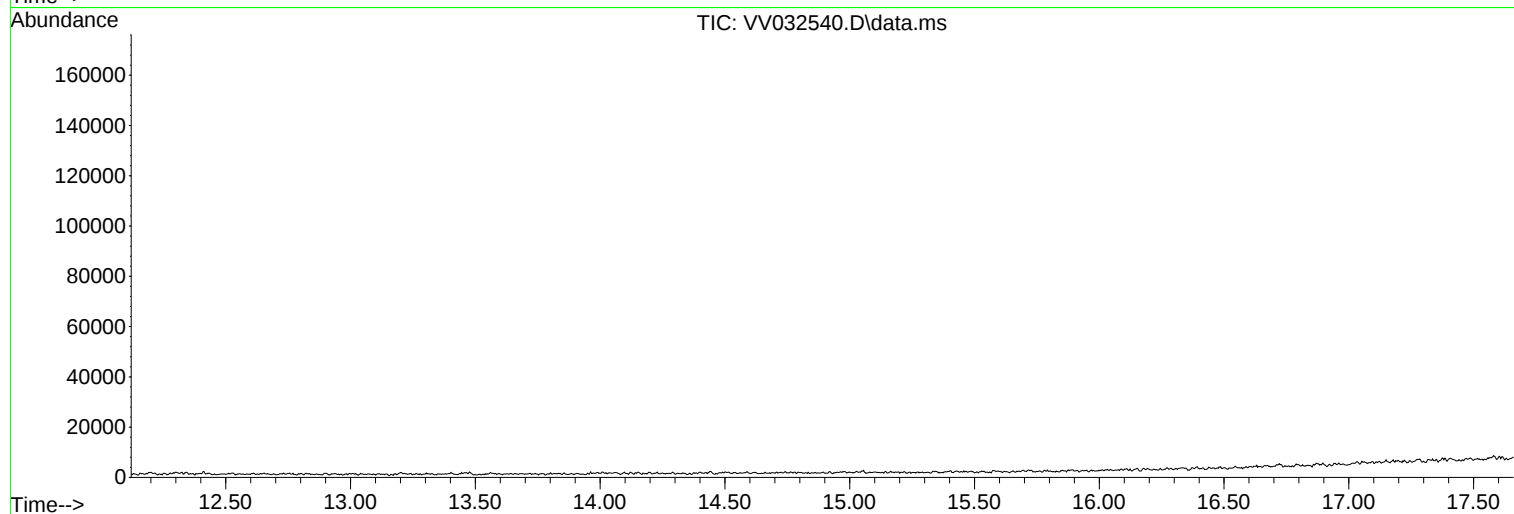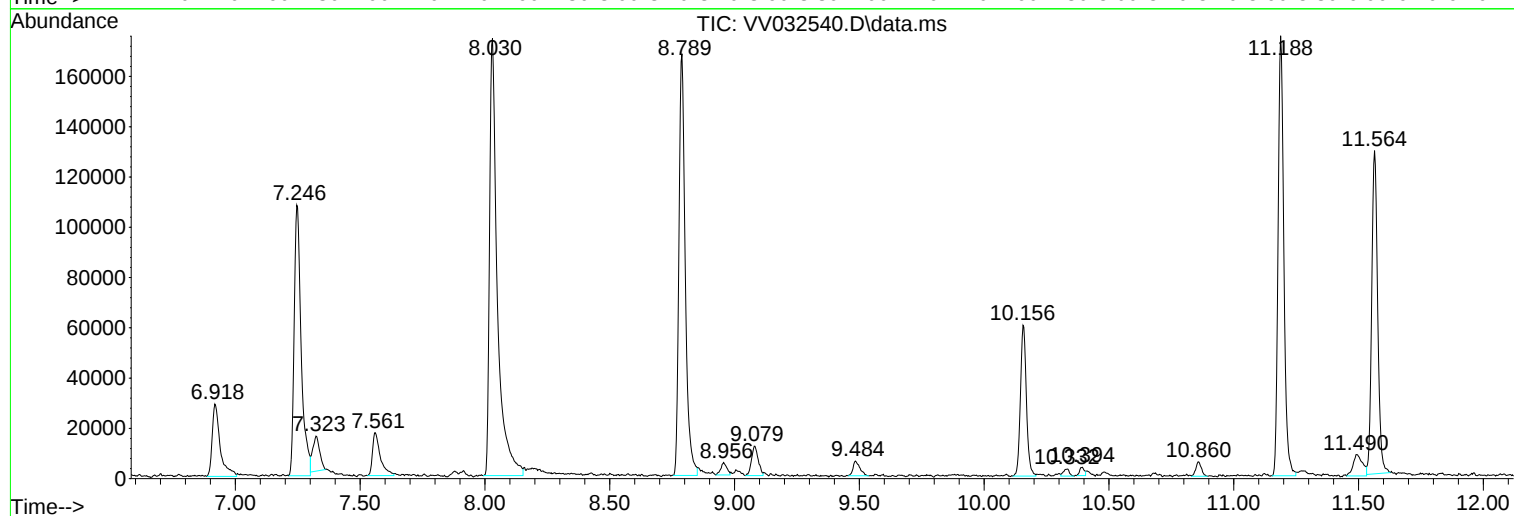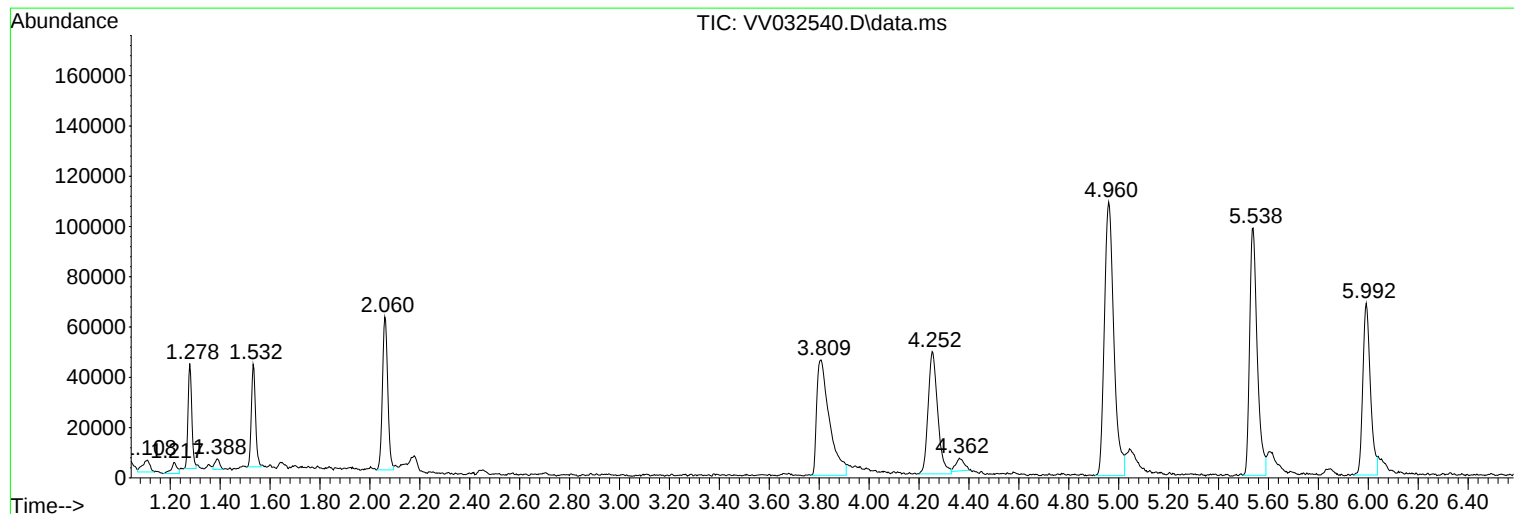

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102023\
Data File : VV032540.D
Acq On : 20 Oct 2023 22:17
Operator : SY/MD
Sample : 04950-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49E8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102023\
Data File : VV032540.D
Acq On : 20 Oct 2023 22:17
Operator : SY/MD
Sample : 04950-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49E8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc