

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102023\
 Data File : VV032542.D
 Acq On : 20 Oct 2023 23:06
 Operator : SY/MD
 Sample : 04994-11
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B37

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032542.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.191	38	47	51	rBV3	3359	4297	1.03%	0.135%
2	1.278	65	74	85	rBV	41002	46210	11.12%	1.448%
3	1.359	92	99	108	rBV	4146	6677	1.61%	0.209%
4	1.532	143	153	166	rBV	40208	49169	11.83%	1.541%
5	2.060	308	317	332	rVB	60224	89211	21.47%	2.796%
6	2.175	346	353	365	rVB3	7322	14683	3.53%	0.460%
7	2.449	431	438	447	rVB6	3376	6420	1.55%	0.201%
8	2.632	481	495	500	rBV9	3829	8658	2.08%	0.271%
9	3.812	849	862	897	rBV2	38316	161361	38.84%	5.057%
10	4.275	981	1006	1026	rBV4	128079	415462	100.00%	13.021%
11	4.381	1028	1039	1067	rVB5	18373	63292	15.23%	1.984%
12	4.960	1202	1219	1239	rBV2	109066	286656	69.00%	8.984%
13	5.539	1388	1399	1415	rBV2	95283	200557	48.27%	6.286%
14	5.992	1524	1540	1554	rBV	67478	147276	35.45%	4.616%
15	6.436	1666	1678	1692	rBV2	36319	75330	18.13%	2.361%
16	6.918	1818	1828	1848	rBV2	28625	60198	14.49%	1.887%
17	7.246	1918	1930	1950	rBV	107989	212784	51.22%	6.669%
18	7.561	2020	2028	2039	rBV	17424	32294	7.77%	1.012%
19	7.879	2119	2127	2135	rBV4	3506	6105	1.47%	0.191%
20	8.030	2163	2174	2206	rBV	177533	391755	94.29%	12.278%
21	8.182	2212	2221	2237	rVB3	9925	20575	4.95%	0.645%
22	8.789	2396	2410	2431	rBV	161672	291285	70.11%	9.129%
23	10.156	2825	2835	2848	rBV	60947	99194	23.88%	3.109%
24	10.326	2878	2888	2898	rBV3	6953	11676	2.81%	0.366%
25	11.188	3144	3156	3173	rBV	172500	269726	64.92%	8.454%
26	11.564	3262	3273	3293	rBV	129591	208279	50.13%	6.528%
27	12.294	3493	3500	3509	rBV9	7637	11520	2.77%	0.361%




Sum of corrected areas: 3190650

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102023\
Data File : VV032542.D
Acq On : 20 Oct 2023 23:06
Operator : SY/MD
Sample : 04994-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B37

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

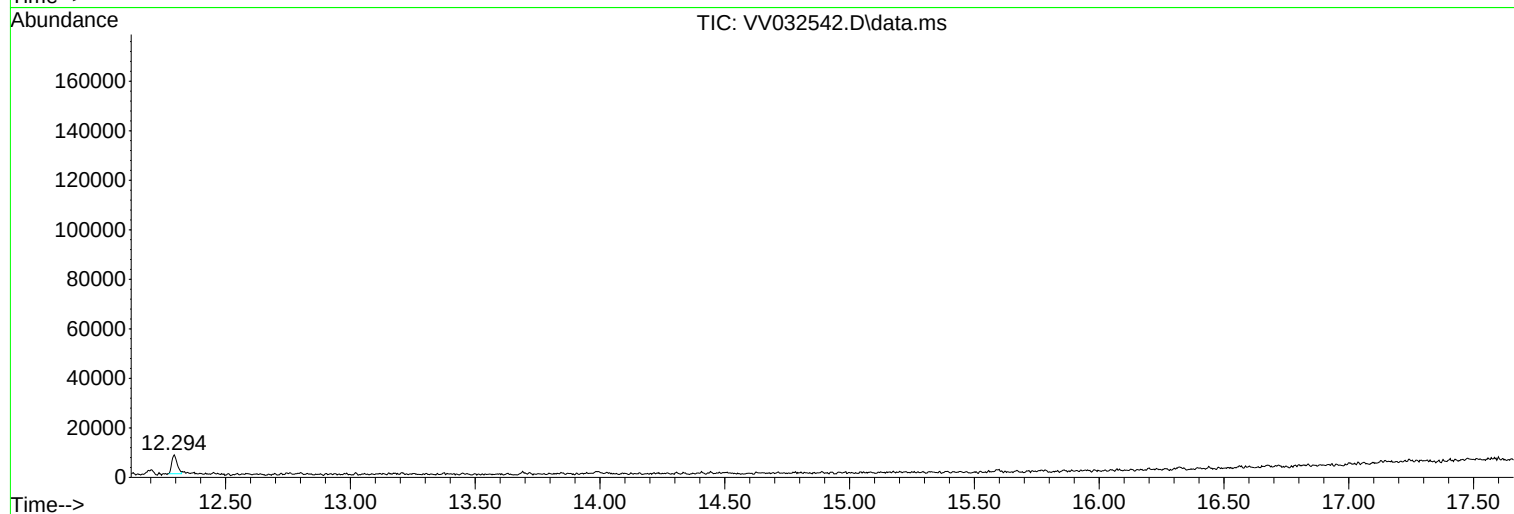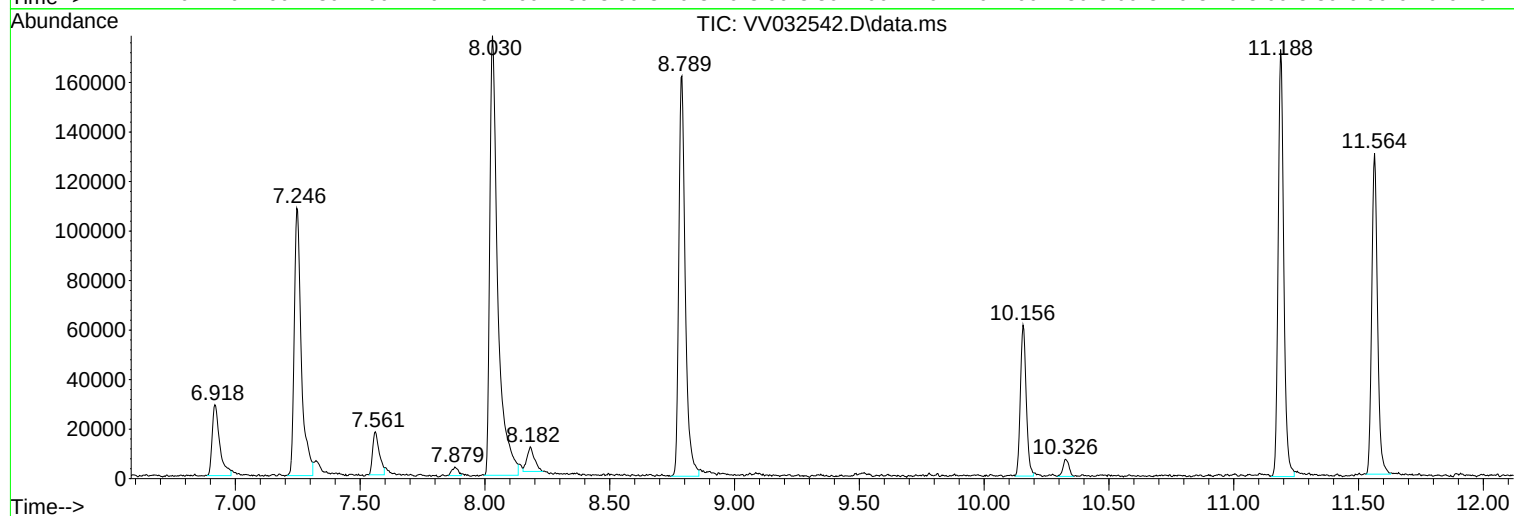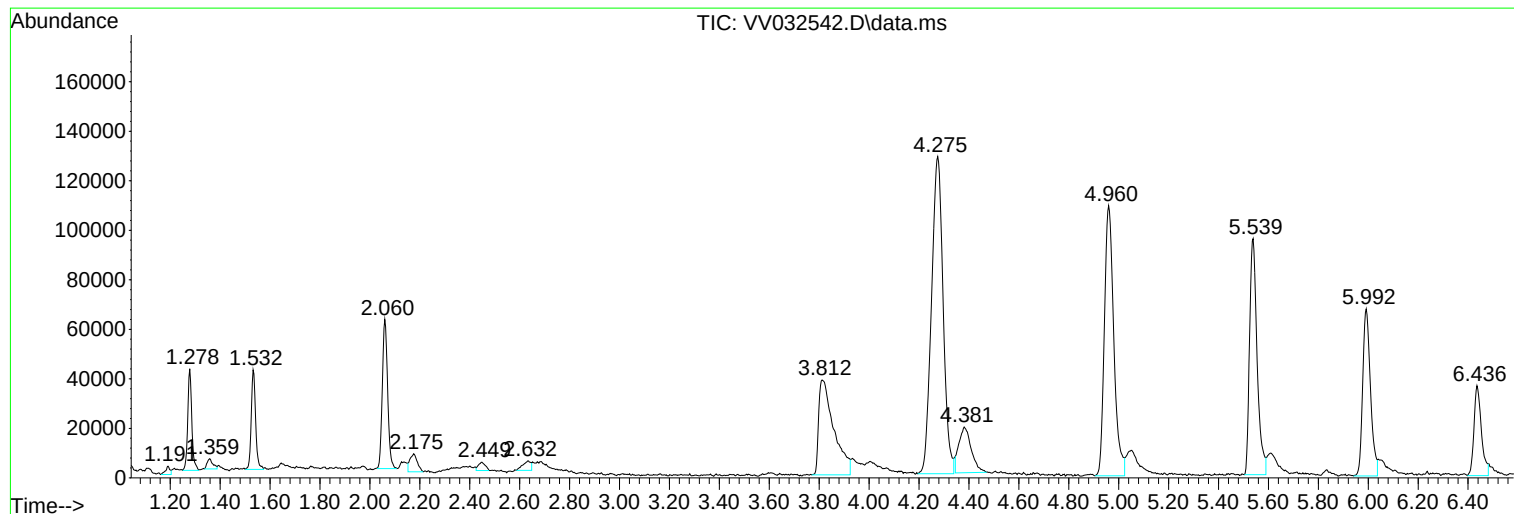

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102023\
Data File : VV032542.D
Acq On : 20 Oct 2023 23:06
Operator : SY/MD
Sample : 04994-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B37

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102023\
Data File : VV032542.D
Acq On : 20 Oct 2023 23:06
Operator : SY/MD
Sample : 04994-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B37

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc