

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102023\
 Data File : VV032552.D
 Acq On : 21 Oct 2023 03:09
 Operator : SY/MD
 Sample : 04993-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AT7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV032552.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.812	847	862	902	rBV2	47676	195224	1.72%	1.436%
2	4.252	983	999	1020	rBV2	45036	119784	1.06%	0.881%
3	4.960	1204	1219	1238	rBV3	99352	260469	2.30%	1.916%
4	5.539	1386	1399	1414	rBV2	88011	187046	1.65%	1.376%
5	5.992	1527	1540	1554	rBV	63438	134721	1.19%	0.991%
6	7.246	1919	1930	1955	rBV	102362	204621	1.80%	1.506%
7	7.908	2115	2136	2165	rBV	6541210	11346327	100.00%	83.483%
8	8.030	2165	2174	2208	rVB	195525	416000	3.67%	3.061%
9	8.789	2398	2410	2428	rBV	152589	275612	2.43%	2.028%
10	11.188	3144	3156	3174	rBV	160333	254279	2.24%	1.871%
11	11.564	3262	3273	3290	rBV	120892	197033	1.74%	1.450%




Sum of corrected areas: 13591116

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102023\
Data File : VV032552.D
Acq On : 21 Oct 2023 03:09
Operator : SY/MD
Sample : 04993-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AT7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

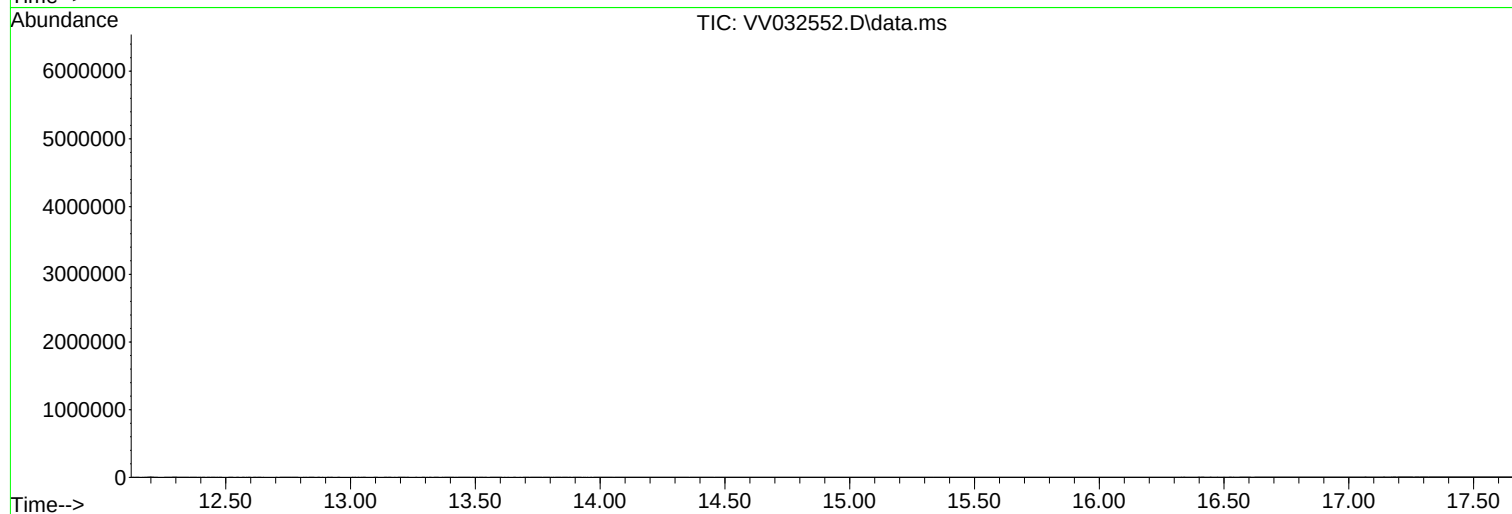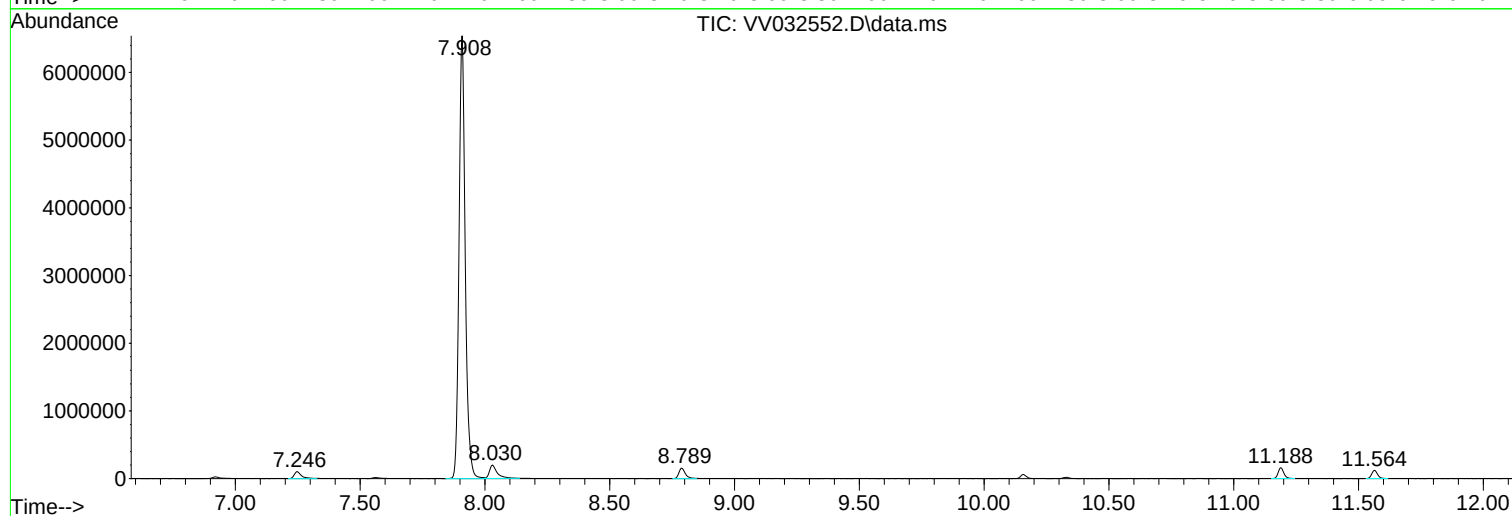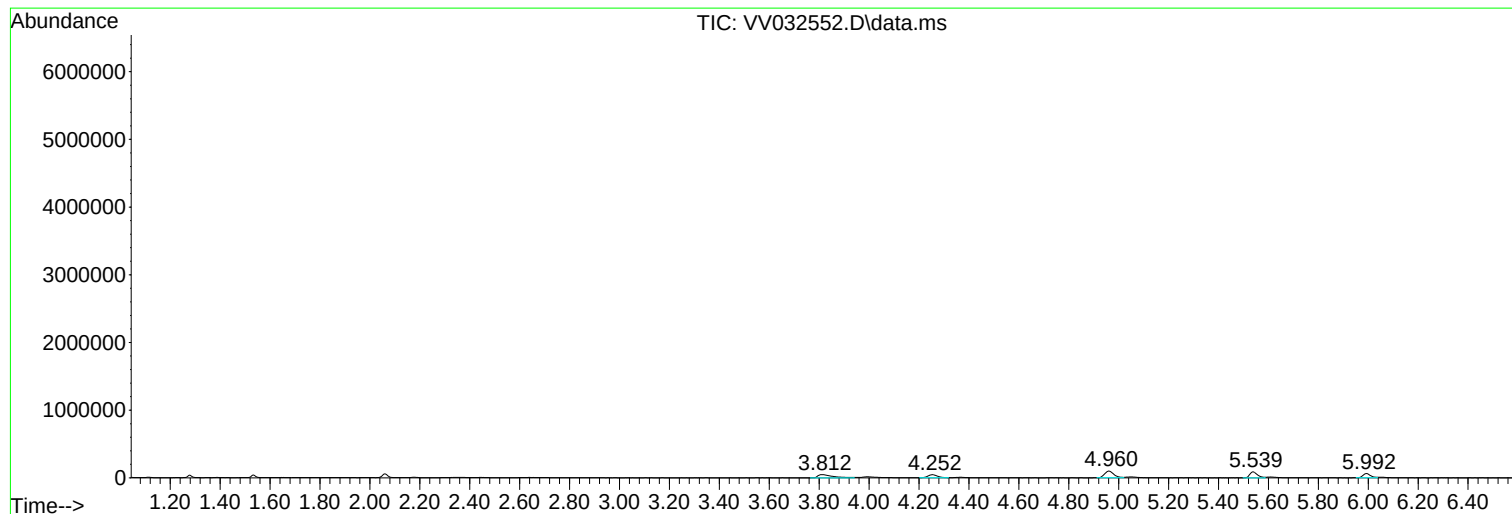

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102023\
Data File : VV032552.D
Acq On : 21 Oct 2023 03:09
Operator : SY/MD
Sample : 04993-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AT7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102023\
Data File : VV032552.D
Acq On : 21 Oct 2023 03:09
Operator : SY/MD
Sample : 04993-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AT7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc