


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102023\
Data File : VV032509.D
Acq On : 20 Oct 2023 08:26
Operator : SY/MD
Sample : BFB224
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB224

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Sat Oct 21 02:44:24 2023

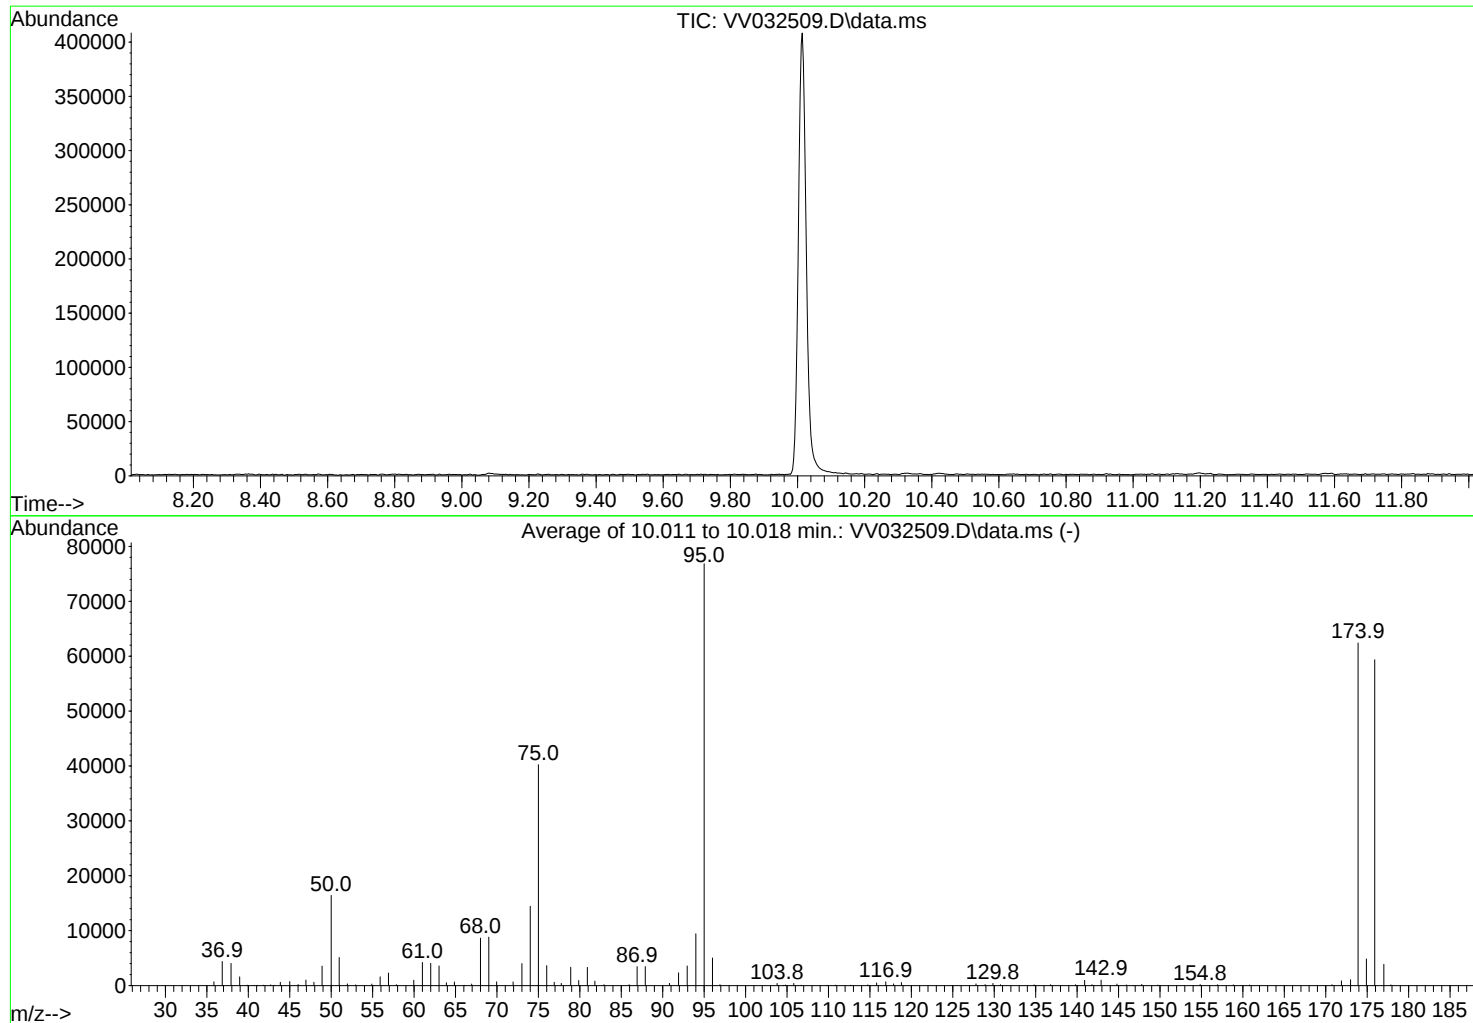

AutoFind: Scans 2790, 2791, 2792; Background Corrected with Scan 2778

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.4	16432	PASS
75	95	30	80	52.4	40245	PASS
95	95	100	100	100.0	76835	PASS
96	95	5	9	6.5	5024	PASS
173	174	0.00	2	1.7	1063	PASS
174	95	50	120	81.2	62421	PASS
175	174	5	9	7.8	4841	PASS
176	174	95	105	95.1	59365	PASS
177	176	5	10	6.5	3871	PASS

m/z	Abundance
35.80	187.0
36.70	137.0
37.10	107.0
37.80	111.0
39.10	125.0
39.80	199.0
42.20	100.0
43.80	313.0
50.80	101.0

Instrument :
MSVOA_V
ClientSampleId :
BFB224

m/z	Abundance
35.90	992.0
36.90	4759.0
37.90	4124.0
38.90	1825.0
39.90	298.0
41.10	116.0
42.70	128.0
43.90	857.0
45.00	819.0
46.00	152.0
46.90	1098.0
47.90	613.0
48.90	3521.0
50.00	16258.0
51.00	5366.0
51.90	344.0
53.00	122.0
54.90	256.0
55.90	1592.0
56.90	2302.0
57.90	129.0
59.90	995.0
61.00	4389.0
62.00	4228.0
63.00	3516.0
63.90	512.0
64.80	685.0
66.10	104.0
67.00	310.0
68.00	8928.0
69.00	8835.0
69.90	750.0
72.00	658.0
73.00	3947.0
74.00	14733.0
75.00	41224.0
76.00	3557.0
76.90	640.0
77.80	422.0
78.90	3365.0
79.90	885.0
80.90	3410.0
81.80	799.0
83.00	165.0
86.00	182.0
86.90	3690.0
87.90	3557.0
90.80	391.0
91.90	2317.0
92.90	3490.0
94.00	9433.0
95.00	77512.0
96.00	5292.0
96.90	110.0
103.80	399.0
104.60	173.0
105.80	431.0
106.70	122.0
109.80	117.0
110.80	127.0
112.70	103.0
114.90	147.0
115.80	502.0
116.90	642.0
117.90	319.0
118.80	577.0
127.80	279.0
128.90	211.0
129.90	423.0
130.70	133.0
134.80	145.0
136.80	156.0
139.70	158.0
140.90	934.0
141.80	175.0
142.90	1119.0
144.80	269.0
146.00	120.0
146.80	131.0
147.80	204.0
149.80	118.0
154.80	218.0
157.00	174.0
158.90	139.0
170.80	151.0
171.90	861.0
173.00	964.0
173.90	61520.0
174.90	4994.0
175.90	58680.0
177.00	3806.0
177.90	143.0

Instrument :
MSVOA_V
ClientSampleId :
BFB224

m/z	Abundance
35.90	899.0
36.90	4819.0
38.00	4277.0
39.00	1767.0
39.90	258.0
41.80	102.0
42.70	124.0
43.10	122.0
43.90	945.0
45.00	735.0
46.00	184.0
47.00	1015.0
47.90	600.0
48.90	3623.0
50.00	16968.0
51.00	5361.0
51.90	332.0
53.00	144.0
54.90	262.0
55.90	1610.0
56.90	2361.0
57.80	169.0
60.00	1011.0
61.00	4335.0
62.00	4145.0
63.00	3691.0
63.90	523.0
64.90	681.0
67.00	303.0
68.00	8935.0
69.00	9125.0
69.90	686.0
72.00	683.0
73.00	4127.0
74.00	14888.0
75.00	41600.0
76.00	3747.0
76.90	654.0
77.70	438.0
78.90	3440.0
79.80	941.0
80.90	3400.0
81.80	840.0
82.90	170.0
86.00	161.0
86.90	3597.0
87.90	3624.0
90.80	408.0
91.90	2361.0
93.00	3700.0
94.00	9665.0
95.00	79152.0
96.00	5172.0
96.90	148.0
103.80	409.0
104.80	168.0
105.80	400.0
106.70	111.0
110.80	115.0
112.70	101.0
114.70	136.0
115.80	481.0
116.90	700.0
117.80	345.0
118.80	565.0
127.80	283.0
128.90	206.0
129.80	414.0
130.80	161.0
134.80	134.0
136.80	161.0
139.80	166.0
140.90	993.0
141.80	187.0
142.90	1042.0
144.80	288.0
146.00	121.0
147.80	220.0
149.70	119.0
154.90	198.0
157.00	153.0
158.80	136.0
160.80	127.0
170.70	188.0
171.90	889.0
173.00	1113.0
173.90	64480.0
174.90	4994.0
175.90	61008.0
177.00	4018.0
177.90	127.0

Instrument :
MSVOA_V
ClientSampleId :
BFB224

m/z	Abundance
35.90	780.0
36.90	4350.0
38.00	4050.0
39.00	1563.0
40.00	257.0
40.70	108.0
41.80	112.0
42.70	112.0
43.10	106.0
43.90	970.0
45.00	677.0
46.00	200.0
47.00	918.0
47.90	594.0
48.90	3519.0
50.00	16070.0
51.00	4899.0
52.00	294.0
52.90	168.0
54.90	274.0
55.90	1557.0
56.90	2190.0
57.80	201.0
59.90	901.0
61.00	3932.0
62.00	3739.0
63.00	3480.0
63.90	484.0
64.90	630.0
66.90	262.0
68.00	8079.0
69.00	8455.0
70.00	614.0
71.90	614.0
73.00	3945.0
74.00	13695.0
75.00	37912.0
76.00	3562.0
76.90	544.0
77.70	362.0
78.90	3193.0
79.80	928.0
80.90	3143.0
81.80	810.0
82.80	149.0
85.80	138.0
86.90	3107.0
87.90	3195.0
90.80	383.0
91.90	2317.0
93.00	3561.0
94.00	9235.0
95.00	73840.0
96.00	4608.0
96.90	197.0
103.80	412.0
104.80	169.0
105.80	349.0
114.70	150.0
115.80	436.0
116.90	688.0
117.80	302.0
118.80	474.0
127.80	336.0
128.90	163.0
129.80	360.0
130.80	164.0
134.80	124.0
136.80	143.0
139.90	120.0
140.90	912.0
141.80	147.0
142.90	909.0
144.80	292.0
145.90	144.0
147.80	209.0
149.70	121.0
154.80	171.0
156.90	154.0
158.80	117.0
160.80	167.0
170.70	175.0
171.90	872.0
173.00	1111.0
173.90	61264.0
174.90	4535.0
175.90	58408.0
177.00	3790.0
177.80	114.0

Instrument :
MSVOA_V
ClientSampleId :
BFB224