

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102119\
 Data File : VV013255.D
 Acq On : 21 Oct 2019 20:34
 Operator : SY/MD
 Sample : K5321-07
 Misc : 25.00ML/MSVOA V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Quant Time: Oct 22 04:10:46 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR102119WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Oct 22 03:42:02 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	493986	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	524928	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	259972	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	185559	5.10	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	102.00%
7) Chloroethane-d5	1.58	69	152828	5.08	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	101.60%
11) 1,1-Dichloroethene-d2	2.13	63	233855	3.61	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	72.20%
20) 2-Butanone-d5	3.96	46	335306	47.94	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	95.88%
24) Chloroform-d	4.40	84	409546	4.78	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.60%
26) 1,2-Dichloroethane-d4	5.08	65	197907	4.98	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.60%
32) Benzene-d6	5.10	84	833515	4.90	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.00%
36) 1,2-Dichloropropane-d6	6.12	67	252340	4.94	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	98.80%
41) Toluene-d8	7.36	98	695741	4.42	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.40%
43) trans-1,3-Dichloropropene-	7.66	79	84885	4.38	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	87.60%
46) 2-Hexanone-d5	8.13	63	290239	42.08	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	84.16%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	175204	4.75	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	95.00%
64) 1,2-Dichlorobenzene-d4	11.67	152	271276	5.36	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	107.20%


Target Compounds					Ovalue
16) Methylene chloride	2.53	84	45966	0.788 ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV102119\
Data File : VV013255.D
Acq On : 21 Oct 2019 20:34
Operator : SY/MD
Sample : K5321-07
Misc : 25.00ML/MSVOA V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Time: Oct 22 04:10:46 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR102119WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Oct 22 03:42:02 2019
Response via : Initial Calibration

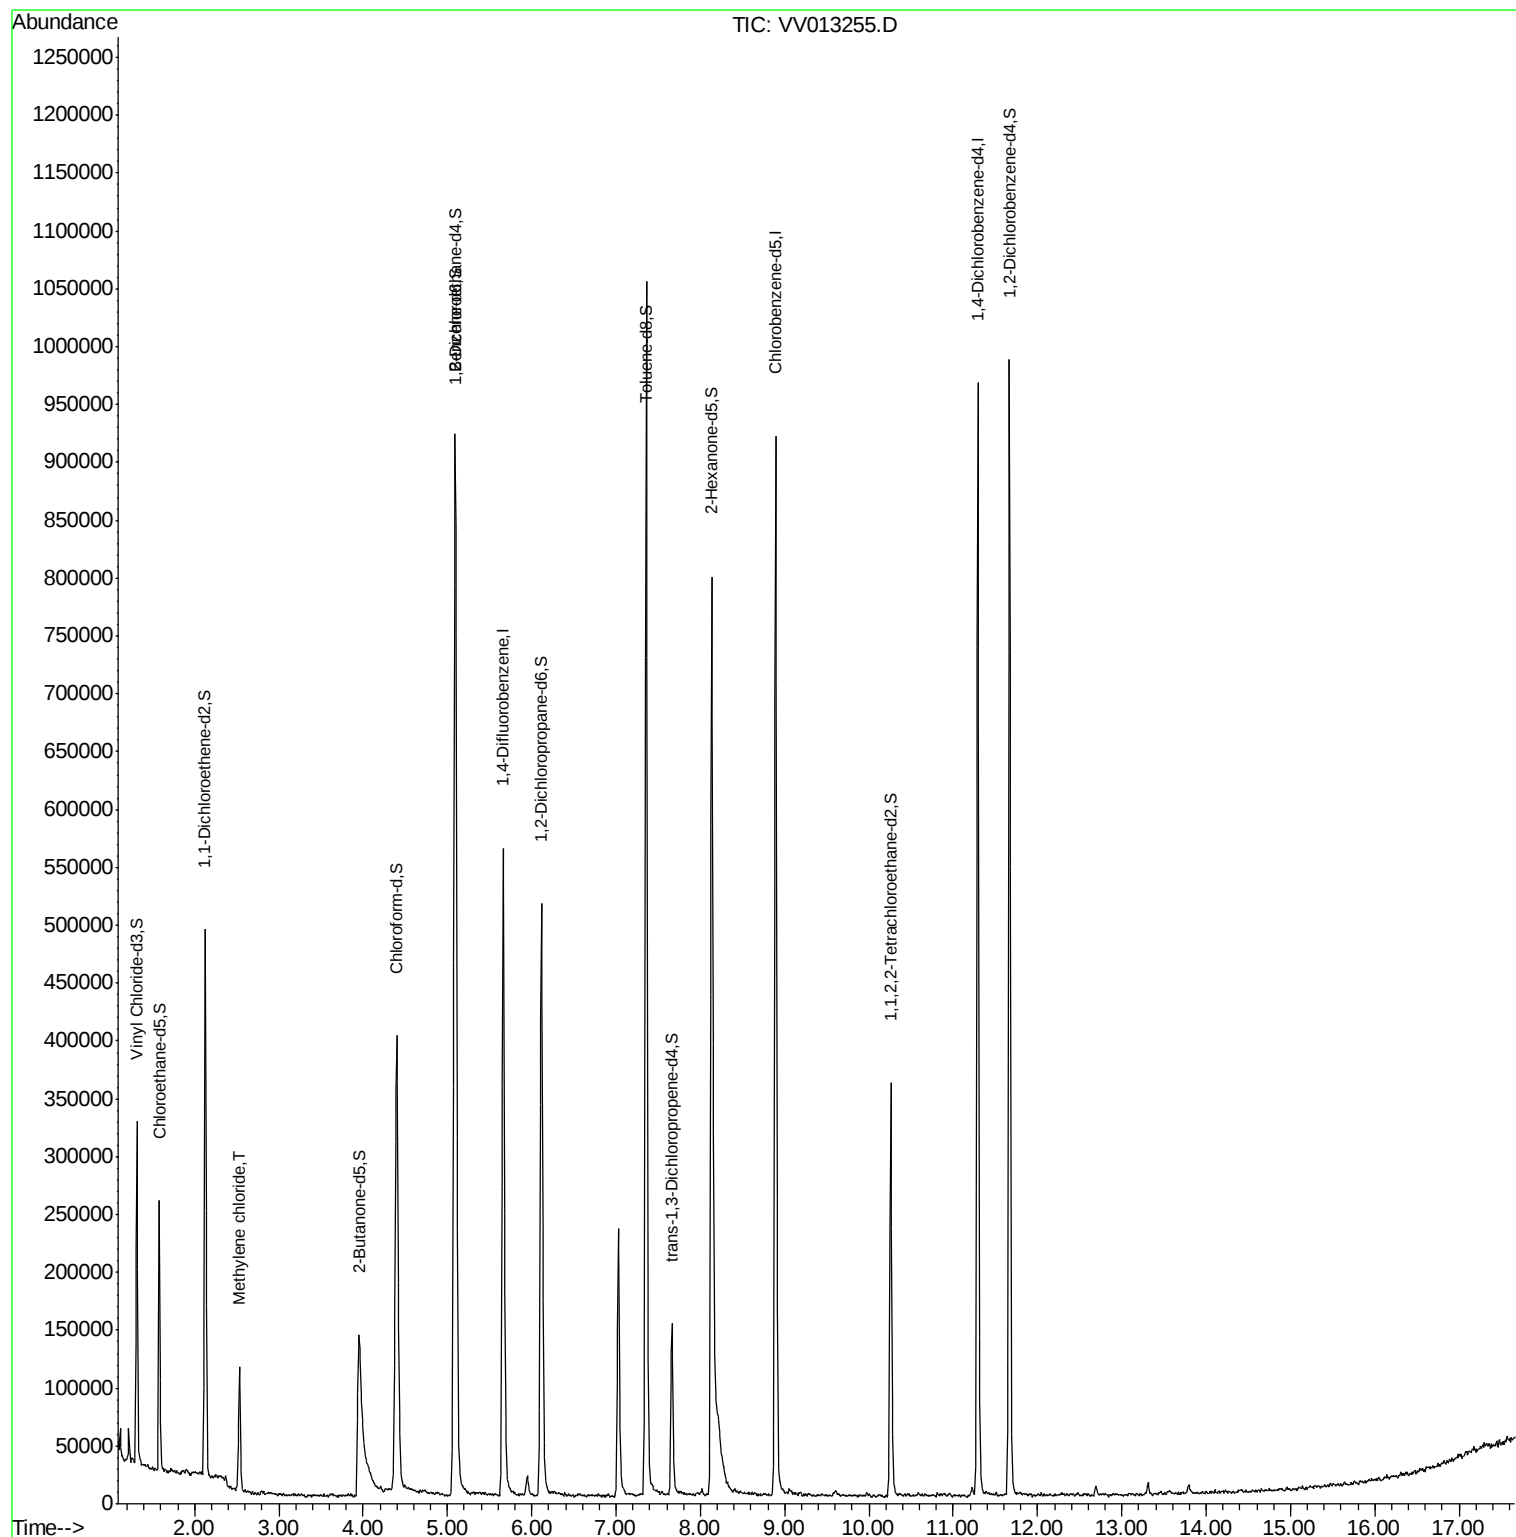

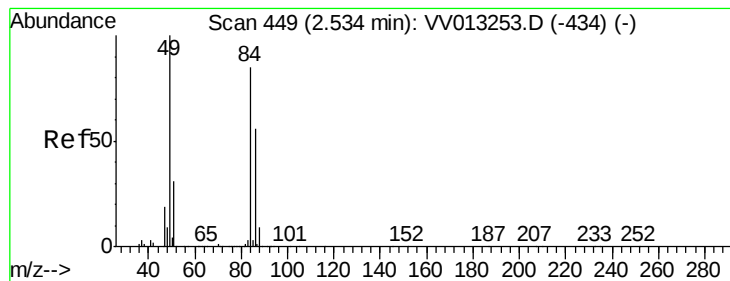

#16
 Methvlene chloride
 Concen: 0.788 ug/L
 RT: 2.53 min Scan# 449
 Delta R.T. 0.00 min
 Lab File: VV013255.D
 Acq: 21 Oct 2019 20:34

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Tot Ion	Ion	Ratio	Lower	Upper
84	100			
86	63.0	46.2	85.8	
49	113.4	76.4	141.8	

