


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV102119\
 Data File : VV013242.D
 Acq On : 21 Oct 2019 09:35
 Operator : SY/MD
 Sample : BFB45
 Misc : 25.00ML/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB45

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR101819WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Mon Oct 21 13:49:27 2019

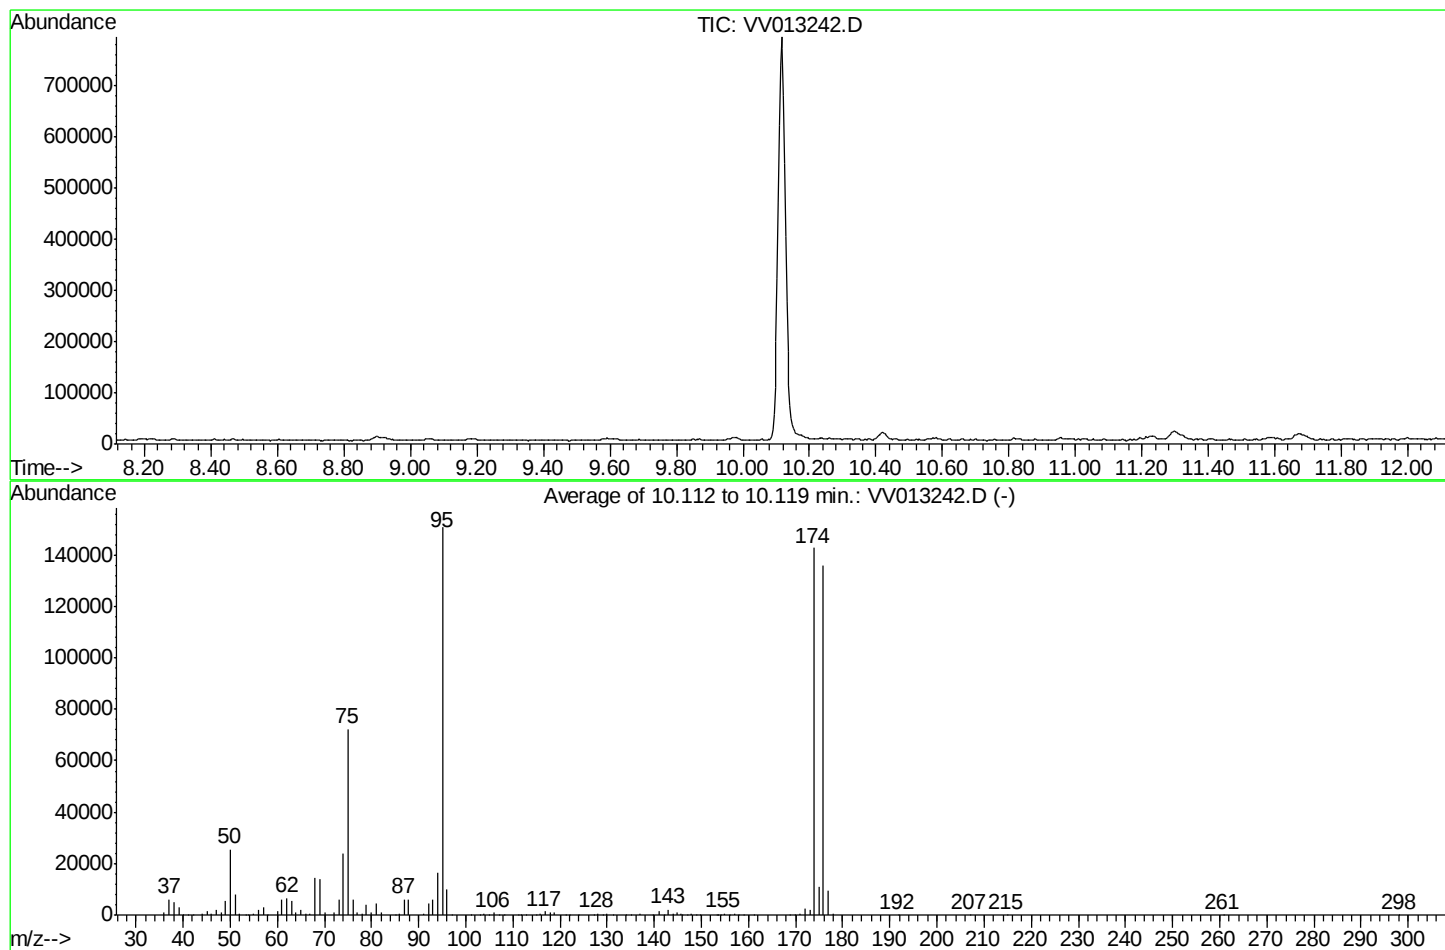

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2791

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.9	25530	PASS
75	95	30	80	48.0	72341	PASS
95	95	100	100	100.0	150762	PASS
96	95	5	9	6.6	9955	PASS
173	174	0.00	2	1.3	1909	PASS
174	95	50	120	94.8	142848	PASS
175	174	5	9	7.5	10783	PASS
176	174	95	101	95.1	135888	PASS
177	176	5	9	6.9	9313	PASS

m/z	Abundance
36.00	1230.0
37.10	6271.0
38.00	5060.0
39.10	2846.0
40.00	1875.0
40.70	228.0
41.30	260.0
42.30	191.0
43.10	136.0
44.00	2233.0
45.00	1323.0
46.10	374.0
47.00	1845.0
48.00	836.0
49.00	5667.0
50.00	24824.0
51.00	7755.0
52.00	414.0
53.10	248.0
54.00	159.0
55.10	500.0
56.00	2012.0
57.00	3140.0
57.90	205.0
60.00	1226.0
61.00	5949.0
62.10	6133.0
63.00	5162.0
64.00	1084.0
65.00	1844.0
66.20	275.0
66.90	309.0
68.00	13824.0
69.00	13860.0
70.00	1065.0
71.90	860.0
73.00	6052.0
74.10	23552.0
75.00	70848.0
76.00	6270.0
77.00	1160.0
77.90	644.0
78.90	4179.0
79.90	1226.0
80.90	4305.0
82.00	1118.0
84.90	103.0
86.00	258.0
87.00	6132.0
87.90	5945.0
91.00	291.0
92.00	4427.0
93.00	6260.0
94.00	16880.0
95.00	146112.0
96.00	9994.0
97.00	268.0
103.00	137.0
103.90	635.0
104.80	211.0
105.90	652.0
106.90	165.0
108.20	104.0
112.90	172.0
115.00	231.0
116.00	537.0
116.90	1238.0
118.00	733.0
118.90	1017.0
124.00	128.0
127.90	615.0
129.00	281.0
129.90	404.0
131.10	244.0
134.00	137.0
135.00	248.0
136.80	300.0
139.80	128.0
140.90	1524.0
143.00	2157.0
143.90	243.0
144.90	837.0
145.80	313.0
147.80	427.0
149.70	209.0
153.30	209.0
154.10	129.0
154.80	477.0
156.00	202.0
157.00	423.0
159.00	189.0
161.10	179.0

Instrument :
MSVOA_V
ClientSampleId :
BFB45

169.70	123.0
171.00	438.0
172.00	2375.0
173.00	1904.0
173.90	134528.0
175.00	10363.0
175.90	128048.0
176.90	9040.0
178.00	300.0
191.80	103.0
206.90	322.0
214.90	118.0

Instrument :
MSVOA_V
ClientSampleId :
BFB45

m/z	Abundance
36.00	1383.0
37.00	6401.0
38.00	5382.0
39.10	3047.0
40.00	1835.0
41.10	240.0
42.10	192.0
43.10	163.0
44.00	2287.0
45.00	1516.0
46.00	358.0
47.00	1705.0
48.00	840.0
49.00	5826.0
50.00	26256.0
51.00	8274.0
52.00	440.0
53.20	288.0
53.90	208.0
55.00	492.0
56.00	2142.0
57.00	3269.0
57.90	184.0
60.00	1463.0
61.00	6482.0
62.00	6822.0
63.00	5576.0
64.00	1021.0
65.00	1905.0
66.00	274.0
66.90	373.0
68.00	14854.0
69.00	14580.0
70.00	1134.0
71.90	997.0
73.00	6362.0
74.00	24904.0
75.00	74912.0
76.00	6466.0
76.90	1146.0
78.00	652.0
78.90	4348.0
79.90	1226.0
80.90	4806.0
82.00	1171.0
85.00	123.0
85.90	345.0
86.90	6377.0
87.90	6085.0
90.90	362.0
92.00	4503.0
93.00	6408.0
94.00	16936.0
95.00	155968.0
96.00	10379.0
97.00	259.0
101.10	101.0
102.90	145.0
103.80	709.0
104.80	228.0
105.90	834.0
107.00	173.0
108.20	102.0
111.80	104.0
112.90	149.0
115.00	281.0
115.80	634.0
116.80	1435.0
117.90	820.0
118.80	1054.0
121.30	115.0
122.00	108.0
123.80	115.0
127.10	125.0
127.80	661.0
128.90	252.0
129.90	468.0
131.20	274.0
135.00	251.0
136.90	298.0
139.80	178.0
140.90	1634.0
142.00	229.0
143.00	2270.0
143.90	352.0
144.90	846.0
145.70	343.0
146.90	119.0
147.80	411.0
149.00	186.0
149.80	266.0
153.40	179.0

Instrument :
MSVOA_V
ClientSampleId :
BFB45

154.10	124.0
154.80	533.0
156.10	251.0
156.90	521.0
159.00	213.0
161.10	201.0
168.60	121.0
171.00	437.0
172.00	2635.0
173.00	1932.0
173.90	147968.0
175.00	11120.0
175.90	140608.0
176.90	9677.0
178.00	355.0
191.80	102.0
206.90	278.0
214.90	134.0

Instrument :
MSVOA_V
ClientSampleId :
BFB45

m/z	Abundance
35.90	1269.0
37.00	5835.0
38.00	5587.0
39.10	2785.0
39.90	1721.0
41.10	251.0
42.10	213.0
43.10	197.0
44.00	2174.0
45.10	1551.0
46.00	297.0
47.00	1787.0
48.00	785.0
49.00	5731.0
50.00	25512.0
51.00	8084.0
52.10	433.0
53.20	249.0
53.90	227.0
55.00	505.0
56.00	2174.0
57.00	3274.0
58.00	147.0
60.00	1583.0
61.00	6237.0
62.00	6855.0
63.00	5454.0
64.00	1010.0
65.00	1883.0
66.00	290.0
66.90	456.0
68.00	14162.0
69.00	14101.0
70.00	1163.0
71.90	927.0
73.00	6026.0
74.00	23616.0
75.00	71264.0
76.00	5787.0
76.80	1149.0
78.00	612.0
78.90	4132.0
79.90	1148.0
80.90	4766.0
81.90	1206.0
85.00	136.0
85.90	374.0
86.90	6031.0
87.90	5974.0
90.90	445.0
92.00	4045.0
93.00	5927.0
94.00	15483.0
95.00	150208.0
96.00	9494.0
97.10	254.0
101.10	116.0
102.90	107.0
103.80	693.0
104.80	192.0
105.90	905.0
107.00	156.0
111.10	104.0
111.80	122.0
115.00	283.0
115.80	713.0
116.80	1387.0
117.80	778.0
118.90	892.0
121.30	127.0
123.80	139.0
125.00	112.0
127.10	173.0
127.90	659.0
128.90	228.0
129.90	548.0
131.30	203.0
134.90	197.0
137.00	263.0
139.80	183.0
140.90	1478.0
142.00	257.0
142.90	2271.0
143.90	345.0
144.90	884.0
145.70	362.0
146.00	304.0
146.90	132.0
147.80	338.0
149.00	244.0
149.90	314.0
153.60	126.0

Instrument :
MSVOA_V
ClientSampleId :
BFB45

154.80	564.0
156.10	182.0
156.90	544.0
158.00	159.0
158.90	190.0
161.00	156.0
168.70	118.0
171.00	410.0
172.00	2636.0
173.00	1893.0
173.90	146048.0
175.00	10868.0
175.90	139008.0
176.90	9222.0
178.00	366.0
207.00	227.0
260.70	102.0
298.10	111.0

Instrument :
MSVOA_V
ClientSampleId :
BFB45

m/z	Abundance
35.00	229.0
35.80	228.0
37.20	148.0
38.20	115.0
38.80	121.0
40.00	1650.0
40.80	109.0
43.00	293.0
44.00	1901.0
44.80	152.0
46.30	180.0
49.20	132.0
49.50	125.0
52.20	152.0
54.30	106.0
55.00	126.0
60.70	114.0
61.40	124.0
65.00	108.0
68.40	123.0
74.40	174.0
77.00	152.0
78.10	117.0
93.00	119.0
96.30	121.0
115.60	102.0
123.30	120.0
125.00	116.0
133.00	165.0
134.60	112.0
207.00	191.0
207.20	198.0
235.20	101.0
280.80	159.0

Instrument :
MSVOA_V
ClientSampleId :
BFB45