

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102120\
 Data File : VV019048.D
 Acq On : 21 Oct 2020 14:37
 Operator : SY/MD
 Sample : L4483-05 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FH3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	80	rVB	109467	110765	2.11%	0.589%
2	1.579	145	152	162	rVB	107664	121019	2.30%	0.643%
3	2.122	312	321	350	rVB	210572	334053	6.36%	1.776%
4	2.412	408	411	413	rBV3	934	515	0.01%	0.003%
5	2.849	544	547	550	rBV3	497	329	0.01%	0.002%
6	3.244	668	670	671	rBV	225	82	0.00%	0.000%
7	3.408	719	721	723	rVB2	377	139	0.00%	0.001%
8	3.482	742	744	746	rBV2	428	209	0.00%	0.001%
9	3.511	749	753	761	rBV2	376	604	0.01%	0.003%
10	3.595	777	779	780	rBV2	137	40	0.00%	0.000%
11	3.682	803	806	807	rBV	417	180	0.00%	0.001%
12	3.862	857	862	865	rBV	445	419	0.01%	0.002%
13	3.916	867	879	912	rBV2	77206	244611	4.66%	1.301%
14	4.376	1007	1022	1049	rBV	163625	417046	7.94%	2.218%
15	4.711	1119	1126	1131	rBV6	918	1373	0.03%	0.007%
16	4.945	1197	1199	1201	rBV	386	199	0.00%	0.001%
17	5.074	1221	1239	1247	rBV2	387200	995487	18.96%	5.293%
18	5.482	1361	1366	1370	rBV4	673	698	0.01%	0.004%
19	5.540	1381	1384	1386	rBV	116	76	0.00%	0.000%
20	5.563	1388	1391	1394	rVB	462	336	0.01%	0.002%
21	5.582	1394	1397	1403	rVB3	669	627	0.01%	0.003%
22	5.640	1403	1415	1443	rBV	372934	743937	14.17%	3.956%
23	5.929	1493	1505	1521	rBV2	25707	53838	1.03%	0.286%
24	6.093	1542	1556	1587	rBV	258511	528362	10.06%	2.809%
25	6.772	1766	1767	1768	rBV	321	113	0.00%	0.001%
26	6.797	1774	1775	1778	rBV	402	260	0.00%	0.001%
27	7.010	1829	1841	1870	rBV	116548	213313	4.06%	1.134%
28	7.202	1897	1901	1903	rBV3	602	443	0.01%	0.002%
29	7.293	1927	1929	1931	rBV	186	75	0.00%	0.000%
30	7.338	1931	1943	1963	rBV	388959	664575	12.66%	3.534%
31	7.572	2013	2016	2017	rBV	185	84	0.00%	0.000%
32	7.643	2028	2038	2058	rBV	81075	140869	2.68%	0.749%
33	7.833	2095	2097	2102	rVB	475	347	0.01%	0.002%
34	7.858	2102	2105	2106	rBV2	113	62	0.00%	0.000%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102120\
 Data File : VV019048.D
 Acq On : 21 Oct 2020 14:37
 Operator : SY/MD
 Sample : L4483-05 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FH3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
 Title : VOC Analysis

35	7.878	2106	2111	2115	rBV	316	331	0.01%	0.002%
36	7.961	2134	2137	2140	rVB	258	162	0.00%	0.001%
37	7.977	2140	2142	2143	rBV	172	73	0.00%	0.000%
38	8.109	2172	2183	2218	rBV	242442	459690	8.75%	2.444%
39	8.370	2262	2264	2267	rBV	252	143	0.00%	0.001%
40	8.431	2280	2283	2286	rBV2	315	218	0.00%	0.001%
41	8.447	2286	2288	2289	rBV	274	83	0.00%	0.000%
42	8.534	2313	2315	2317	rBV	266	173	0.00%	0.001%
43	8.601	2331	2336	2339	rBV3	380	291	0.01%	0.002%
44	8.624	2341	2343	2344	rBV	151	66	0.00%	0.000%
45	8.659	2351	2354	2357	rBV	213	195	0.00%	0.001%
46	8.707	2366	2369	2371	rBV2	271	182	0.00%	0.001%
47	8.736	2376	2378	2382	rBV2	146	115	0.00%	0.001%
48	8.813	2399	2402	2403	rBV	132	63	0.00%	0.000%
49	8.900	2408	2429	2470	rBV2	2768277	5251228	100.00%	27.922%
50	9.186	2513	2518	2520	rBV2	308	222	0.00%	0.001%
51	9.283	2544	2548	2551	rBV2	634	479	0.01%	0.003%
52	9.315	2557	2558	2560	rVB2	285	88	0.00%	0.000%
53	9.363	2571	2573	2574	rBV	116	43	0.00%	0.000%
54	9.444	2596	2598	2599	rBV	186	81	0.00%	0.000%
55	9.514	2616	2620	2621	rBV2	205	120	0.00%	0.001%
56	9.563	2633	2635	2638	rBV	181	113	0.00%	0.001%
57	9.598	2644	2646	2648	rBV2	132	74	0.00%	0.000%
58	9.630	2648	2656	2662	rBV2	313	575	0.01%	0.003%
59	9.688	2672	2674	2676	rBV	188	109	0.00%	0.001%
60	9.794	2698	2707	2710	rBV	257	289	0.01%	0.002%
61	9.913	2741	2744	2751	rVB	389	289	0.01%	0.002%
62	9.945	2751	2754	2755	rBV2	90	47	0.00%	0.000%
63	9.961	2755	2759	2760	rBV	158	108	0.00%	0.001%
64	9.971	2760	2762	2767	rVB	366	198	0.00%	0.001%
65	10.000	2768	2771	2774	rBV	208	119	0.00%	0.001%
66	10.022	2774	2778	2780	rBV2	368	277	0.01%	0.001%
67	10.083	2794	2797	2799	rVB	173	99	0.00%	0.001%
68	10.099	2799	2802	2805	rBV2	161	129	0.00%	0.001%
69	10.145	2813	2816	2819	rBV2	145	92	0.00%	0.000%
70	10.161	2819	2821	2826	rVB2	347	222	0.00%	0.001%
71	10.190	2826	2830	2831	rBV2	212	146	0.00%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102120\
Data File : VV019048.D
Acq On : 21 Oct 2020 14:37
Operator : SY/MD
Sample : L4483-05 100X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FH3

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0

Filtering: 5
Min Area: 0 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
Title : VOC Analysis

72	10.238	2833	2845	2863	rBV	270379	427063	8.13%	2.271%
73	10.601	2955	2958	2960	rBV	229	142	0.00%	0.001%
74	10.961	3067	3070	3072	rBV2	177	119	0.00%	0.001%
75	11.202	3134	3145	3156	rBV	170156	264083	5.03%	1.404%
76	11.292	3156	3173	3197	rVB2	1632694	3342524	63.65%	17.773%
77	11.511	3239	3241	3244	rBV2	527	316	0.01%	0.002%
78	11.662	3270	3288	3308	rBV2	2050516	3829730	72.93%	20.364%
79	13.283	3781	3792	3814	rBV	339652	523031	9.96%	2.781%
80	13.768	3933	3943	3968	rVB	80118	127629	2.43%	0.679%


Sum of corrected areas: 18806654

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV102120\
Data File : VV019048.D
Acq On : 21 Oct 2020 14:37
Operator : SY/MD
Sample : L4483-05 100X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FH3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

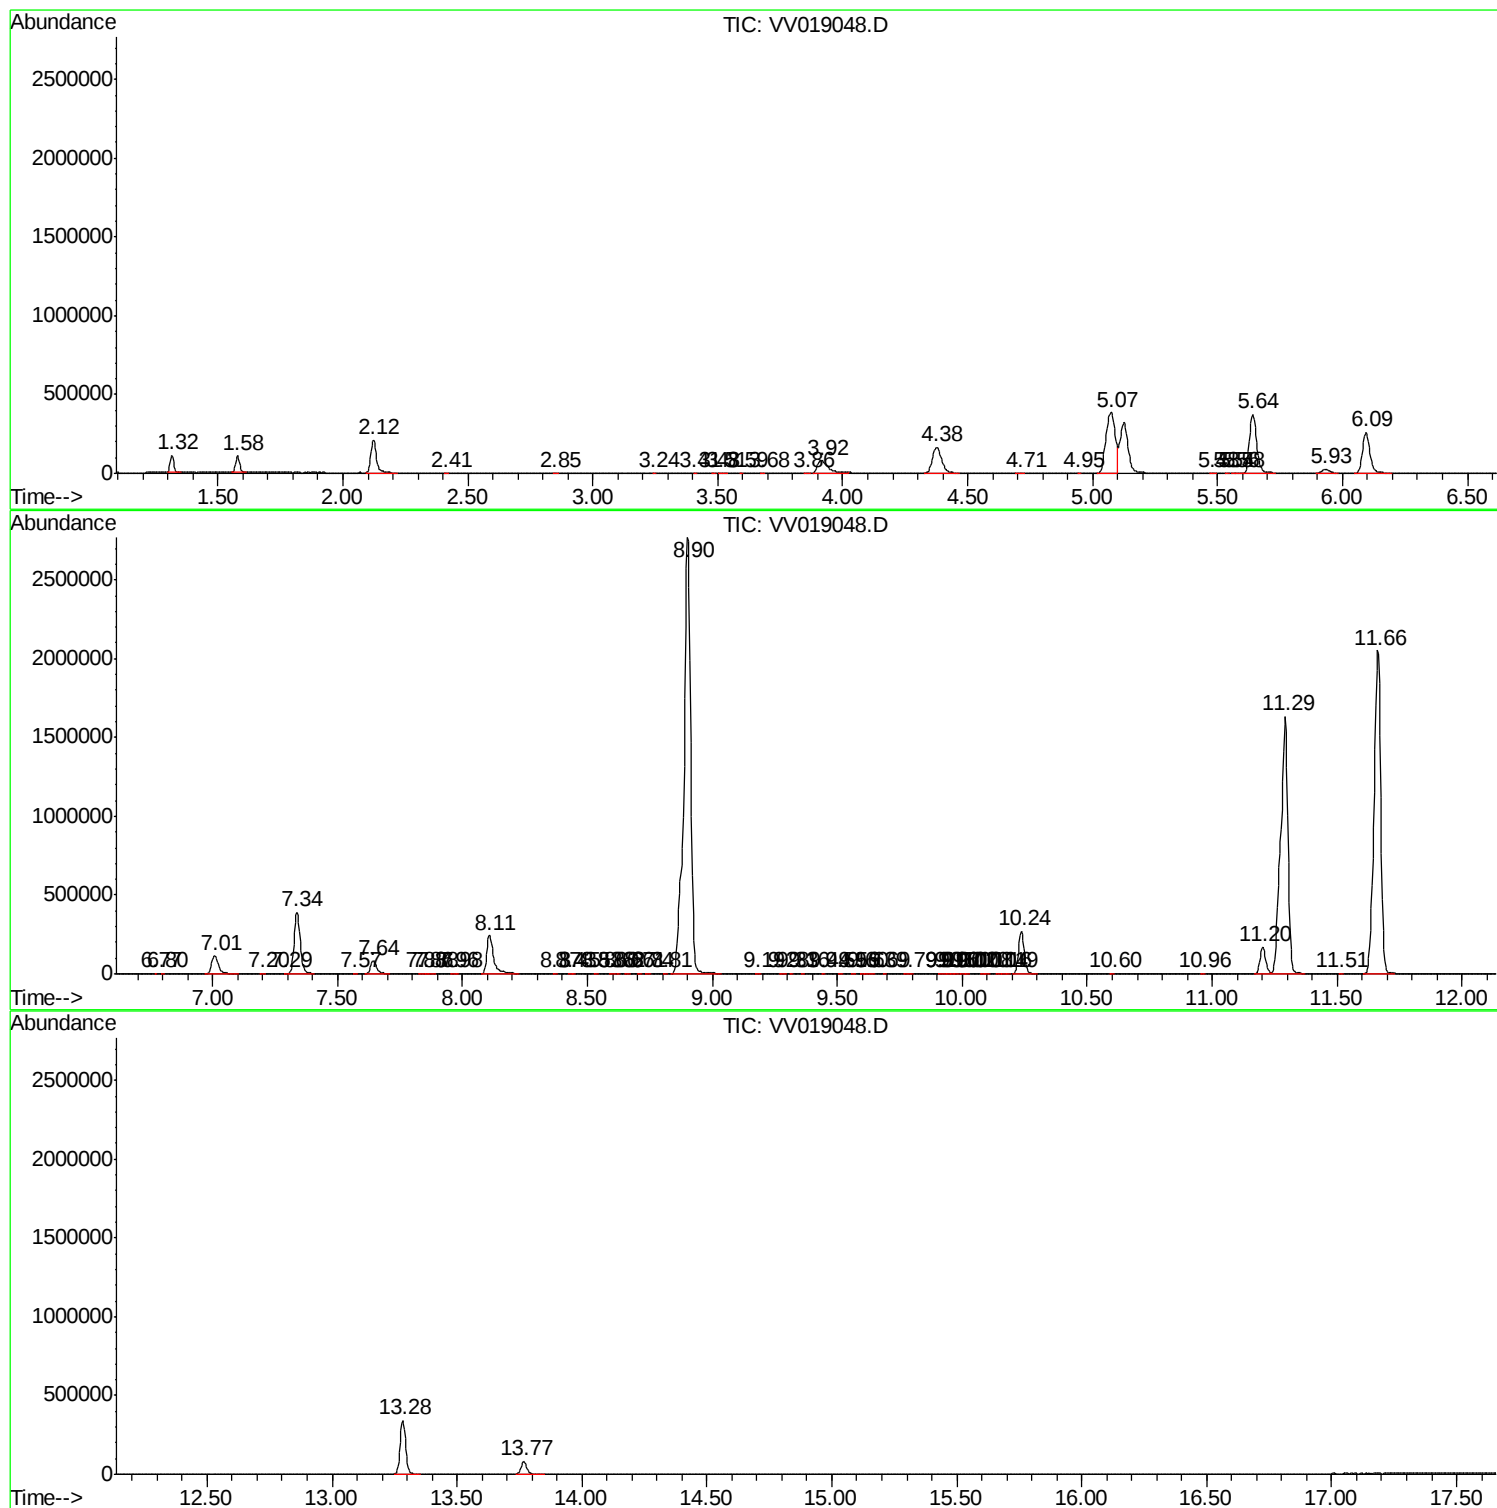

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV102120\
Data File : VV019048.D
Acq On : 21 Oct 2020 14:37
Operator : SY/MD
Sample : L4483-05 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FH3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV102120\
Data File : VV019048.D
Acq On : 21 Oct 2020 14:37
Operator : SY/MD
Sample : L4483-05 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FH3

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc