

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102120\
 Data File : VV019053.D
 Acq On : 21 Oct 2020 16:56
 Operator : SY/MD
 Sample : L4483-03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FH1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	83	rVB	223908	224559	15.84%	1.965%
2	1.579	145	152	164	rVB	177678	200824	14.17%	1.757%
3	2.122	311	321	365	rVB	344300	547827	38.64%	4.793%
4	2.955	577	580	581	rBV	421	230	0.02%	0.002%
5	2.991	589	591	593	rBV	342	165	0.01%	0.001%
6	3.219	661	662	663	rBV	139	42	0.00%	0.000%
7	3.228	663	665	668	rVB2	194	88	0.01%	0.001%
8	3.293	683	685	687	rBV2	139	48	0.00%	0.000%
9	3.347	700	702	707	rVB	223	157	0.01%	0.001%
10	3.383	709	713	715	rBV2	310	259	0.02%	0.002%
11	3.418	721	724	726	rBV	408	283	0.02%	0.002%
12	3.486	742	745	748	rVB	304	223	0.02%	0.002%
13	3.505	748	751	754	rVB	261	169	0.01%	0.001%
14	3.531	754	759	761	rBV2	390	324	0.02%	0.003%
15	3.544	761	763	764	rBV2	291	102	0.01%	0.001%
16	3.608	778	783	784	rBV	417	340	0.02%	0.003%
17	3.917	867	879	921	rBV2	119707	411197	29.01%	3.598%
18	4.376	1007	1022	1053	rVB	238015	591462	41.72%	5.175%
19	4.666	1109	1112	1114	rBV2	442	303	0.02%	0.003%
20	4.791	1149	1151	1152	rBV2	224	107	0.01%	0.001%
21	4.913	1186	1189	1190	rBV	166	101	0.01%	0.001%
22	4.968	1203	1206	1209	rBV	341	281	0.02%	0.002%
23	5.003	1214	1217	1220	rBV3	509	326	0.02%	0.003%
24	5.074	1220	1239	1261	rBV2	581836	1417615	100.00%	12.403%
25	5.486	1362	1367	1369	rBV3	434	380	0.03%	0.003%
26	5.556	1386	1389	1392	rVB2	365	215	0.02%	0.002%
27	5.640	1403	1415	1443	rBV	380651	755728	53.31%	6.612%
28	5.926	1494	1504	1521	rBV2	44658	89279	6.30%	0.781%
29	6.045	1537	1541	1542	rBV	403	251	0.02%	0.002%
30	6.093	1543	1556	1583	rVV	305384	619323	43.69%	5.419%
31	6.537	1691	1694	1699	rBV4	771	539	0.04%	0.005%
32	6.576	1704	1706	1708	rBV2	269	117	0.01%	0.001%
33	6.592	1708	1711	1712	rVV2	439	144	0.01%	0.001%
34	6.624	1720	1721	1723	rBV	47	19	0.00%	0.000%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102120\
 Data File : VV019053.D
 Acq On : 21 Oct 2020 16:56
 Operator : SY/MD
 Sample : L4483-03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FH1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
 Title : VOC Analysis

35	6.643	1723	1727	1730	rBV2	577	474	0.03%	0.004%
36	6.669	1731	1735	1738	rBV4	483	422	0.03%	0.004%
37	6.717	1748	1750	1752	rBV4	209	88	0.01%	0.001%
38	6.752	1757	1761	1765	rBV3	949	841	0.06%	0.007%
39	6.907	1806	1809	1812	rBV2	614	438	0.03%	0.004%
40	7.006	1829	1840	1871	rBV	186085	340296	24.00%	2.977%
41	7.338	1931	1943	1972	rBV	682510	1183010	83.45%	10.351%
42	7.643	2028	2038	2062	rBV	133940	234639	16.55%	2.053%
43	8.109	2173	2183	2218	rBV2	335702	691346	48.77%	6.049%
44	8.714	2369	2371	2372	rBV	329	134	0.01%	0.001%
45	8.871	2409	2420	2451	rBV	649446	1098555	77.49%	9.612%
46	9.164	2508	2511	2514	rBV3	657	420	0.03%	0.004%
47	9.662	2664	2666	2669	rBV	297	148	0.01%	0.001%
48	10.006	2771	2773	2778	rBV	470	348	0.02%	0.003%
49	10.029	2778	2780	2784	rBV3	396	254	0.02%	0.002%
50	10.238	2833	2845	2864	rBV	349086	555892	39.21%	4.864%
51	10.530	2934	2936	2939	rBV2	556	253	0.02%	0.002%
52	11.209	3138	3147	3154	rBV2	7032	10814	0.76%	0.095%
53	11.270	3155	3166	3190	rVV	623385	981982	69.27%	8.592%
54	11.646	3271	3283	3307	rBV2	706750	1356700	95.70%	11.870%
55	12.019	3397	3399	3402	rBV4	332	156	0.01%	0.001%
56	12.244	3466	3469	3471	rBV2	229	170	0.01%	0.001%
57	12.283	3478	3481	3484	rBV2	298	240	0.02%	0.002%
58	12.354	3501	3503	3506	rBV	322	207	0.01%	0.002%
59	12.382	3510	3512	3515	rBV	288	157	0.01%	0.001%
60	12.402	3516	3518	3520	rVB2	306	107	0.01%	0.001%
61	12.415	3520	3522	3524	rBV	114	52	0.00%	0.000%
62	12.427	3524	3526	3528	rBV	229	135	0.01%	0.001%
63	12.501	3546	3549	3554	rVB2	279	231	0.02%	0.002%
64	12.524	3554	3556	3562	rBV2	262	245	0.02%	0.002%
65	12.591	3574	3577	3580	rBV	290	266	0.02%	0.002%
66	12.669	3594	3601	3611	rBV4	3252	6202	0.44%	0.054%
67	12.743	3620	3624	3627	rBV2	449	314	0.02%	0.003%
68	12.759	3627	3629	3630	rVV	169	73	0.01%	0.001%
69	12.778	3633	3635	3638	rVV2	339	188	0.01%	0.002%
70	12.820	3645	3648	3651	rBV2	248	180	0.01%	0.002%
71	12.884	3666	3668	3672	rVB2	306	229	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102120\
 Data File : VV019053.D
 Acq On : 21 Oct 2020 16:56
 Operator : SY/MD
 Sample : L4483-03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FH1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
 Title : VOC Analysis

72	12.907	3672	3675	3677	rBV	241	165	0.01%	0.001%
73	12.968	3691	3694	3697	rVB2	256	138	0.01%	0.001%
74	13.148	3747	3750	3751	rBV2	227	117	0.01%	0.001%
75	13.244	3777	3780	3783	rBV2	301	182	0.01%	0.002%
76	13.286	3783	3793	3808	rVV	32486	51025	3.60%	0.446%
77	13.437	3835	3840	3842	rBV2	470	448	0.03%	0.004%
78	13.501	3858	3860	3864	rBV	184	104	0.01%	0.001%
79	13.582	3880	3885	3889	rBV	370	410	0.03%	0.004%
80	13.604	3890	3892	3894	rVB	332	135	0.01%	0.001%
81	13.768	3933	3943	3958	rBV	28365	43632	3.08%	0.382%
82	13.871	3973	3975	3977	rBV2	229	110	0.01%	0.001%
83	13.887	3979	3980	3982	rVV	311	118	0.01%	0.001%
84	13.942	3995	3997	3999	rBV2	431	212	0.01%	0.002%
85	14.038	4022	4027	4028	rBV2	447	325	0.02%	0.003%
86	14.199	4065	4077	4084	rBV5	831	1987	0.14%	0.017%
87	14.251	4091	4093	4095	rBV2	303	135	0.01%	0.001%
88	14.267	4095	4098	4102	rBV3	438	272	0.02%	0.002%
89	14.318	4111	4114	4116	rBV	366	275	0.02%	0.002%
90	14.607	4201	4204	4207	rBV	392	266	0.02%	0.002%


Sum of corrected areas: 11429289

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV102120\
Data File : VV019053.D
Acq On : 21 Oct 2020 16:56
Operator : SY/MD
Sample : L4483-03
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FH1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

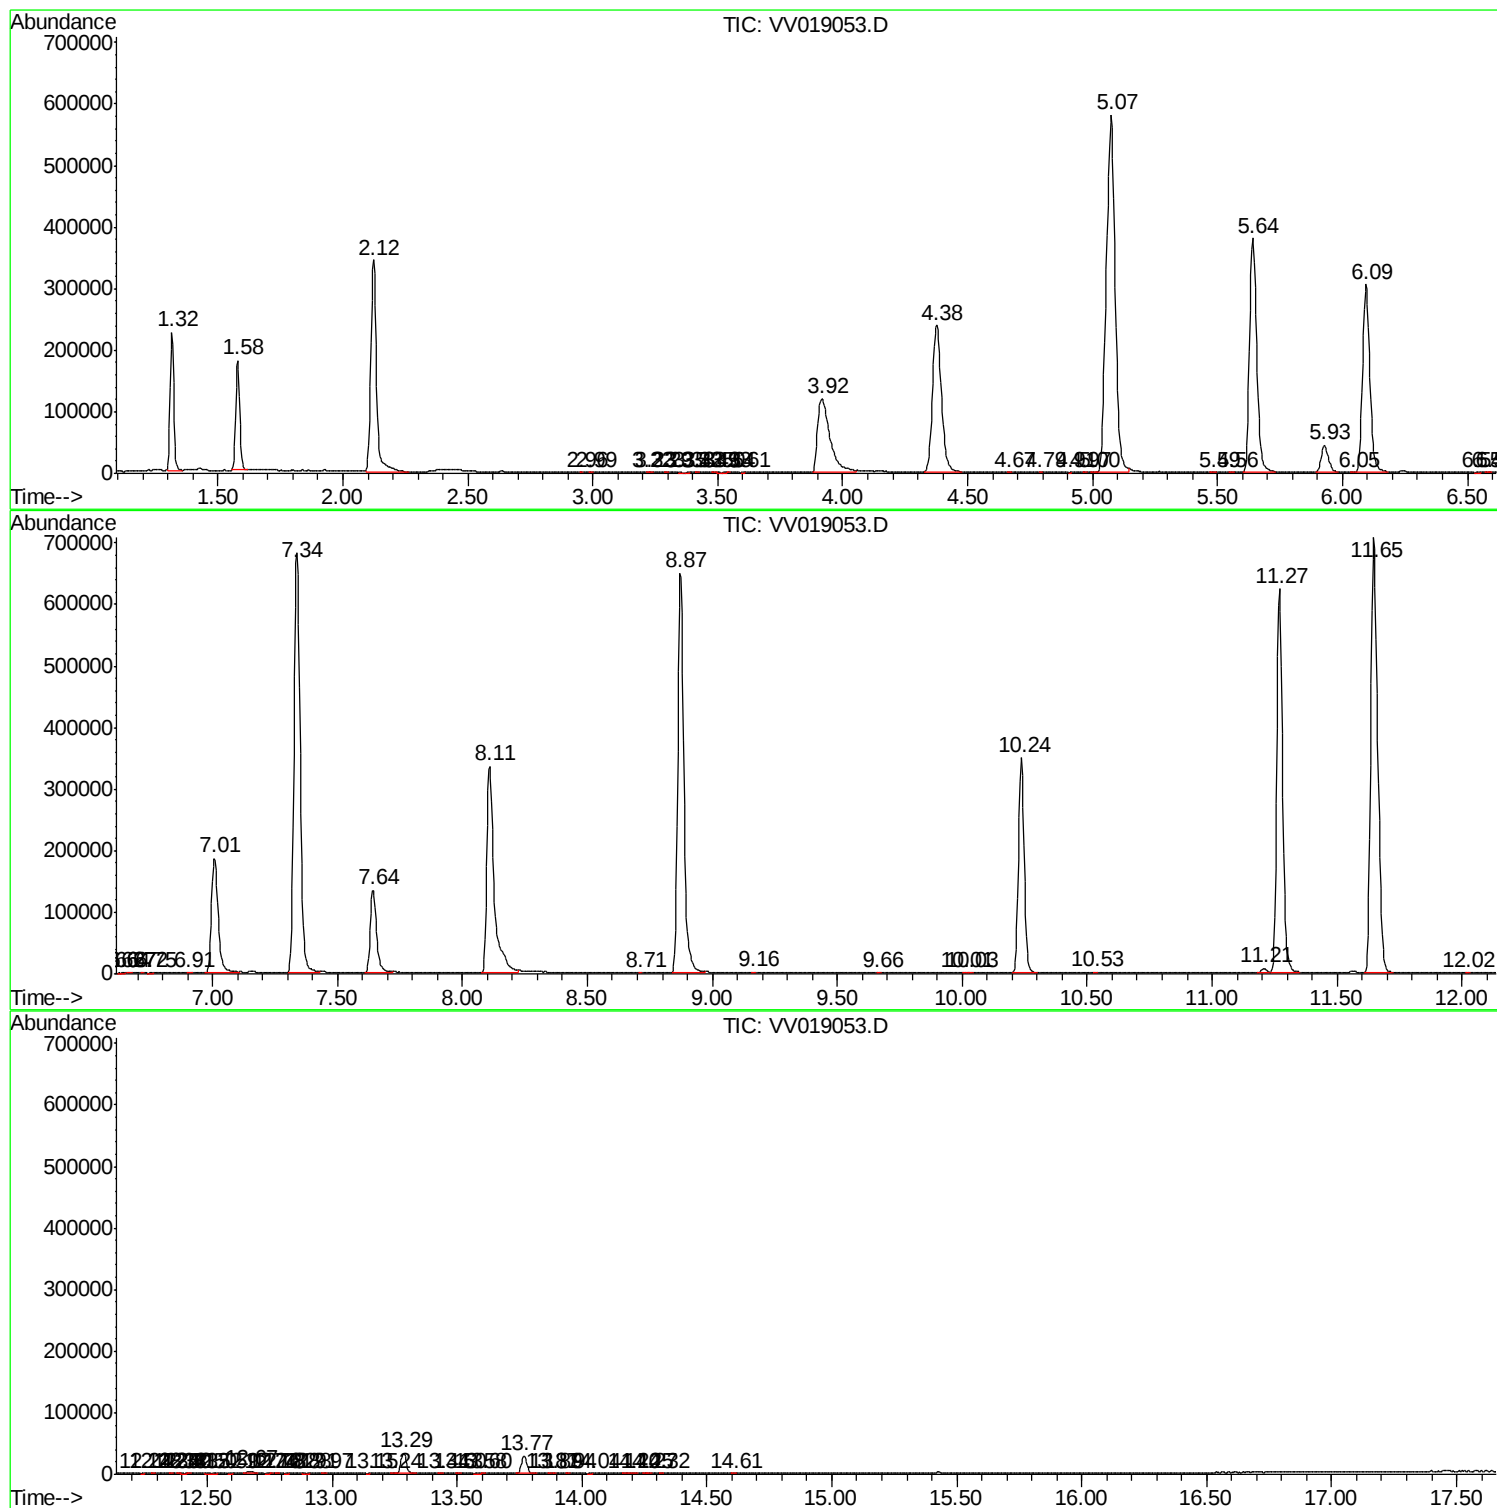

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV102120\
Data File : VV019053.D
Acq On : 21 Oct 2020 16:56
Operator : SY/MD
Sample : L4483-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FH1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV102120\
Data File : VV019053.D
Acq On : 21 Oct 2020 16:56
Operator : SY/MD
Sample : L4483-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FH1

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc