

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102120\
 Data File : VV019057.D
 Acq On : 21 Oct 2020 18:31
 Operator : SY/MD
 Sample : L4483-05DL 500X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FH3DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	85	rVB	210789	213248	13.01%	1.813%
2	1.579	144	152	166	rVB	166766	188549	11.51%	1.603%
3	2.122	309	321	356	rVB	355329	550529	33.60%	4.680%
4	2.489	431	435	438	rBV2	691	646	0.04%	0.005%
5	2.695	495	499	503	rVB2	524	471	0.03%	0.004%
6	2.772	520	523	531	rVB2	314	326	0.02%	0.003%
7	2.843	539	545	548	rBV2	209	228	0.01%	0.002%
8	3.103	623	626	632	rVB2	469	368	0.02%	0.003%
9	3.187	649	652	656	rVB2	367	312	0.02%	0.003%
10	3.212	656	660	664	rBV	270	269	0.02%	0.002%
11	3.399	714	718	722	rBV2	337	272	0.02%	0.002%
12	3.518	751	755	758	rVB3	394	281	0.02%	0.002%
13	3.672	799	803	807	rBV	313	196	0.01%	0.002%
14	3.698	807	811	818	rVB	283	309	0.02%	0.003%
15	3.733	818	822	828	rVB2	316	394	0.02%	0.003%
16	3.910	863	877	899	rBV	89964	249110	15.20%	2.118%
17	4.203	964	968	976	rVB3	589	818	0.05%	0.007%
18	4.312	999	1002	1005	rVB	506	308	0.02%	0.003%
19	4.376	1005	1022	1051	rBV	195025	489443	29.87%	4.161%
20	4.585	1083	1087	1096	rBV4	385	570	0.03%	0.005%
21	4.650	1103	1107	1109	rBV4	589	434	0.03%	0.004%
22	4.817	1157	1159	1163	rVB	406	244	0.01%	0.002%
23	4.849	1163	1169	1173	rBV4	615	595	0.04%	0.005%
24	4.933	1190	1195	1196	rBV2	366	276	0.02%	0.002%
25	4.955	1199	1202	1207	rVB2	333	253	0.02%	0.002%
26	4.987	1208	1212	1215	rBV3	330	362	0.02%	0.003%
27	5.071	1220	1238	1283	rBV3	475188	1387090	84.65%	11.791%
28	5.370	1329	1331	1337	rVB2	456	365	0.02%	0.003%
29	5.431	1346	1350	1353	rVB2	504	466	0.03%	0.004%
30	5.470	1360	1362	1369	rVB3	527	406	0.02%	0.003%
31	5.531	1377	1381	1383	rBV2	239	193	0.01%	0.002%
32	5.592	1395	1400	1403	rVB3	235	224	0.01%	0.002%
33	5.640	1403	1415	1439	rBV	361102	722772	44.11%	6.144%
34	5.801	1463	1465	1469	rBV2	462	320	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102120\
 Data File : VV019057.D
 Acq On : 21 Oct 2020 18:31
 Operator : SY/MD
 Sample : L4483-05DL 500X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FH3DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
 Title : VOC Analysis

35	5.852	1478	1481	1484	rVV3	408	314	0.02%	0.003%
36	5.875	1486	1488	1490	rVV2	393	202	0.01%	0.002%
37	5.926	1493	1504	1522	rVV	38787	81203	4.96%	0.690%
38	6.093	1540	1556	1584	rBV	333269	676170	41.27%	5.748%
39	6.286	1613	1616	1617	rBV2	566	257	0.02%	0.002%
40	6.421	1656	1658	1660	rBV	404	240	0.01%	0.002%
41	6.611	1715	1717	1720	rBV2	323	196	0.01%	0.002%
42	6.772	1764	1767	1769	rBV	276	208	0.01%	0.002%
43	6.842	1786	1789	1792	rBV	425	282	0.02%	0.002%
44	6.936	1816	1818	1823	rBV2	571	483	0.03%	0.004%
45	7.006	1828	1840	1863	rBV	176621	322727	19.70%	2.743%
46	7.251	1914	1916	1919	rBV2	518	329	0.02%	0.003%
47	7.338	1930	1943	1963	rBV	657619	1125981	68.72%	9.572%
48	7.559	2009	2012	2015	rVB3	649	426	0.03%	0.004%
49	7.643	2026	2038	2058	rBV	127822	226553	13.83%	1.926%
50	7.859	2104	2105	2109	rBV2	336	230	0.01%	0.002%
51	8.003	2144	2150	2157	rBV4	1576	1880	0.11%	0.016%
52	8.109	2171	2183	2216	rBV2	338456	673530	41.11%	5.725%
53	8.489	2298	2301	2302	rBV2	471	311	0.02%	0.003%
54	8.576	2323	2328	2330	rBV4	523	522	0.03%	0.004%
55	8.678	2355	2360	2362	rBV2	487	424	0.03%	0.004%
56	8.788	2391	2394	2395	rBV	313	212	0.01%	0.002%
57	8.807	2398	2400	2406	rVB4	736	592	0.04%	0.005%
58	8.875	2409	2421	2425	rBV	677337	1058521	64.60%	8.998%
59	9.080	2479	2485	2488	rBV4	650	772	0.05%	0.007%
60	9.231	2529	2532	2534	rBV3	335	204	0.01%	0.002%
61	9.354	2568	2570	2573	rVB3	436	188	0.01%	0.002%
62	9.669	2665	2668	2670	rBV	500	283	0.02%	0.002%
63	9.714	2679	2682	2687	rBV3	378	457	0.03%	0.004%
64	9.862	2724	2728	2729	rBV	525	311	0.02%	0.003%
65	10.045	2783	2785	2789	rBV2	257	193	0.01%	0.002%
66	10.151	2814	2818	2819	rBV2	303	248	0.02%	0.002%
67	10.238	2830	2845	2867	rBV	364326	578849	35.33%	4.921%
68	10.608	2957	2960	2962	rBV3	664	427	0.03%	0.004%
69	10.936	3059	3062	3064	rVB	476	263	0.02%	0.002%
70	11.051	3096	3098	3106	rVB4	419	443	0.03%	0.004%
71	11.206	3137	3146	3155	rBV3	30552	49436	3.02%	0.420%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102120\
 Data File : VV019057.D
 Acq On : 21 Oct 2020 18:31
 Operator : SY/MD
 Sample : L4483-05DL 500X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FH3DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
 Title : VOC Analysis

72	11.270	3155	3166	3200	rVB2	666121	1404218	85.70%	11.937%
73	11.511	3238	3241	3244	rBV2	440	271	0.02%	0.002%
74	11.595	3265	3267	3269	rBV2	451	192	0.01%	0.002%
75	11.649	3270	3284	3308	rVV3	779631	1638552	100.00%	13.929%
76	11.800	3328	3331	3334	rBV3	679	523	0.03%	0.004%
77	12.318	3490	3492	3495	rBV3	344	228	0.01%	0.002%
78	12.379	3508	3511	3513	rBV	473	262	0.02%	0.002%
79	12.405	3517	3519	3525	rBV2	464	363	0.02%	0.003%
80	12.434	3526	3528	3530	rBV3	393	220	0.01%	0.002%
81	12.627	3586	3588	3591	rBV4	360	233	0.01%	0.002%
82	13.286	3782	3793	3812	rBV	50231	80390	4.91%	0.683%
83	13.443	3839	3842	3844	rBV2	471	322	0.02%	0.003%
84	13.485	3853	3855	3860	rBV	394	360	0.02%	0.003%
85	13.665	3908	3911	3916	rBV3	568	530	0.03%	0.005%
86	13.771	3934	3944	3957	rBV5	11238	17734	1.08%	0.151%
87	13.823	3957	3960	3962	rBV3	602	367	0.02%	0.003%
88	14.148	4059	4061	4067	rBV2	549	498	0.03%	0.004%
89	14.360	4124	4127	4133	rBV4	531	508	0.03%	0.004%
90	14.556	4186	4188	4190	rBV2	413	208	0.01%	0.002%
91	14.652	4216	4218	4220	rBV	393	202	0.01%	0.002%
92	14.996	4323	4325	4328	rVB	384	188	0.01%	0.002%
93	15.058	4341	4344	4350	rBV3	315	275	0.02%	0.002%
94	15.382	4443	4445	4449	rBV2	339	222	0.01%	0.002%
95	15.582	4501	4507	4510	rBV4	586	606	0.04%	0.005%
96	15.739	4553	4556	4561	rVB3	566	443	0.03%	0.004%
97	15.765	4561	4564	4568	rBV4	399	361	0.02%	0.003%
98	15.964	4624	4626	4628	rBV2	492	193	0.01%	0.002%
99	15.977	4628	4630	4634	rBV	483	356	0.02%	0.003%
100	16.083	4660	4663	4665	rBV3	698	430	0.03%	0.004%


Sum of corrected areas: 11763769

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV102120\
Data File : VV019057.D
Acq On : 21 Oct 2020 18:31
Operator : SY/MD
Sample : L4483-05DL 500X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
C0FH3DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

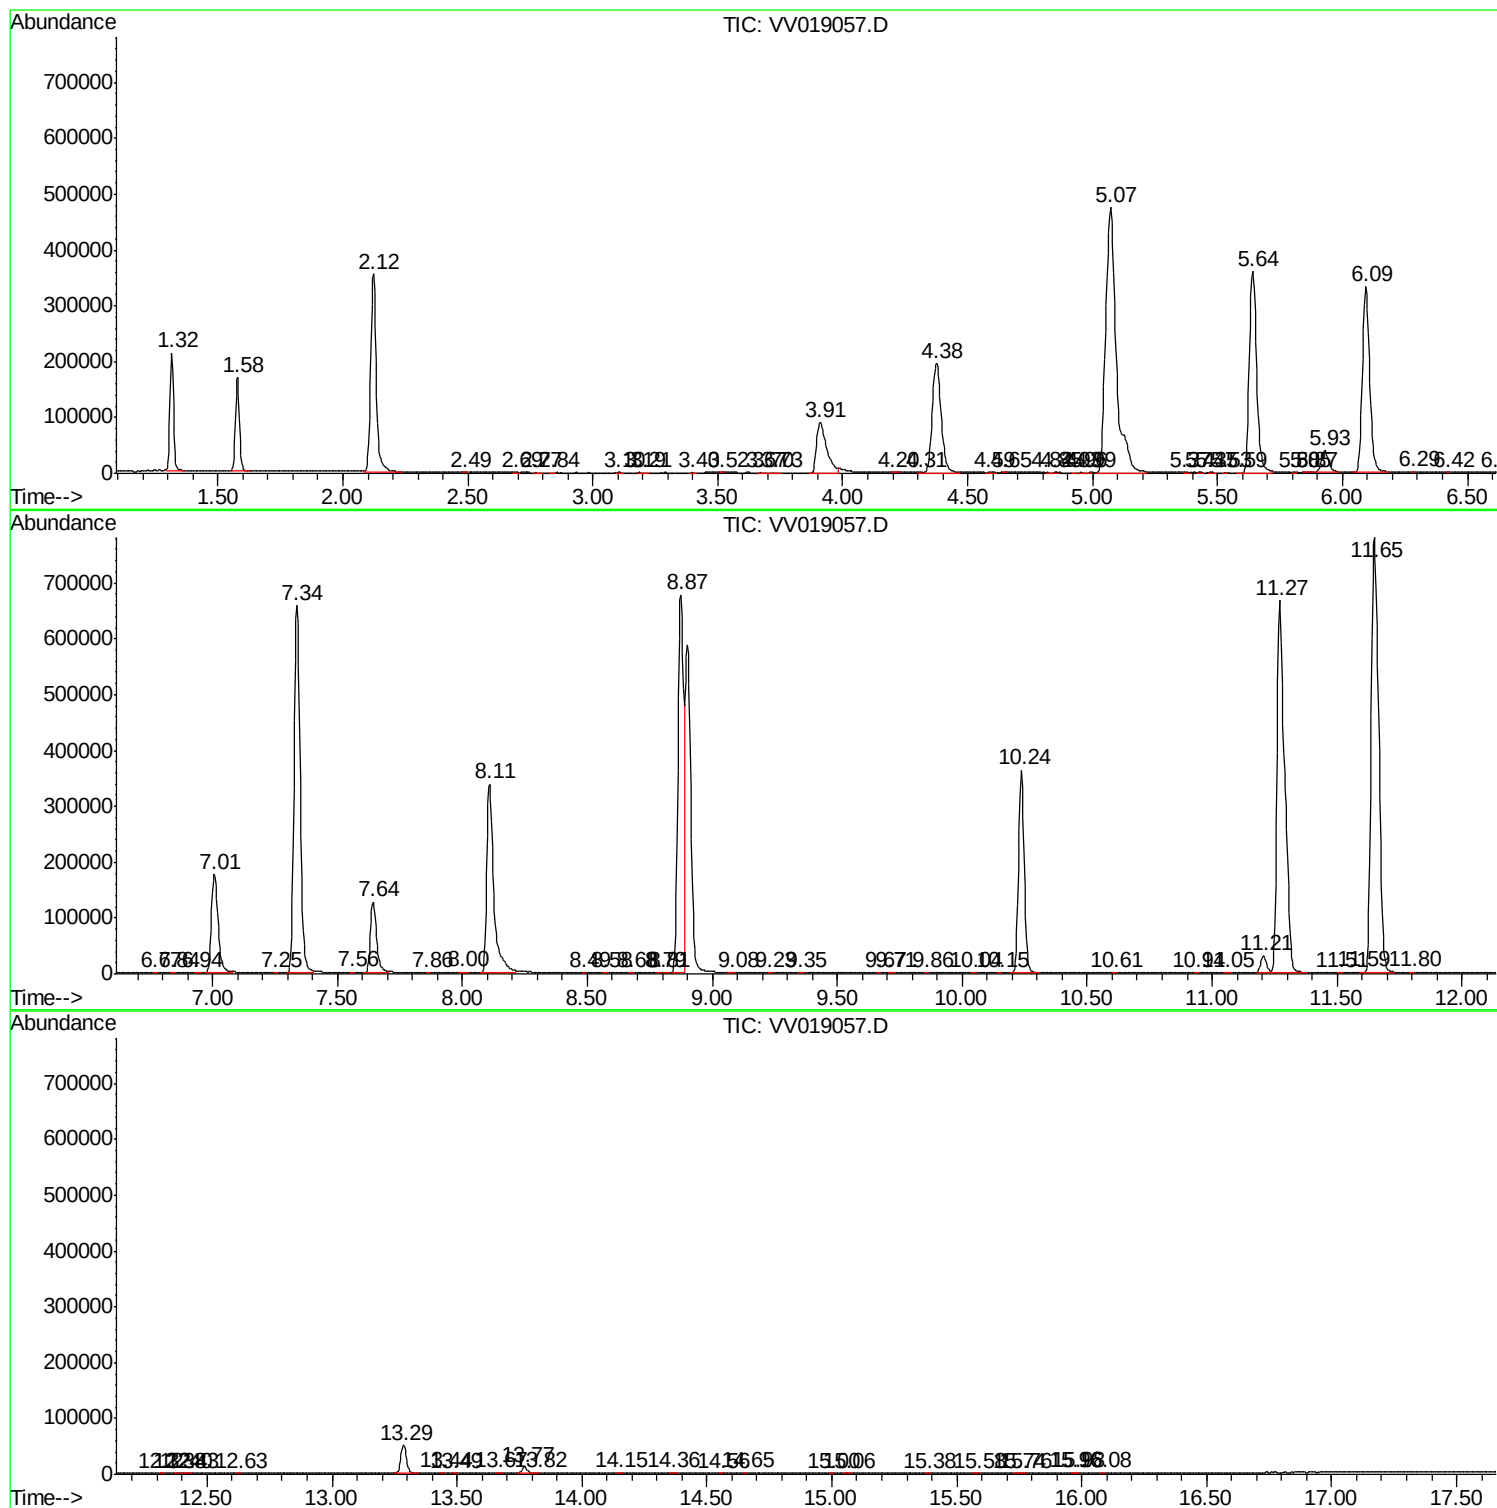

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV102120\
Data File : VV019057.D
Acq On : 21 Oct 2020 18:31
Operator : SY/MD
Sample : L4483-05DL 500X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FH3DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV102120\
Data File : VV019057.D
Acq On : 21 Oct 2020 18:31
Operator : SY/MD
Sample : L4483-05DL 500X
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
C0FH3DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM101420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc