

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102120\
 Data File : VV019060.D
 Acq On : 21 Oct 2020 19:42
 Operator : SY/MD
 Sample : L4483-05 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FH3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	82	rVB	206839	204914	16.68%	2.103%
2	1.579	145	152	168	rVB	178655	196211	15.97%	2.013%
3	2.122	311	321	351	rVB	317293	488876	39.79%	5.016%
4	2.917	565	568	569	rBV	350	225	0.02%	0.002%
5	3.283	677	682	685	rBV3	453	530	0.04%	0.005%
6	3.344	698	701	703	rBV2	343	240	0.02%	0.002%
7	3.913	867	878	911	rBV2	92689	285195	23.21%	2.926%
8	4.376	1005	1022	1053	rBV	194845	488421	39.75%	5.012%
9	4.582	1084	1086	1089	rBV	260	113	0.01%	0.001%
10	4.669	1111	1113	1115	rBV2	278	179	0.01%	0.002%
11	4.769	1141	1144	1146	rBV	331	215	0.02%	0.002%
12	4.781	1146	1148	1149	rVV	149	43	0.00%	0.000%
13	4.923	1190	1192	1195	rVB	192	73	0.01%	0.001%
14	4.942	1195	1198	1200	rBV	234	137	0.01%	0.001%
15	4.971	1203	1207	1210	rBV2	276	250	0.02%	0.003%
16	5.071	1221	1238	1267	rBV2	474347	1228714	100.00%	12.608%
17	5.392	1336	1338	1341	rVB2	411	176	0.01%	0.002%
18	5.424	1346	1348	1353	rVB2	519	397	0.03%	0.004%
19	5.489	1365	1368	1372	rVB	483	448	0.04%	0.005%
20	5.515	1372	1376	1381	rBV3	658	705	0.06%	0.007%
21	5.559	1386	1390	1391	rBV3	169	66	0.01%	0.001%
22	5.592	1397	1400	1402	rBV2	273	176	0.01%	0.002%
23	5.640	1403	1415	1441	rBV	360494	716560	58.32%	7.353%
24	5.926	1494	1504	1524	rBV	39656	80746	6.57%	0.829%
25	6.093	1543	1556	1588	rBV	296163	601107	48.92%	6.168%
26	6.315	1623	1625	1628	rBV3	375	166	0.01%	0.002%
27	6.344	1629	1634	1637	rVV3	630	620	0.05%	0.006%
28	6.415	1655	1656	1659	rBV2	341	147	0.01%	0.002%
29	6.839	1786	1788	1791	rBV2	354	151	0.01%	0.002%
30	7.006	1829	1840	1864	rBV	180010	331750	27.00%	3.404%
31	7.338	1931	1943	1983	rBV	665225	1156676	94.14%	11.869%
32	7.640	2028	2037	2066	rBV	125492	220548	17.95%	2.263%
33	7.910	2119	2121	2124	rVB2	604	370	0.03%	0.004%
34	7.942	2128	2131	2133	rBV	559	302	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102120\
 Data File : VV019060.D
 Acq On : 21 Oct 2020 19:42
 Operator : SY/MD
 Sample : L4483-05 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FH3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
 Title : VOC Analysis

35	7.994	2144	2147	2150	rBV3	956	721	0.06%	0.007%
36	8.106	2172	2182	2225	rBV2	290236	596452	48.54%	6.120%
37	8.376	2263	2266	2269	rBV	498	258	0.02%	0.003%
38	8.479	2294	2298	2301	rBV2	412	336	0.03%	0.003%
39	8.527	2310	2313	2315	rBV2	214	171	0.01%	0.002%
40	8.547	2318	2319	2320	rVV2	185	44	0.00%	0.000%
41	8.556	2320	2322	2325	rVB2	306	120	0.01%	0.001%
42	8.582	2328	2330	2332	rBV	170	69	0.01%	0.001%
43	8.604	2335	2337	2338	rBV	302	123	0.01%	0.001%
44	8.730	2373	2376	2380	rBV2	444	345	0.03%	0.004%
45	8.762	2384	2386	2389	rVV	249	146	0.01%	0.001%
46	8.781	2389	2392	2399	rVB3	438	482	0.04%	0.005%
47	8.871	2408	2420	2453	rBV	558291	905501	73.70%	9.291%
48	9.029	2468	2469	2470	rBV	299	92	0.01%	0.001%
49	9.132	2498	2501	2503	rBV	274	158	0.01%	0.002%
50	9.183	2515	2517	2518	rBV	162	58	0.00%	0.001%
51	9.219	2525	2528	2531	rBV	265	167	0.01%	0.002%
52	9.270	2541	2544	2547	rBV2	241	175	0.01%	0.002%
53	9.476	2605	2608	2613	rBV2	234	240	0.02%	0.002%
54	9.546	2628	2630	2633	rVB	147	78	0.01%	0.001%
55	9.624	2652	2654	2659	rBV2	280	179	0.01%	0.002%
56	9.669	2665	2668	2675	rVB2	367	337	0.03%	0.003%
57	9.694	2675	2676	2678	rBV	113	48	0.00%	0.000%
58	9.720	2678	2684	2691	rBV2	282	394	0.03%	0.004%
59	9.772	2696	2700	2702	rBV2	365	251	0.02%	0.003%
60	9.813	2709	2713	2716	rBV	439	296	0.02%	0.003%
61	9.945	2746	2754	2757	rBV2	393	484	0.04%	0.005%
62	9.981	2762	2765	2768	rVB2	267	168	0.01%	0.002%
63	10.003	2768	2772	2775	rBV	271	197	0.02%	0.002%
64	10.019	2775	2777	2780	rBV	146	105	0.01%	0.001%
65	10.077	2794	2795	2799	rVB	394	146	0.01%	0.001%
66	10.106	2799	2804	2806	rBV2	407	359	0.03%	0.004%
67	10.238	2833	2845	2869	rBV	289668	456844	37.18%	4.688%
68	10.360	2880	2883	2885	rBV	128	94	0.01%	0.001%
69	10.402	2893	2896	2901	rBV	349	283	0.02%	0.003%
70	10.498	2924	2926	2928	rBV	152	93	0.01%	0.001%
71	10.556	2941	2944	2945	rBV	205	125	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102120\
Data File : VV019060.D
Acq On : 21 Oct 2020 19:42
Operator : SY/MD
Sample : L4483-05 100X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FH3

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
Title : VOC Analysis

72	10.723	2993	2996	3001	rVB2	362	275	0.02%	0.003%
73	10.845	3033	3034	3036	rVB2	137	29	0.00%	0.000%
74	10.862	3036	3039	3042	rBV	176	157	0.01%	0.002%
75	10.900	3048	3051	3055	rVB2	557	367	0.03%	0.004%
76	10.948	3063	3066	3069	rBV	344	227	0.02%	0.002%
77	11.167	3130	3134	3135	rBV	250	190	0.02%	0.002%
78	11.199	3141	3144	3147	rBV2	307	189	0.02%	0.002%
79	11.270	3154	3166	3194	rBV	555435	854850	69.57%	8.772%
80	11.646	3271	3283	3310	rBV	593147	917613	74.68%	9.416%


Sum of corrected areas: 9745483

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV102120\
Data File : VV019060.D
Acq On : 21 Oct 2020 19:42
Operator : SY/MD
Sample : L4483-05 100X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FH3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

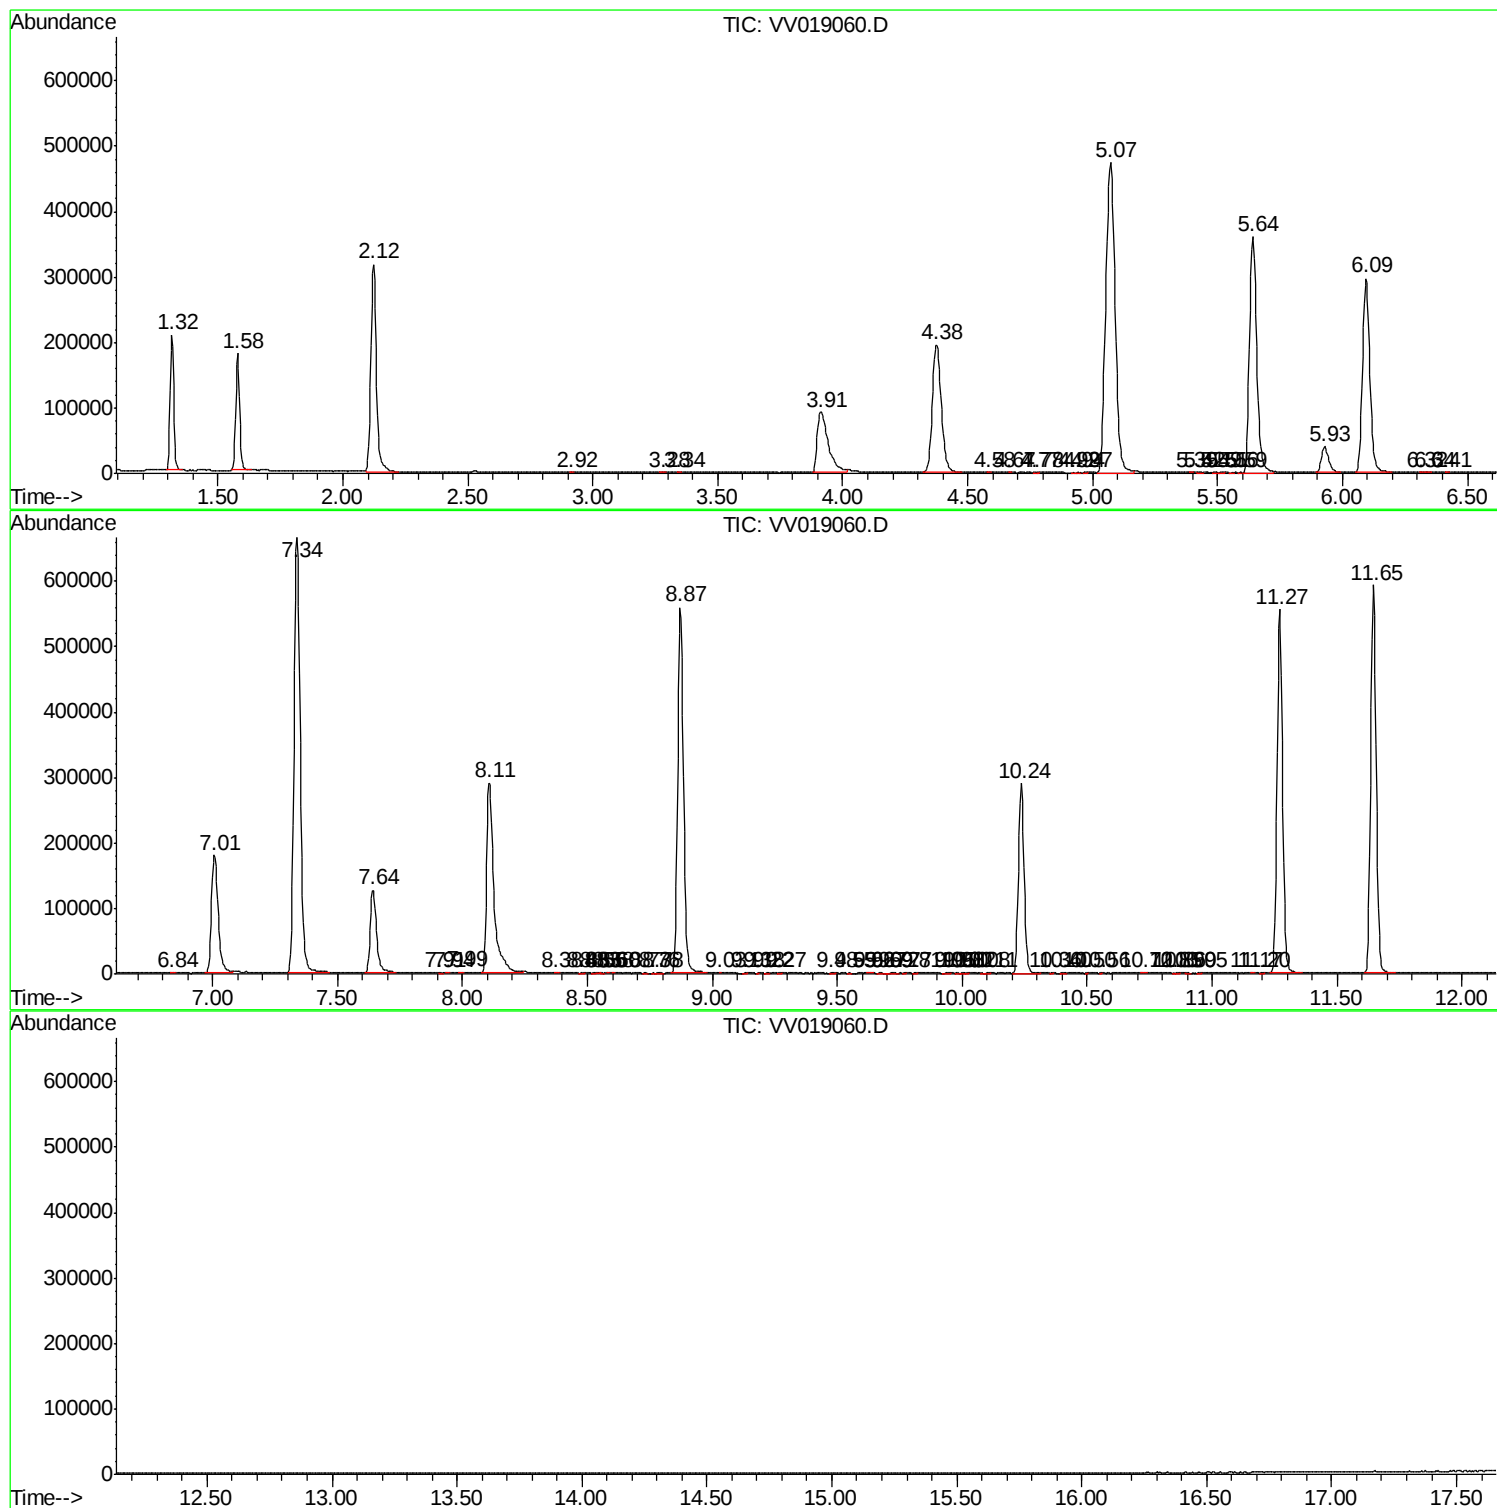

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV102120\
Data File : VV019060.D
Acq On : 21 Oct 2020 19:42
Operator : SY/MD
Sample : L4483-05 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FH3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV102120\
Data File : VV019060.D
Acq On : 21 Oct 2020 19:42
Operator : SY/MD
Sample : L4483-05 100X
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
C0FH3

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM101420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc