


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102121\
Data File : VV022957.D
Acq On : 21 Oct 2021 14:27
Operator : SY/MD
Sample : M4264-03ME
Misc : 3.95g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB7G8ME

Manual Integrations
APPROVED

MMDadoda
10/25/2021 11:49:19 AM

Quant Time: Oct 22 03:53:52 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Oct 22 03:48:35 2021
Response via : Initial Calibration

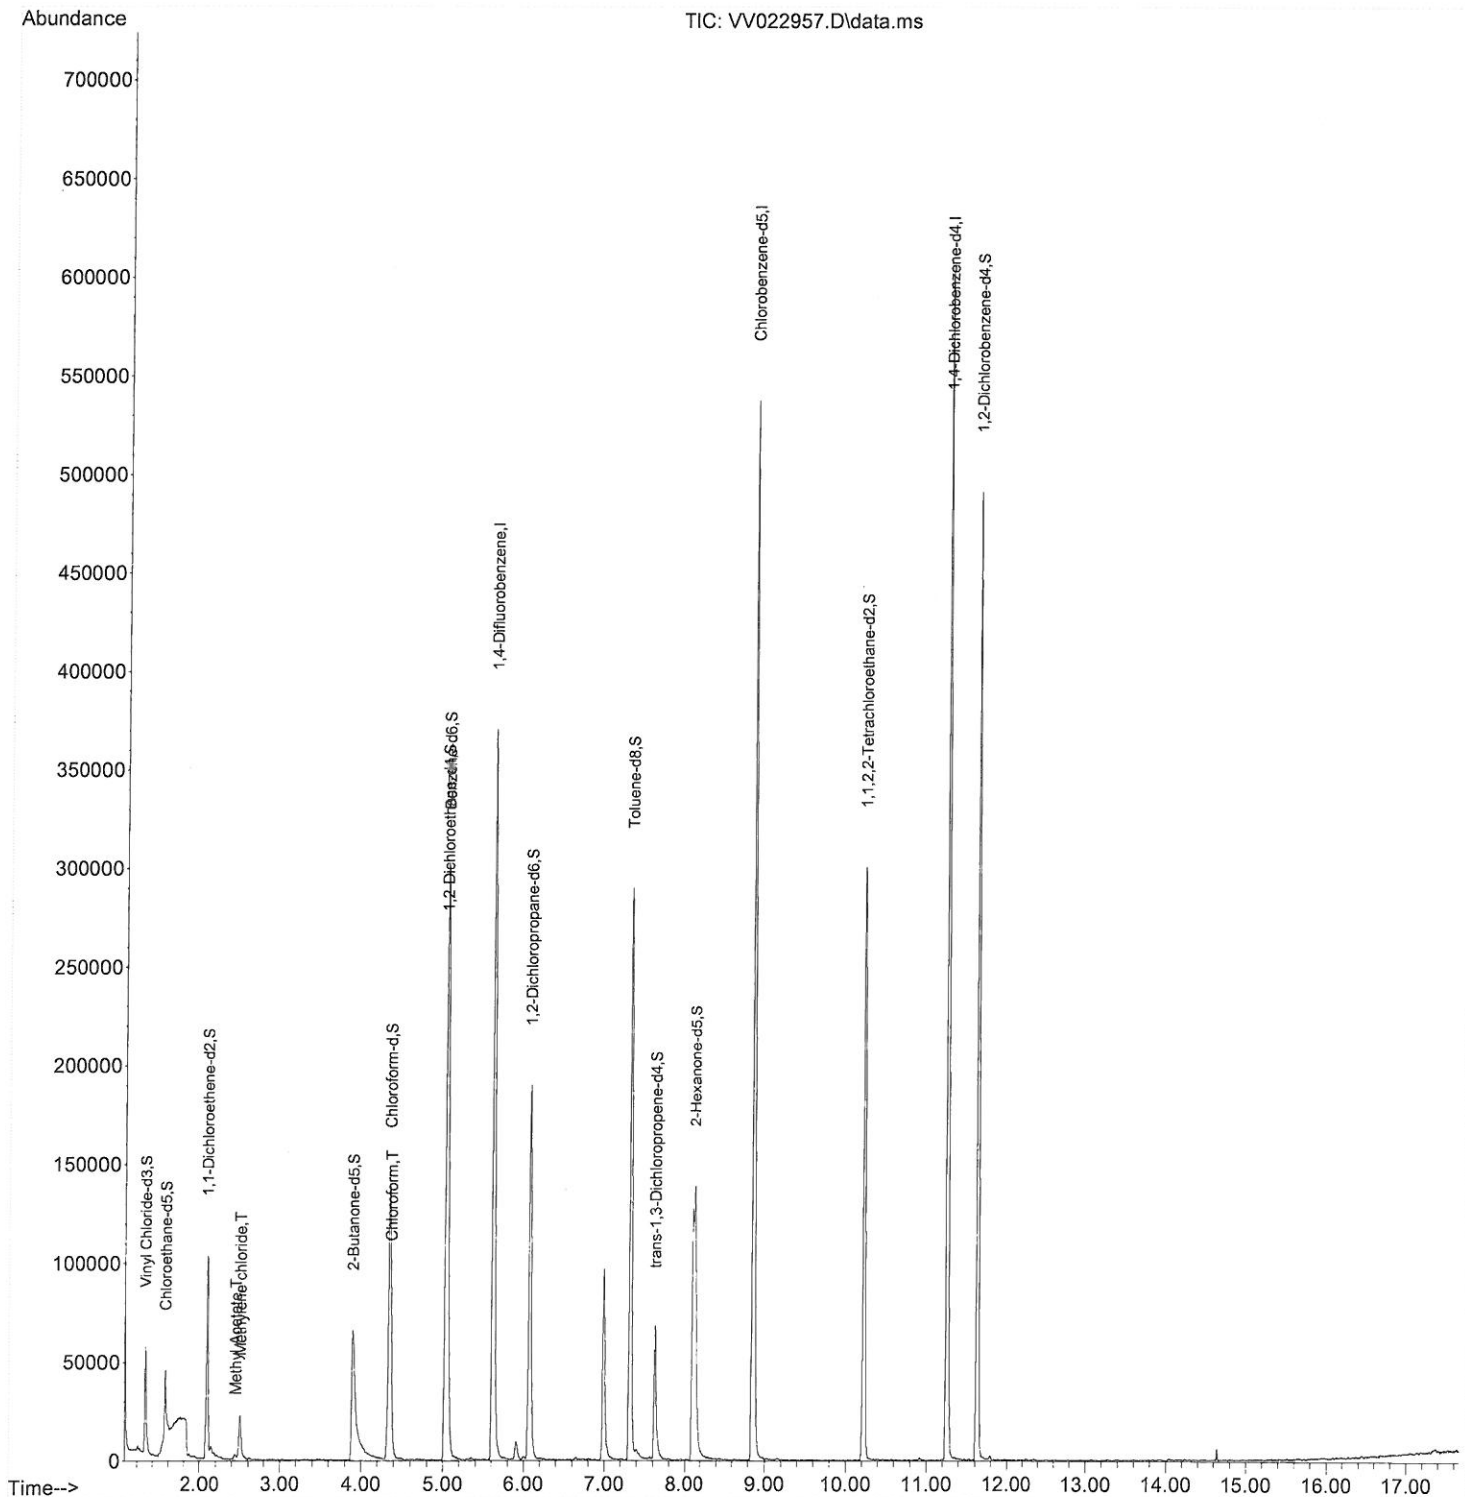

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102121\Not Reviewed Data\
 Data File : VV022957.D
 Acq On : 21 Oct 2021 14:27
 Operator : SY/MD
 Sample : M4264-03ME
 Misc : 3.95g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB7G8ME

Manual Integrations
 APPROVED

MMDadoda
 10/25/2021 11:49:19 AM

Quant Time: Oct 25 11:30:04 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Oct 22 03:48:35 2021
 Response via : Initial Calibration

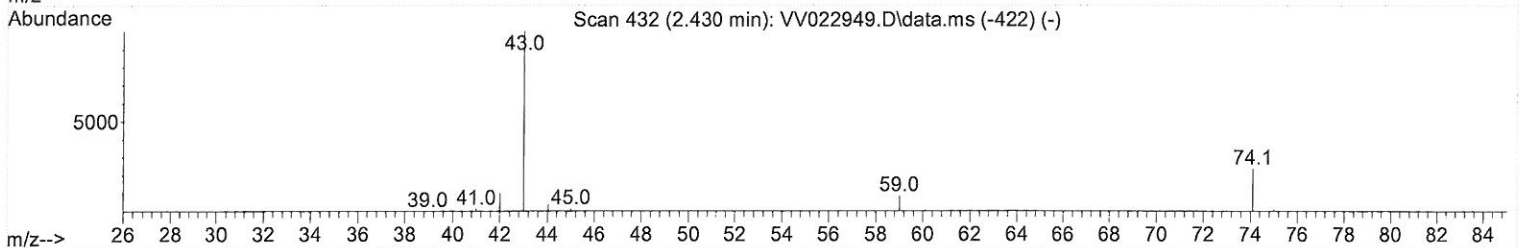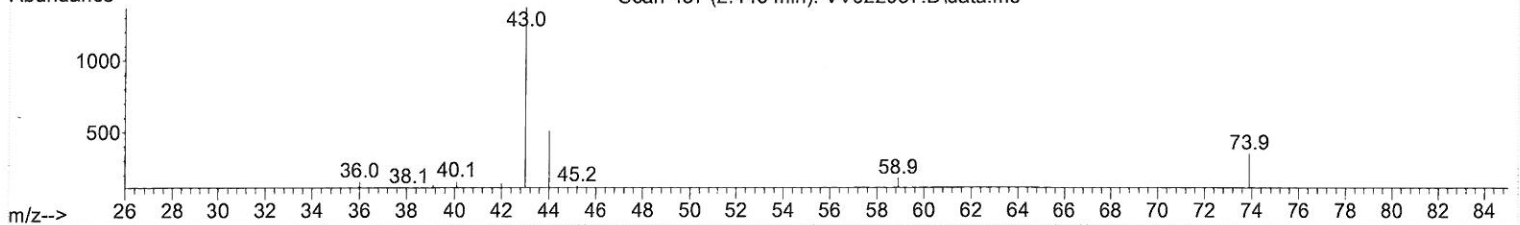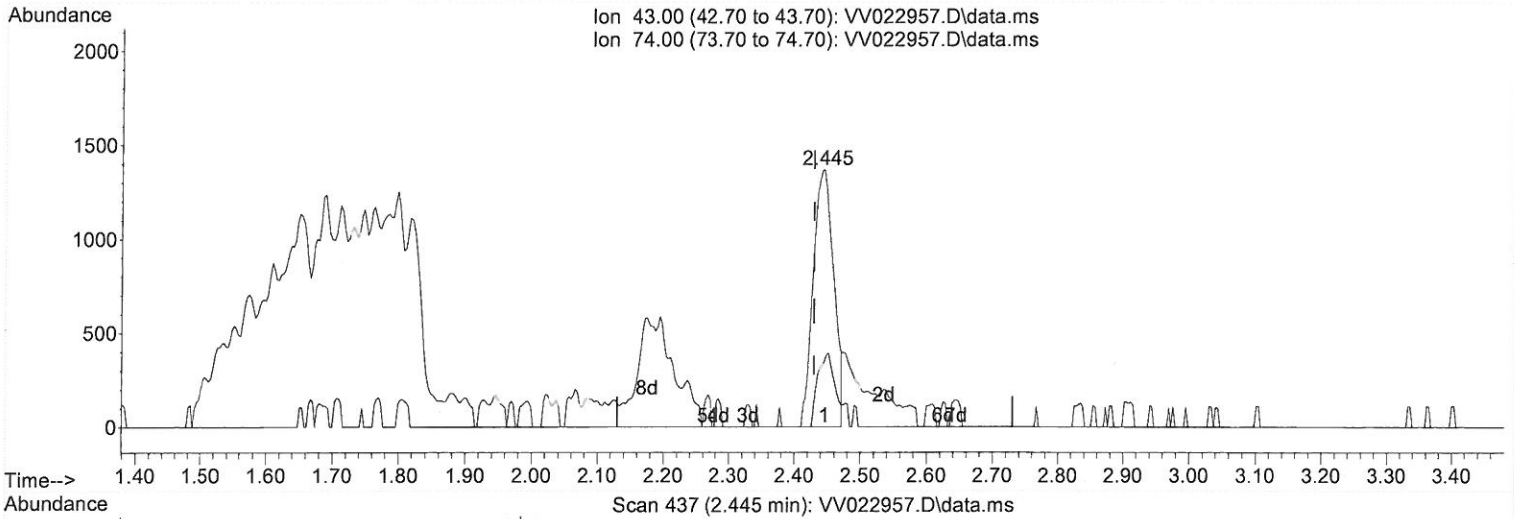

TIC: VV022957.D\data.ms

(15) Methyl Acetate (T)

2.445min (+ 0.016) 1.10 ug/L

response 2944

Ion	Exp%	Act%
43.00	100.00	100.00
74.00	25.70	24.52
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102121\
 Data File : VV022957.D
 Acq On : 21 Oct 2021 14:27
 Operator : SY/MD
 Sample : M4264-03ME
 Misc : 3.95g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB7G8ME

Manual Integrations
 APPROVED

MMDadoda
 10/25/2021 11:49:19 AM

Quant Time: Oct 22 03:53:52 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Oct 22 03:48:35 2021
 Response via : Initial Calibration

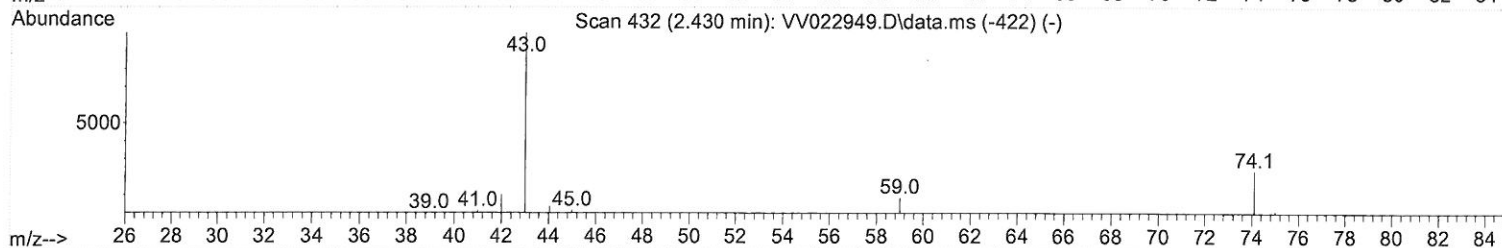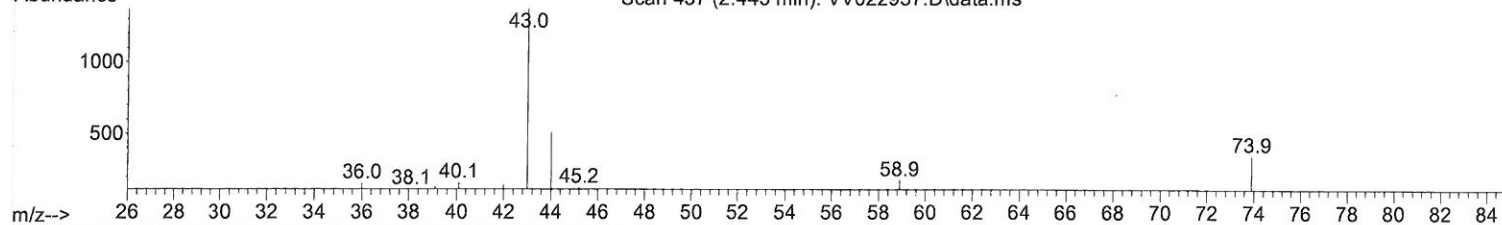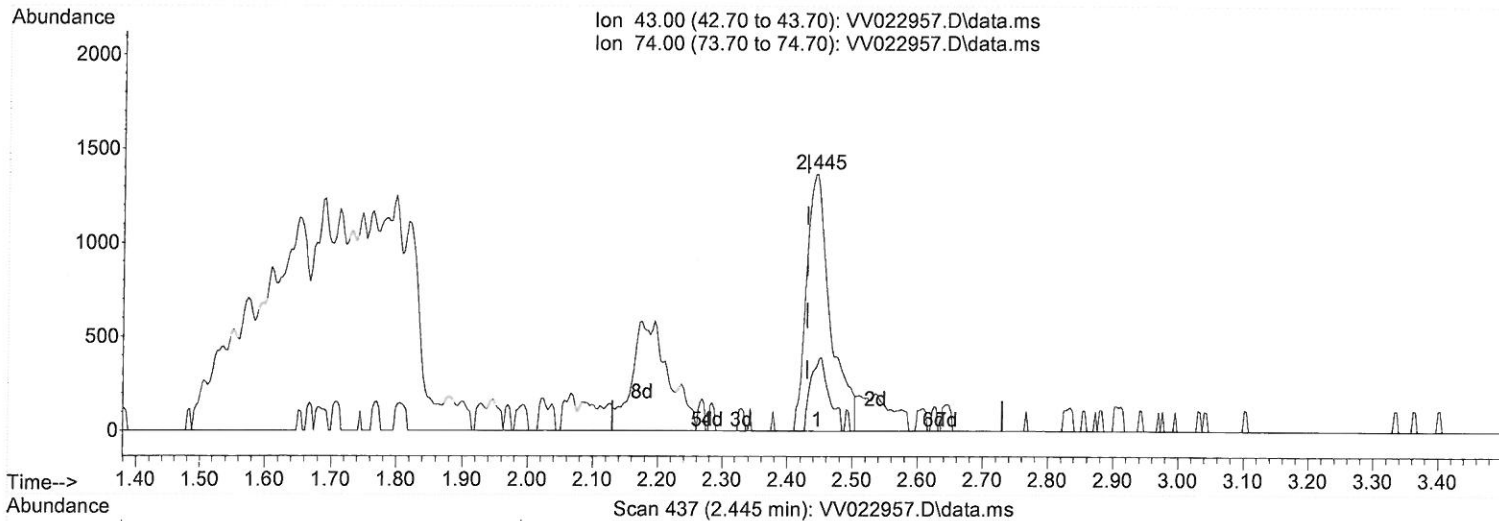

(15) Methyl Acetate (T)

2.445min (+ 0.016) 1.31 ug/L m

response 3499

Ion	Exp%	Act%
43.00	100.00	100.00
74.00	25.70	20.63
0.00	0.00	0.00
0.00	0.00	0.00

MD
 10/26/21

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102121\Not Reviewed Data\
Data File : VV022957.D
Acq On : 21 Oct 2021 14:27
Operator : SY/MD
Sample : M4264-03ME
Misc : 3.95g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB7G8ME

Manual Integrations
APPROVED

MMDadoda
10/25/2021 11:49:19 AM

Quant Time: Oct 25 11:30:04 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Oct 22 03:48:35 2021
Response via : Initial Calibration

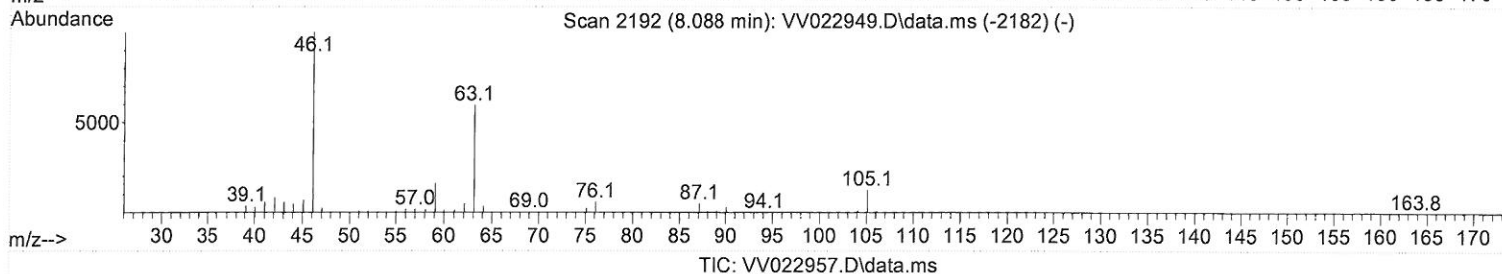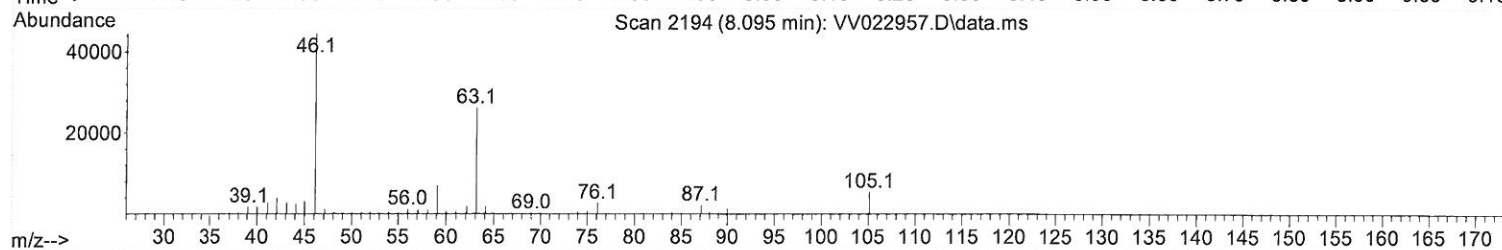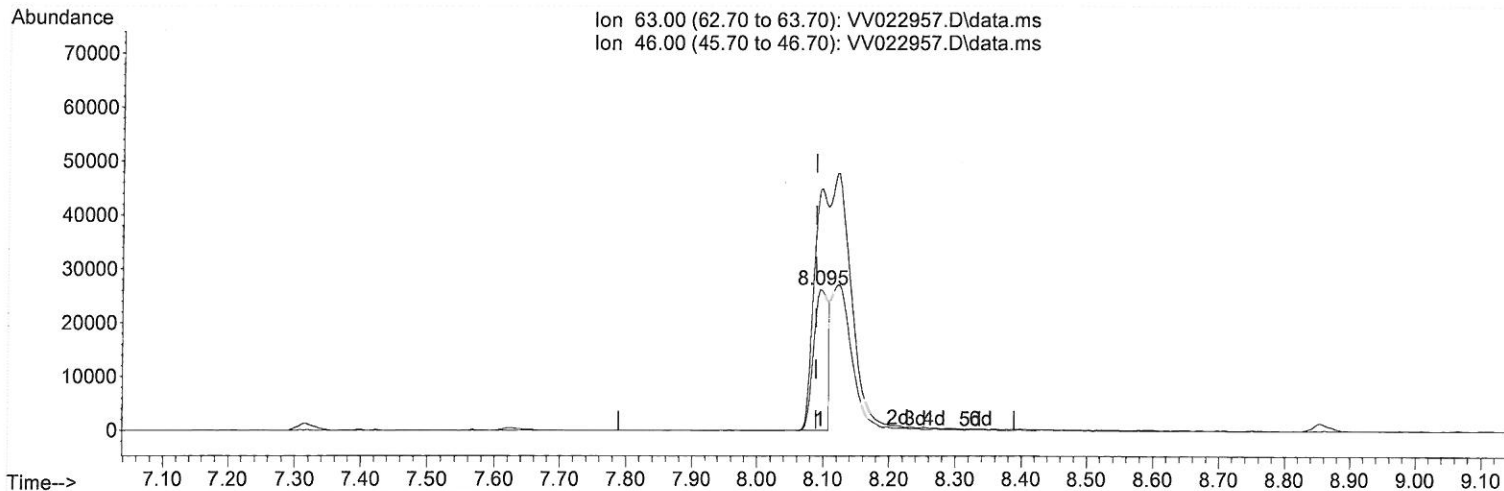

(47) 2-Hexanone-d5 (S)

8.095min (+ 0.006) 40.82 ug/L

response 39854

Ion	Exp%	Act%
63.00	100.00	100.00
46.00	163.00	174.36
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102121\
 Data File : VV022957.D
 Acq On : 21 Oct 2021 14:27
 Operator : SY/MD
 Sample : M4264-03ME
 Misc : 3.95g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB7G8ME

Manual Integrations
 APPROVED

MMDadoda
 10/25/2021 11:49:19 AM

Quant Time: Oct 22 03:53:52 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Oct 22 03:48:35 2021
 Response via : Initial Calibration

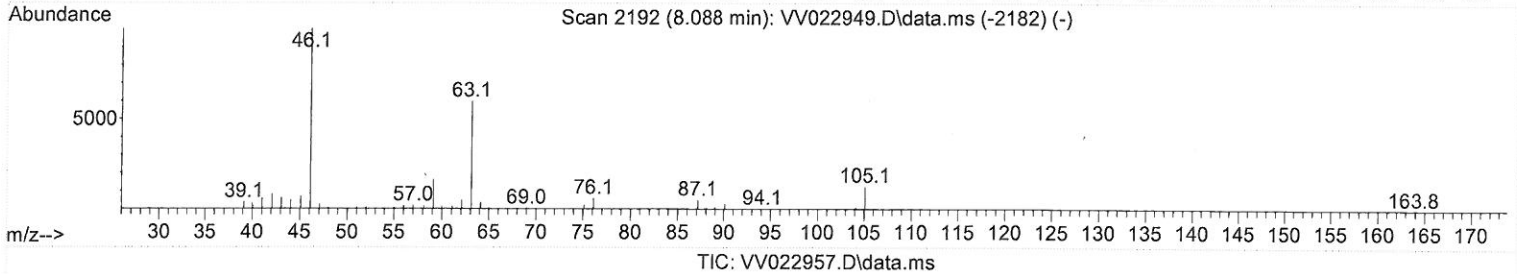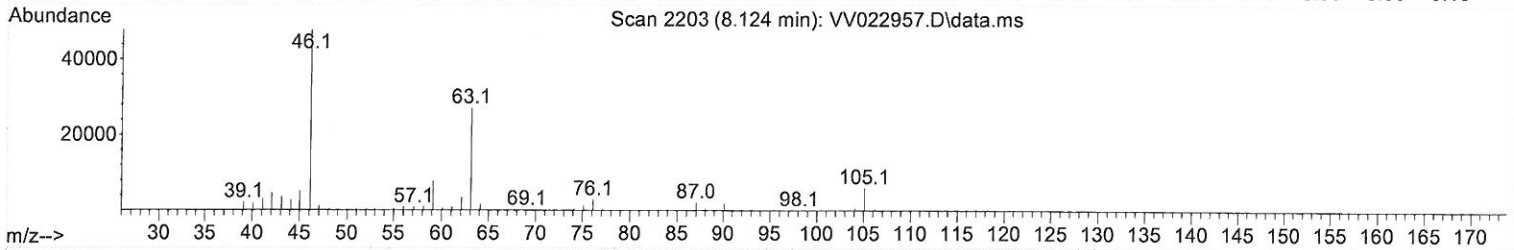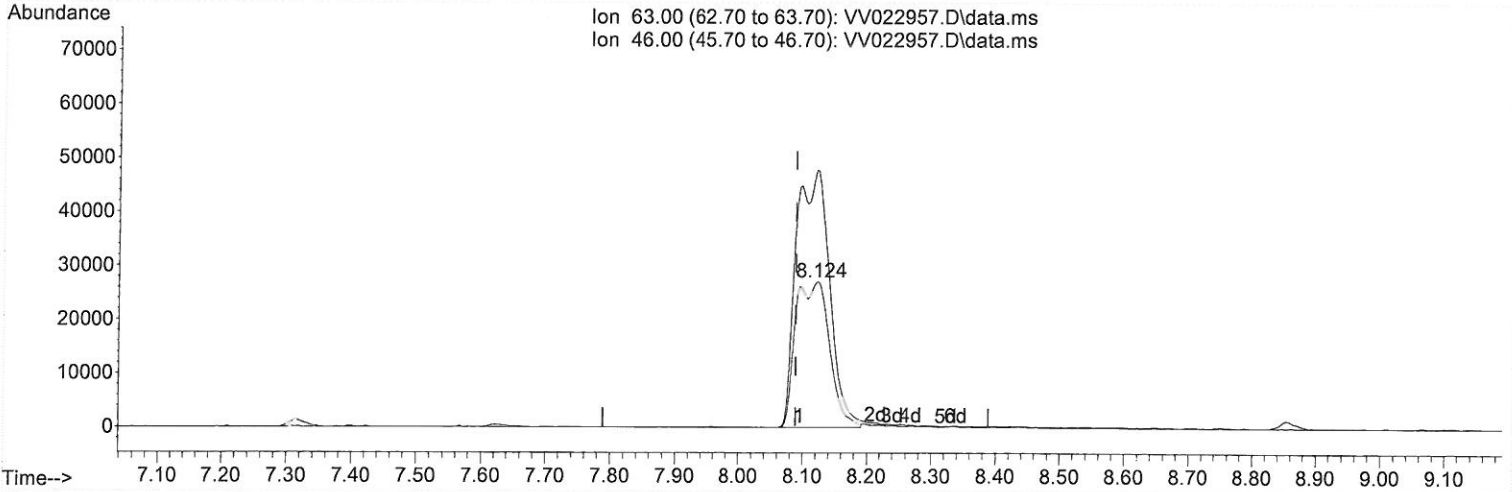

(47) 2-Hexanone-d5 (S)

8.124min (+ 0.035) 101.19 ug/L m

response 98805

Ion Exp% Act%

63.00 100.00 100.00

46.00 163.00 70.33#

0.00 0.00 0.00

0.00 0.00 0.00

MD
 10/26/21

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW102121\
 Data File : VW022957.D
 Acq On : 21 Oct 2021 14:27
 Operator : SY/MD
 Sample : M4264-03ME
 Misc : 3.95g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB7G8ME

Manual Integrations
 APPROVED

MMDadoda
 10/25/2021 11:49:19 AM

Quant Time: Oct 22 03:53:52 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Oct 22 03:48:35 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	339837	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	330494	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.255	152	161936	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	44280	21.068	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	42.140%#		
7) Chloroethane-d5	1.561	69	27472	16.628	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	33.260%#		
11) 1,1-Dichloroethene-d2	2.085	63	52058	12.562	ug/L	-0.02
Spiked Amount 50.000	Range 60 - 125		Recovery =	25.120%#		
21) 2-Butanone-d5	3.892	46	143798	124.295	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	124.300%		
24) Chloroform-d	4.349	84	149478	38.927	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	77.860%		
26) 1,2-Dichloroethane-d4	5.030	65	96140	43.160	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	86.320%		
32) Benzene-d6	5.043	84	242396	31.659	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	63.320%#		
36) 1,2-Dichloropropane-d6	6.069	67	96300	40.857	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	81.720%		
41) Toluene-d8	7.316	98	199261	28.372	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	56.740%#		
43) trans-1,3-Dichloroprop...	7.622	79	43966	39.425	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	78.840%		
47) 2-Hexanone-d5	8.124	63	98805m	101.192	ug/L	0.04
Spiked Amount 100.000	Range 45 - 130		Recovery =	101.190%		
56) 1,1,2,2-Tetrachloroeth...	10.223	84	162282	49.513	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	99.020%		
66) 1,2-Dichlorobenzene-d4	11.628	152	131721	49.880	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	99.760%		
Target Compounds						
15) Methyl Acetate	2.445	43	3499m	1.312	ug/L	Qvalue 98
16) Methylene chloride	2.500	84	10999	3.688	ug/L	98
25) Chloroform	4.365	83	3156	0.680	ug/L	91

(#) = qualifier out of range (m) = manual integration (+) = signals summed