

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102121\
 Data File : VV022950.D
 Acq On : 21 Oct 2021 11:23
 Operator : SY/MD
 Sample : VV1021MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK263

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M

Title : VOC Analysis

Signal : TIC: VV022950.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	97	rVB	161138	162094	16.48%	2.080%
2	1.568	157	164	178	rVB	109427	120824	12.28%	1.550%
3	2.108	321	332	352	rBV	226776	334092	33.96%	4.286%
4	2.259	377	379	382	rBV3	564	375	0.04%	0.005%
5	2.439	433	435	438	rBV2	543	310	0.03%	0.004%
6	2.609	483	488	491	rBV2	391	343	0.03%	0.004%
7	3.204	671	673	677	rVB4	375	229	0.02%	0.003%
8	3.314	703	707	709	rBV	397	287	0.03%	0.004%
9	3.410	735	737	740	rVB2	400	230	0.02%	0.003%
10	3.680	815	821	824	rBV3	269	223	0.02%	0.003%
11	3.751	839	843	845	rBV3	361	220	0.02%	0.003%
12	3.886	875	885	910	rBV2	61182	184724	18.78%	2.370%
13	4.349	1013	1029	1053	rBV	143554	387456	39.38%	4.971%
14	4.551	1090	1092	1095	rBV2	617	330	0.03%	0.004%
15	4.590	1100	1104	1105	rBV	301	203	0.02%	0.003%
16	4.667	1125	1128	1133	rBV5	680	459	0.05%	0.006%
17	4.777	1158	1162	1165	rVB2	394	247	0.03%	0.003%
18	4.867	1186	1190	1195	rVB	536	420	0.04%	0.005%
19	4.963	1216	1220	1224	rBV2	517	477	0.05%	0.006%
20	5.047	1228	1246	1278	rBV2	382550	983795	100.00%	12.622%
21	5.256	1308	1311	1314	rVB4	711	533	0.05%	0.007%
22	5.420	1361	1362	1367	rVB2	394	261	0.03%	0.003%
23	5.532	1394	1397	1402	rVB5	561	483	0.05%	0.006%
24	5.616	1411	1423	1451	rBV	329504	669522	68.06%	8.590%
25	5.857	1494	1498	1501	rBV3	447	379	0.04%	0.005%
26	5.912	1505	1515	1530	rBV6	6717	14755	1.50%	0.189%
27	6.024	1545	1550	1551	rBV3	495	356	0.04%	0.005%
28	6.069	1551	1564	1585	rBV	219871	443213	45.05%	5.686%
29	6.262	1621	1624	1628	rVB3	717	481	0.05%	0.006%
30	6.358	1652	1654	1657	rVB2	383	202	0.02%	0.003%
31	6.426	1673	1675	1680	rVB2	431	338	0.03%	0.004%
32	6.539	1705	1710	1712	rBV3	573	365	0.04%	0.005%
33	6.564	1715	1718	1721	rBV2	318	214	0.02%	0.003%
34	6.789	1783	1788	1791	rBV3	624	459	0.05%	0.006%
35	6.818	1794	1797	1801	rBV3	310	269	0.03%	0.003%
36	6.985	1839	1849	1871	rBV2	118946	216604	22.02%	2.779%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102121\
 Data File : VV022950.D
 Acq On : 21 Oct 2021 11:23
 Operator : SY/MD
 Sample : VV1021MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK263

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
 Title : VOC Analysis

37	7.207	1916	1918	1922	rVB4	582	356	0.04%	0.005%
38	7.227	1922	1924	1927	rBV	464	266	0.03%	0.003%
39	7.317	1940	1952	1971	rBV	456955	784902	79.78%	10.070%
40	7.587	2032	2036	2037	rBV	681	359	0.04%	0.005%
41	7.622	2037	2047	2062	rBV	84859	146142	14.85%	1.875%
42	7.815	2102	2107	2109	rBV2	423	363	0.04%	0.005%
43	7.870	2120	2124	2126	rBV	406	342	0.03%	0.004%
44	7.934	2140	2144	2147	rBV2	449	400	0.04%	0.005%
45	7.956	2147	2151	2154	rVB	471	438	0.04%	0.006%
46	7.992	2158	2162	2164	rBV2	354	285	0.03%	0.004%
47	8.088	2182	2192	2225	rBV	234897	427567	43.46%	5.485%
48	8.465	2306	2309	2312	rVB3	423	249	0.03%	0.003%
49	8.493	2316	2318	2321	rVV2	489	270	0.03%	0.003%
50	8.545	2329	2334	2338	rBV3	323	371	0.04%	0.005%
51	8.702	2381	2383	2386	rBV	366	235	0.02%	0.003%
52	8.747	2393	2397	2400	rVB2	437	287	0.03%	0.004%
53	8.854	2418	2430	2462	rVV	508855	836589	85.04%	10.733%
54	9.098	2503	2506	2511	rVB3	592	383	0.04%	0.005%
55	9.133	2511	2517	2518	rBV3	279	262	0.03%	0.003%
56	9.146	2518	2521	2525	rBV3	629	564	0.06%	0.007%
57	9.188	2532	2534	2537	rVB2	532	224	0.02%	0.003%
58	9.230	2543	2547	2549	rBV3	492	296	0.03%	0.004%
59	9.259	2553	2556	2557	rBV	511	258	0.03%	0.003%
60	9.294	2563	2567	2570	rBV3	301	264	0.03%	0.003%
61	9.310	2570	2572	2577	rVB3	515	251	0.03%	0.003%
62	9.333	2577	2579	2582	rBV	348	245	0.02%	0.003%
63	9.387	2592	2596	2599	rBV2	329	206	0.02%	0.003%
64	9.532	2636	2641	2643	rBV2	255	266	0.03%	0.003%
65	9.558	2647	2649	2652	rVB2	491	282	0.03%	0.004%
66	9.767	2711	2714	2716	rVB2	399	242	0.02%	0.003%
67	10.008	2787	2789	2791	rBV	380	225	0.02%	0.003%
68	10.120	2820	2824	2834	rVB6	2817	4401	0.45%	0.056%
69	10.217	2842	2854	2875	rBV	297816	467833	47.55%	6.002%
70	10.455	2926	2928	2932	rVV2	446	261	0.03%	0.003%
71	10.561	2959	2961	2963	rBV	656	343	0.03%	0.004%
72	10.661	2988	2992	2995	rBV3	678	547	0.06%	0.007%
73	10.828	3040	3044	3045	rBV3	404	278	0.03%	0.004%
74	10.915	3063	3071	3080	rVV6	2365	3885	0.39%	0.050%
75	11.024	3103	3105	3107	rBV	492	239	0.02%	0.003%
76	11.072	3116	3120	3127	rBV3	419	460	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102121\
 Data File : VV022950.D
 Acq On : 21 Oct 2021 11:23
 Operator : SY/MD
 Sample : VV1021MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK263

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M

Title : VOC Analysis

77	11.149	3137	3144	3147	rBV4	1194	1506	0.15%	0.019%
78	11.188	3151	3156	3164	rBV5	816	877	0.09%	0.011%
79	11.249	3164	3175	3204	rBV	543386	834831	84.86%	10.710%
80	11.490	3248	3250	3254	rVB2	376	246	0.03%	0.003%
81	11.516	3256	3258	3261	rVB	439	224	0.02%	0.003%
82	11.535	3261	3264	3265	rBV2	359	199	0.02%	0.003%
83	11.625	3280	3292	3309	rBV	467239	740637	75.28%	9.502%
84	11.776	3335	3339	3340	rBV2	589	460	0.05%	0.006%
85	12.043	3420	3422	3427	rBV	249	211	0.02%	0.003%
86	12.127	3445	3448	3450	rBV3	388	256	0.03%	0.003%
87	12.252	3485	3487	3490	rVB	738	332	0.03%	0.004%
88	12.596	3591	3594	3596	rBV2	514	317	0.03%	0.004%
89	12.654	3606	3612	3613	rBV4	950	880	0.09%	0.011%
90	12.677	3617	3619	3622	rBV2	476	279	0.03%	0.004%
91	12.789	3651	3654	3658	rBV3	341	306	0.03%	0.004%
92	12.905	3688	3690	3693	rVB2	501	222	0.02%	0.003%
93	12.927	3693	3697	3699	rBV2	299	250	0.03%	0.003%
94	13.226	3788	3790	3794	rBV2	314	229	0.02%	0.003%
95	13.268	3797	3803	3813	rBV6	1502	2240	0.23%	0.029%
96	13.435	3853	3855	3859	rBV2	480	360	0.04%	0.005%
97	13.744	3948	3951	3954	rBV4	1101	958	0.10%	0.012%
98	14.021	4032	4037	4039	rBV3	393	359	0.04%	0.005%
99	14.185	4081	4088	4093	rBV4	668	755	0.08%	0.010%
100	15.622	4533	4535	4537	rBV3	554	245	0.02%	0.003%




Sum of corrected areas: 7794587

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102121\
Data File : VV022950.D
Acq On : 21 Oct 2021 11:23
Operator : SY/MD
Sample : VV1021MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK263

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

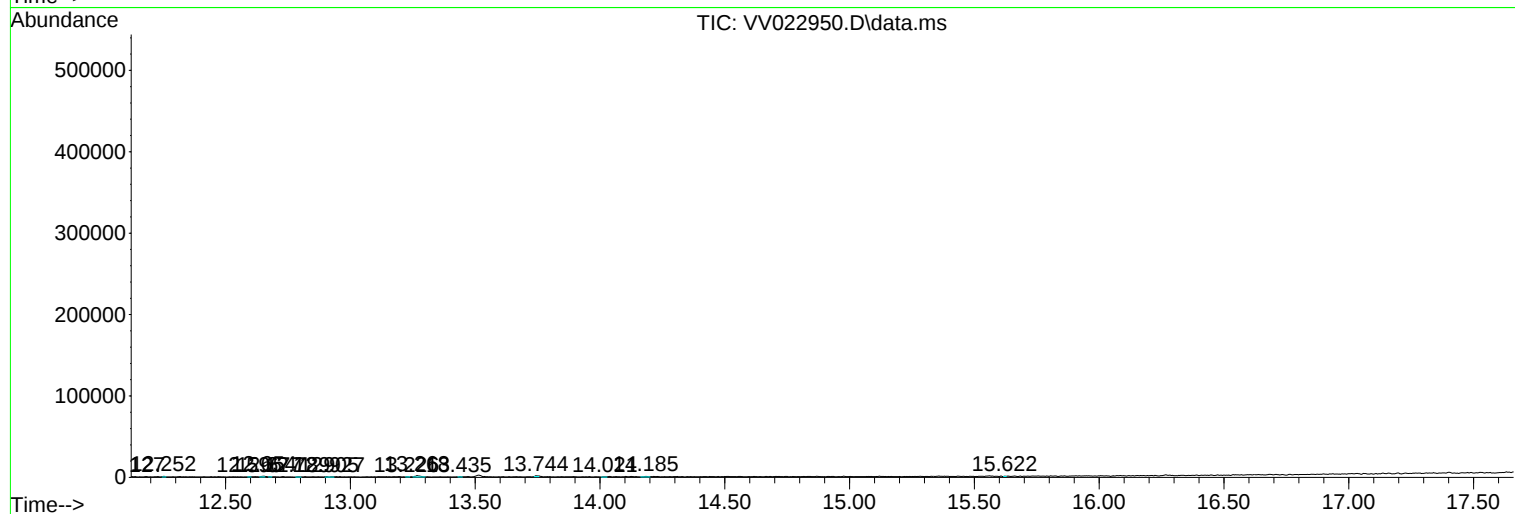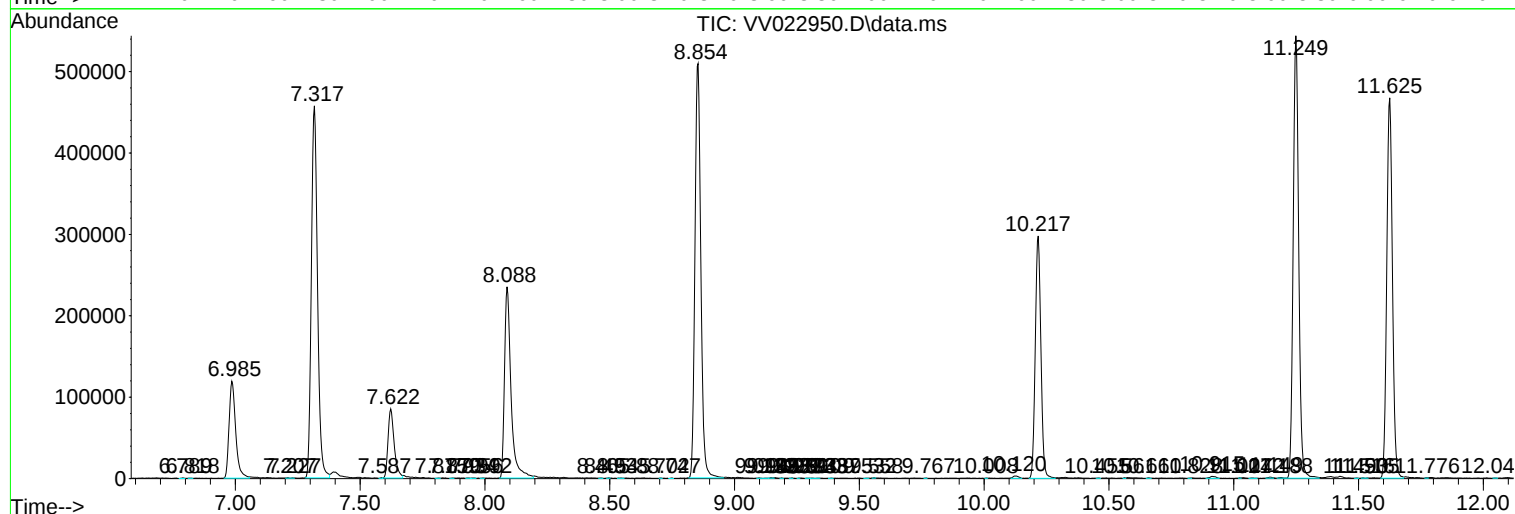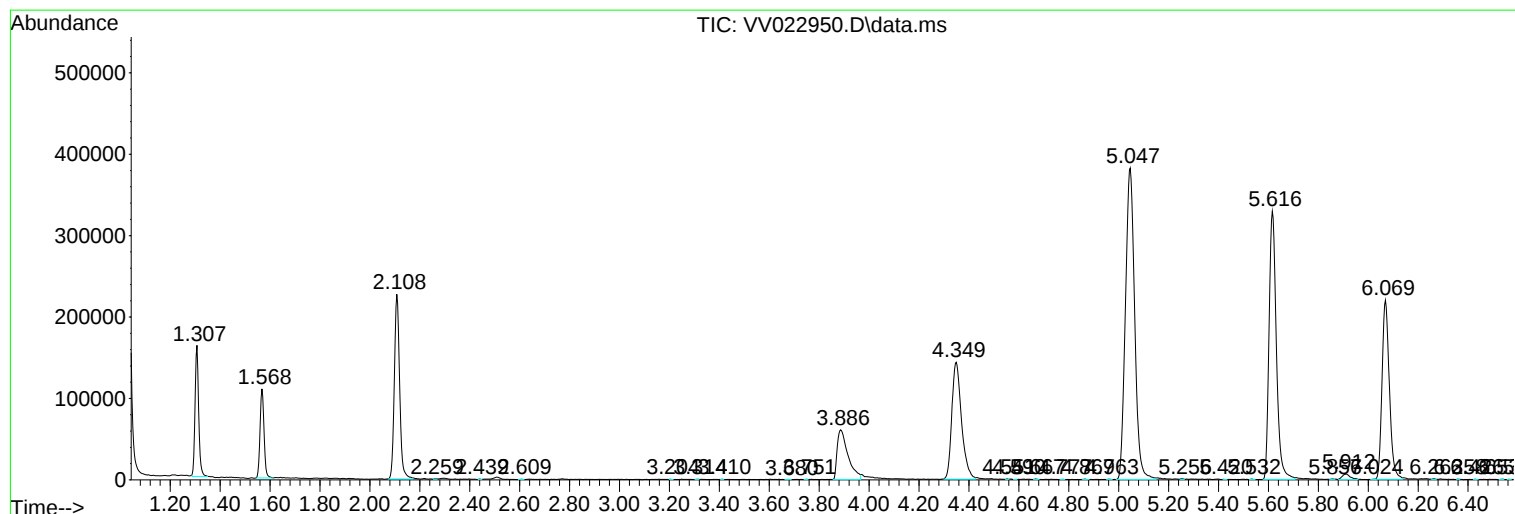

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102121\
Data File : VV022950.D
Acq On : 21 Oct 2021 11:23
Operator : SY/MD
Sample : VV1021MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK263

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102121\
Data File : VV022950.D
Acq On : 21 Oct 2021 11:23
Operator : SY/MD
Sample : VV1021MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK263

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
