

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102121\
 Data File : VV022952.D
 Acq On : 21 Oct 2021 12:09
 Operator : SY/MD
 Sample : M4212-15ME
 Misc : 2.80g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 JDGF8ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M

Title : VOC Analysis

Signal : TIC: VV022952.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	104	rVB	64669	80822	9.03%	1.111%
2	1.565	157	163	176	rBV	41858	57964	6.48%	0.797%
3	2.053	312	315	316	rBV	427	251	0.03%	0.003%
4	2.092	316	327	338	rBV	91160	131142	14.65%	1.803%
5	2.372	410	414	418	rVB3	343	317	0.04%	0.004%
6	2.401	418	423	427	rBV3	313	361	0.04%	0.005%
7	2.436	428	434	437	rBV2	897	1020	0.11%	0.014%
8	2.503	446	455	466	rBV2	6710	11893	1.33%	0.164%
9	2.558	469	472	473	rBV2	340	193	0.02%	0.003%
10	2.799	545	547	552	rBV3	395	337	0.04%	0.005%
11	3.024	613	617	619	rBV4	897	667	0.07%	0.009%
12	3.262	689	691	695	rBV2	387	293	0.03%	0.004%
13	3.384	726	729	731	rBV3	376	254	0.03%	0.003%
14	3.442	743	747	750	rBV2	452	432	0.05%	0.006%
15	3.561	782	784	785	rBV	530	271	0.03%	0.004%
16	3.593	791	794	798	rVB4	388	283	0.03%	0.004%
17	3.626	802	804	808	rVB2	293	177	0.02%	0.002%
18	3.706	828	829	832	rBV2	360	189	0.02%	0.003%
19	3.818	862	864	866	rBV	344	172	0.02%	0.002%
20	3.896	876	888	920	rBV2	63768	224985	25.13%	3.093%
21	4.349	1016	1029	1054	rVB	133439	347694	38.84%	4.781%
22	4.548	1089	1091	1093	rBV3	501	236	0.03%	0.003%
23	4.783	1162	1164	1167	rBV3	301	198	0.02%	0.003%
24	4.815	1172	1174	1178	rBV3	605	328	0.04%	0.005%
25	4.857	1183	1187	1190	rBV2	550	408	0.05%	0.006%
26	5.043	1228	1245	1273	rBV2	305297	778543	86.98%	10.704%
27	5.455	1371	1373	1377	rVB2	546	293	0.03%	0.004%
28	5.474	1377	1379	1381	rBV	293	171	0.02%	0.002%
29	5.529	1394	1396	1397	rBV2	337	170	0.02%	0.002%
30	5.616	1411	1423	1449	rBV	358264	725182	81.02%	9.971%
31	5.908	1505	1514	1532	rVB3	9007	18675	2.09%	0.257%
32	6.069	1553	1564	1589	rVB	189225	392189	43.81%	5.392%
33	6.217	1606	1610	1612	rBV4	641	428	0.05%	0.006%
34	6.272	1622	1627	1630	rBV3	389	311	0.03%	0.004%
35	6.342	1644	1649	1651	rBV	446	269	0.03%	0.004%
36	6.378	1656	1660	1667	rBV2	372	569	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW102121\
 Data File : VW022952.D
 Acq On : 21 Oct 2021 12:09
 Operator : SY/MD
 Sample : M4212-15ME
 Misc : 2.80g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 JDGF8ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
 Title : VOC Analysis

37	6.510	1697	1701	1703	rBV2	260	193	0.02%	0.003%
38	6.587	1723	1725	1730	rVB5	376	225	0.03%	0.003%
39	6.629	1732	1738	1739	rBV2	826	688	0.08%	0.009%
40	6.703	1759	1761	1763	rVB2	398	175	0.02%	0.002%
41	6.751	1773	1776	1778	rBV	624	267	0.03%	0.004%
42	6.793	1785	1789	1790	rBV2	643	373	0.04%	0.005%
43	6.822	1796	1798	1801	rVB	331	187	0.02%	0.003%
44	6.989	1839	1850	1872	rBV	93185	182055	20.34%	2.503%
45	7.169	1904	1906	1911	rBV3	419	293	0.03%	0.004%
46	7.317	1939	1952	1970	rBV	300753	527218	58.90%	7.249%
47	7.625	2038	2048	2075	rBV	64348	127863	14.28%	1.758%
48	7.793	2096	2100	2102	rBV5	1009	840	0.09%	0.012%
49	7.883	2126	2128	2132	rBV3	445	290	0.03%	0.004%
50	7.986	2158	2160	2161	rBV	615	266	0.03%	0.004%
51	8.018	2166	2170	2172	rBV3	268	194	0.02%	0.003%
52	8.114	2181	2200	2236	rBV2	155127	540966	60.44%	7.438%
53	8.407	2288	2291	2293	rBV3	827	450	0.05%	0.006%
54	8.535	2328	2331	2337	rVB3	605	412	0.05%	0.006%
55	8.609	2352	2354	2358	rVB2	474	271	0.03%	0.004%
56	8.648	2364	2366	2370	rVB3	398	262	0.03%	0.004%
57	8.683	2373	2377	2384	rBV4	587	655	0.07%	0.009%
58	8.854	2418	2430	2455	rBV	511851	895115	100.00%	12.307%
59	9.066	2493	2496	2498	rBV	388	214	0.02%	0.003%
60	9.098	2501	2506	2514	rBV5	700	810	0.09%	0.011%
61	9.188	2532	2534	2536	rBV2	377	176	0.02%	0.002%
62	9.207	2536	2540	2541	rBV3	518	368	0.04%	0.005%
63	9.310	2570	2572	2575	rVV2	326	194	0.02%	0.003%
64	9.497	2628	2630	2635	rBV4	502	283	0.03%	0.004%
65	9.567	2648	2652	2653	rBV2	383	247	0.03%	0.003%
66	9.603	2662	2663	2665	rBV	390	179	0.02%	0.002%
67	9.741	2703	2706	2709	rBV2	307	210	0.02%	0.003%
68	9.873	2743	2747	2749	rBV	394	309	0.03%	0.004%
69	9.911	2757	2759	2764	rBV4	483	288	0.03%	0.004%
70	9.953	2769	2772	2776	rVB3	428	257	0.03%	0.004%
71	10.056	2799	2804	2807	rBV3	392	352	0.04%	0.005%
72	10.223	2843	2856	2872	rBV	319595	551234	61.58%	7.579%
73	10.580	2963	2967	2969	rBV2	691	539	0.06%	0.007%
74	10.645	2984	2987	2991	rBV3	313	278	0.03%	0.004%
75	10.751	3018	3020	3022	rBV	356	192	0.02%	0.003%
76	10.911	3067	3070	3071	rBV2	734	358	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW102121\
 Data File : VW022952.D
 Acq On : 21 Oct 2021 12:09
 Operator : SY/MD
 Sample : M4212-15ME
 Misc : 2.80g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 JDGF8ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
 Title : VOC Analysis

77	10.989	3089	3094	3098	rBV4	373	367	0.04%	0.005%
78	11.098	3124	3128	3130	rVB3	374	259	0.03%	0.004%
79	11.198	3154	3159	3163	rBV4	538	548	0.06%	0.008%
80	11.252	3164	3176	3198	rBV	560165	877092	97.99%	12.059%
81	11.548	3263	3268	3270	rBV3	667	499	0.06%	0.007%
82	11.628	3281	3293	3313	rBV	492401	774389	86.51%	10.647%
83	11.899	3374	3377	3381	rVB3	481	348	0.04%	0.005%
84	12.014	3410	3413	3414	rBV	361	181	0.02%	0.002%
85	12.091	3433	3437	3440	rBV3	411	439	0.05%	0.006%
86	12.169	3460	3461	3466	rBV2	386	256	0.03%	0.004%
87	12.210	3472	3474	3476	rBV	497	249	0.03%	0.003%
88	12.452	3548	3549	3554	rVB3	435	290	0.03%	0.004%
89	12.545	3575	3578	3581	rVV	531	426	0.05%	0.006%
90	12.574	3584	3587	3590	rVV3	340	247	0.03%	0.003%
91	12.944	3698	3702	3709	rBV3	407	517	0.06%	0.007%
92	13.069	3739	3741	3745	rVB2	384	215	0.02%	0.003%
93	13.107	3751	3753	3757	rBV2	421	322	0.04%	0.004%
94	13.275	3800	3805	3812	rBV4	1047	1211	0.14%	0.017%
95	13.365	3828	3833	3835	rVB2	388	308	0.03%	0.004%
96	13.403	3842	3845	3846	rBV	332	179	0.02%	0.002%
97	13.480	3866	3869	3871	rBV2	538	371	0.04%	0.005%
98	13.927	4006	4008	4014	rBV2	340	332	0.04%	0.005%
99	14.201	4091	4093	4096	rBV	409	296	0.03%	0.004%
100	14.751	4262	4264	4267	rBV2	518	287	0.03%	0.004%




Sum of corrected areas: 7273061

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102121\
Data File : VV022952.D
Acq On : 21 Oct 2021 12:09
Operator : SY/MD
Sample : M4212-15ME
Misc : 2.80g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
JDGF8ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

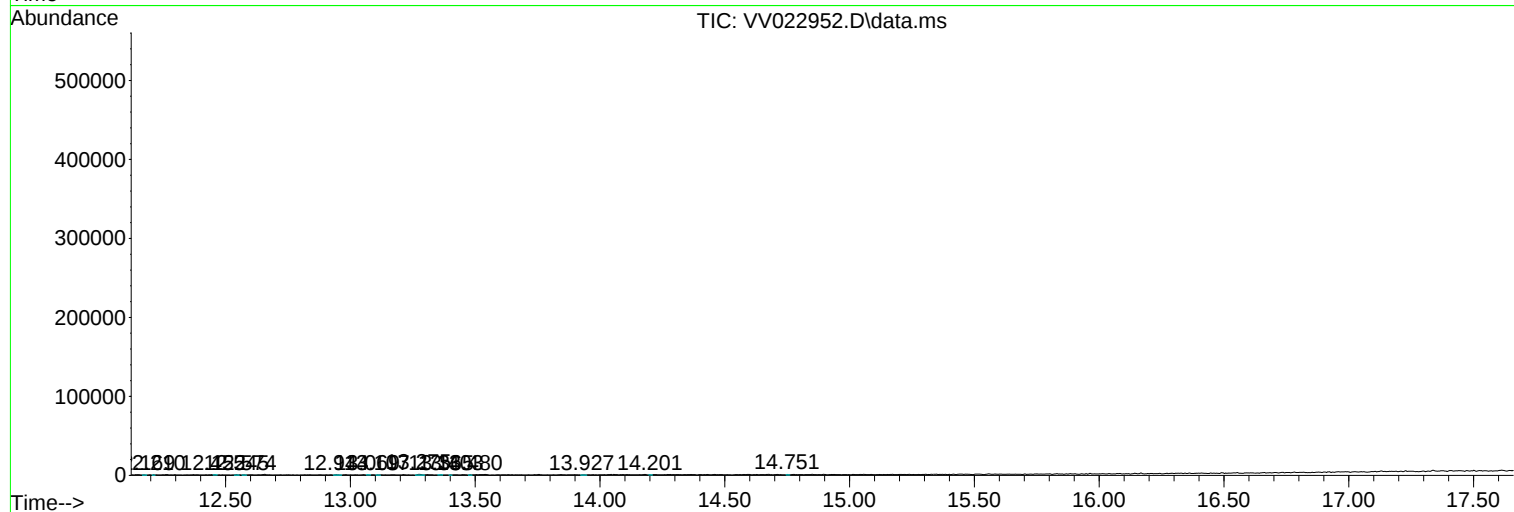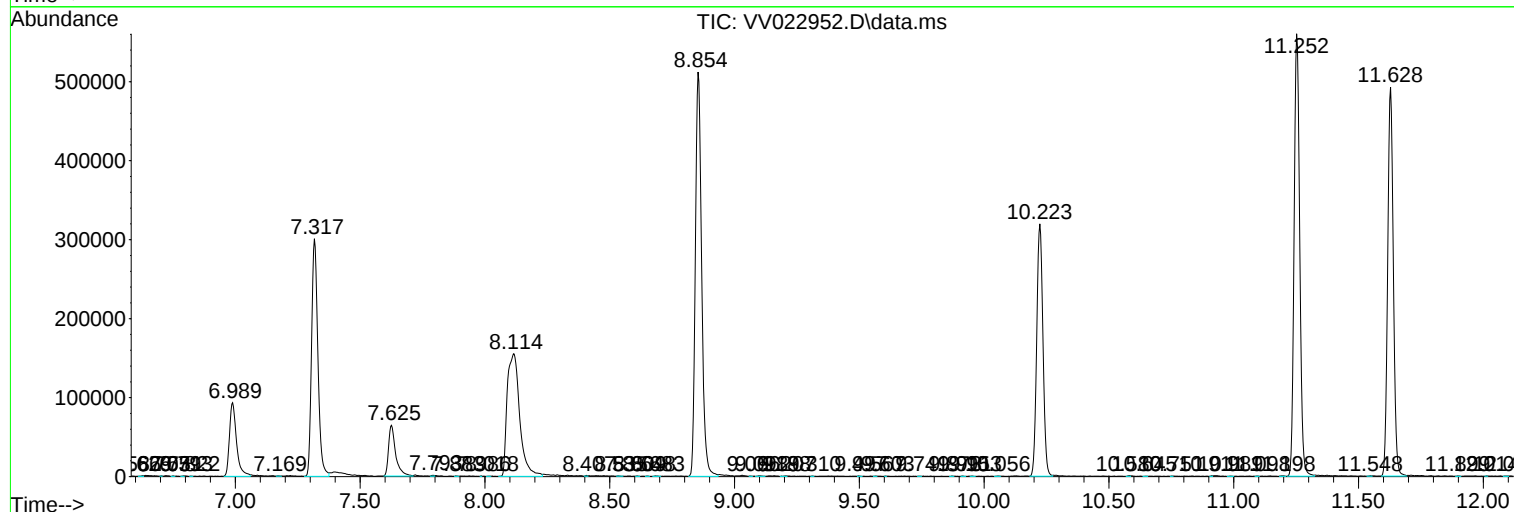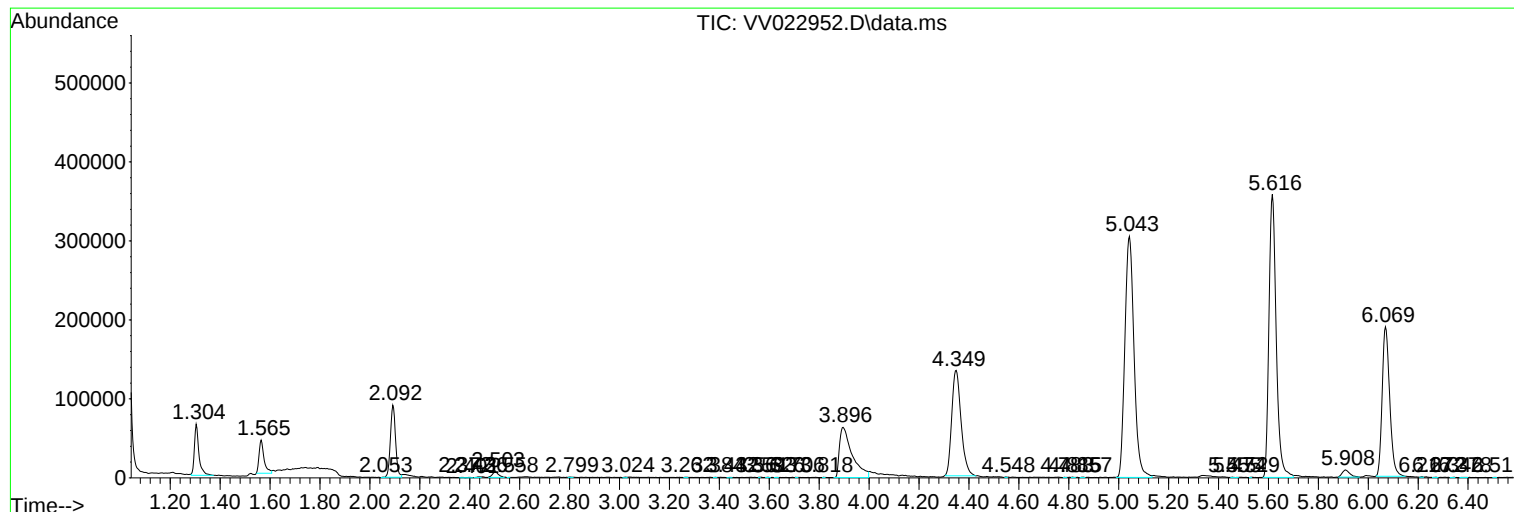

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102121\
Data File : VV022952.D
Acq On : 21 Oct 2021 12:09
Operator : SY/MD
Sample : M4212-15ME
Misc : 2.80g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
JDGF8ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102121\
Data File : VV022952.D
Acq On : 21 Oct 2021 12:09
Operator : SY/MD
Sample : M4212-15ME
Misc : 2.80g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
JDGF8ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
