
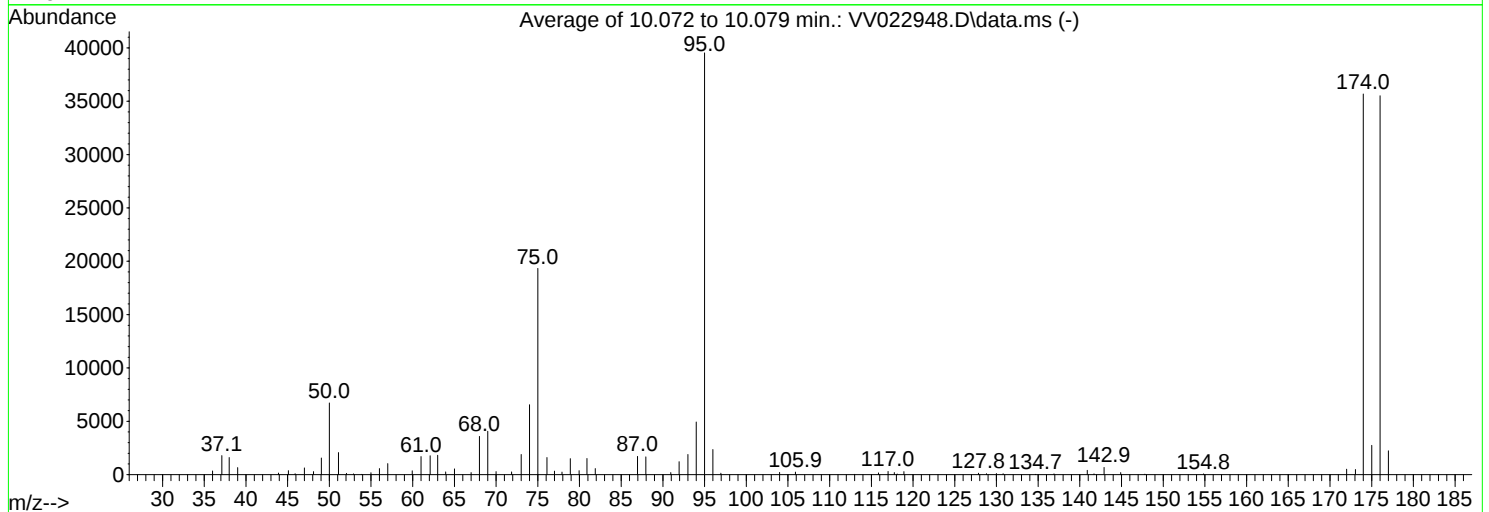


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102121\
Data File : VV022948.D
Acq On : 21 Oct 2021 08:57
Operator : SY/MD
Sample : BFB242
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB242

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Title : VOC Analysis
Last Update : Fri Oct 22 03:48:35 2021

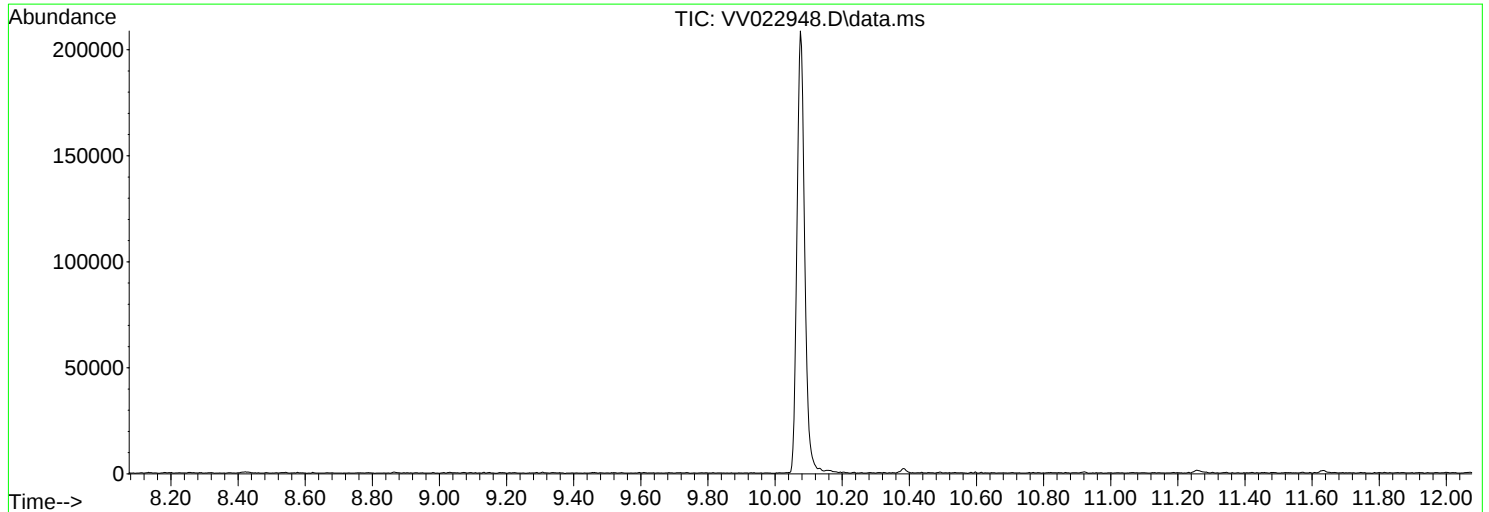

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2799

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.0	6721	PASS
75	95	30	80	48.9	19328	PASS
95	95	100	100	100.0	39536	PASS
96	95	5	9	6.0	2362	PASS
173	174	0.00	2	1.3	480	PASS
174	95	50	120	90.2	35677	PASS
175	174	5	9	7.7	2744	PASS
176	174	95	105	99.5	35515	PASS
177	176	5	10	6.3	2240	PASS

m/z	Abundance
37.50	101.0
39.00	109.0
40.00	167.0
43.90	315.0

Instrument :
MSVOA_V
ClientSampleId :
BFB242

m/z	Abundance
36.00	358.0
37.10	1854.0
38.00	1481.0
39.00	750.0
40.00	170.0
43.90	433.0
45.10	390.0
45.90	149.0
47.00	708.0
48.10	294.0
49.10	1498.0
50.00	6619.0
51.10	2164.0
52.00	133.0
52.90	106.0
55.00	181.0
56.00	590.0
57.00	1073.0
60.00	395.0
61.00	1551.0
62.10	1702.0
63.00	1815.0
64.00	245.0
65.00	517.0
67.00	178.0
68.00	3645.0
69.00	3991.0
69.90	295.0
71.90	274.0
73.00	1829.0
74.00	6464.0
75.00	19160.0
76.10	1520.0
77.00	312.0
77.90	232.0
78.90	1483.0
80.00	293.0
80.90	1489.0
81.90	552.0
86.90	1637.0
88.00	1688.0
90.90	166.0
92.00	1169.0
93.00	1840.0
94.00	4607.0
95.00	38832.0
96.00	2265.0
96.90	129.0
104.00	197.0
105.80	221.0
116.00	162.0
117.00	278.0
117.80	215.0
119.00	267.0
127.90	134.0
130.00	188.0
134.70	101.0
140.90	404.0
141.70	107.0
142.90	730.0
144.90	192.0
147.80	130.0
172.00	454.0
173.10	432.0
174.00	33784.0
175.00	2674.0
176.00	33416.0
177.00	2199.0

Instrument :
MSVOA_V
ClientSampleId :
BFB242

m/z	Abundance
36.00	370.0
37.10	1825.0
38.00	1660.0
39.00	805.0
40.10	164.0
44.00	475.0
45.10	397.0
45.90	107.0
47.00	664.0
48.10	299.0
49.10	1611.0
50.00	6911.0
51.10	2138.0
52.00	130.0
52.90	101.0
55.00	180.0
56.00	585.0
57.00	1062.0
60.00	352.0
61.00	1743.0
62.10	1783.0
63.00	1848.0
63.90	264.0
65.00	571.0
67.00	233.0
68.00	3680.0
69.00	4250.0
70.00	293.0
71.90	280.0
73.00	1983.0
74.00	6757.0
75.00	19968.0
76.10	1634.0
77.00	355.0
77.90	249.0
78.90	1524.0
80.00	368.0
80.90	1561.0
81.90	596.0
87.00	1776.0
87.90	1701.0
90.90	203.0
91.90	1277.0
93.00	1913.0
94.00	5093.0
95.00	40800.0
96.00	2435.0
96.90	146.0
104.00	216.0
105.90	253.0
113.00	102.0
115.80	171.0
117.00	311.0
117.80	205.0
118.90	290.0
127.80	143.0
128.80	125.0
130.00	127.0
130.80	120.0
136.90	111.0
140.90	421.0
141.70	105.0
142.90	689.0
144.90	191.0
154.90	110.0
172.00	518.0
173.00	506.0
174.00	37056.0
175.00	2814.0
176.00	36832.0
177.00	2296.0

Instrument :
MSVOA_V
ClientSampleId :
BFB242

m/z	Abundance
36.00	332.0
37.10	1668.0
38.00	1680.0
39.00	761.0
39.90	166.0
44.00	468.0
45.10	358.0
47.00	535.0
48.10	285.0
49.00	1579.0
50.00	6633.0
51.10	1922.0
52.10	117.0
53.90	111.0
55.00	187.0
56.00	540.0
57.00	962.0
59.90	340.0
61.00	1789.0
62.10	1811.0
63.00	1771.0
63.90	279.0
65.00	525.0
67.00	196.0
68.00	3435.0
69.00	3954.0
70.10	256.0
71.80	218.0
73.00	1879.0
74.00	6432.0
75.00	18856.0
76.10	1671.0
77.00	316.0
77.90	253.0
78.90	1500.0
79.90	457.0
80.90	1501.0
81.90	548.0
87.00	1724.0
87.90	1589.0
91.00	207.0
92.00	1208.0
93.00	1905.0
94.00	5094.0
95.00	38976.0
96.00	2387.0
97.00	145.0
104.00	224.0
106.00	242.0
115.80	167.0
117.00	329.0
117.70	187.0
118.10	170.0
118.80	317.0
127.80	144.0
128.80	126.0
130.80	136.0
136.90	139.0
140.90	393.0
142.90	628.0
144.90	188.0
154.80	122.0
172.00	548.0
173.00	502.0
174.00	36192.0
175.00	2745.0
176.00	36296.0
177.00	2226.0

Instrument :
MSVOA_V
ClientSampleId :
BFB242