

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV102124\
 Data File : VV037901.D
 Acq On : 21 Oct 2024 14:03
 Operator : SY/MD
 Sample : VV1021WBL01
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Oct 22 05:08:05 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Oct 22 05:07:16 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.526	114	471256	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.777	117	467882	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.178	152	220750	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	172824	41.776	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	83.560%		
7) Chloroethane-d5	1.532	69	158643	49.405	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	98.800%		
11) 1,1-Dichloroethene-d2	2.057	65	83429	48.271	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	96.540%		
21) 2-Butanone-d5	3.796	46	143767	97.570	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	97.570%		
24) Chloroform-d	4.240	84	387885	52.702	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	105.400%		
26) 1,2-Dichloroethane-d4	4.934	65	234992	54.548	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	109.100%		
32) Benzene-d6	4.950	84	746333	50.976	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	101.960%		
36) 1,2-Dichloropropane-d6	5.979	67	244010	52.339	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	104.680%		
41) Toluene-d8	7.236	98	636424	47.938	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	95.880%		
43) trans-1,3-Dichloroprop...	7.548	79	95869	44.266	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	88.540%		
47) 2-Hexanone-d5	8.021	63	88138	89.530	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	89.530%		
56) 1,1,2,2-Tetrachloroeth...	10.143	84	273008	50.398	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	100.800%		
66) 1,2-Dichlorobenzene-d4	11.551	152	256478	55.137	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	110.280%		
Target Compounds						Qvalue
10) 1,1,2-Trichloro-1,2,2-...	2.057	101	2925	0.871	ug/L	# 24


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV102124\
Data File : VV037901.D
Acq On : 21 Oct 2024 14:03
Operator : SY/MD
Sample : VV1021WBL01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Oct 22 05:08:05 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Oct 22 05:07:16 2024
Response via : Initial Calibration

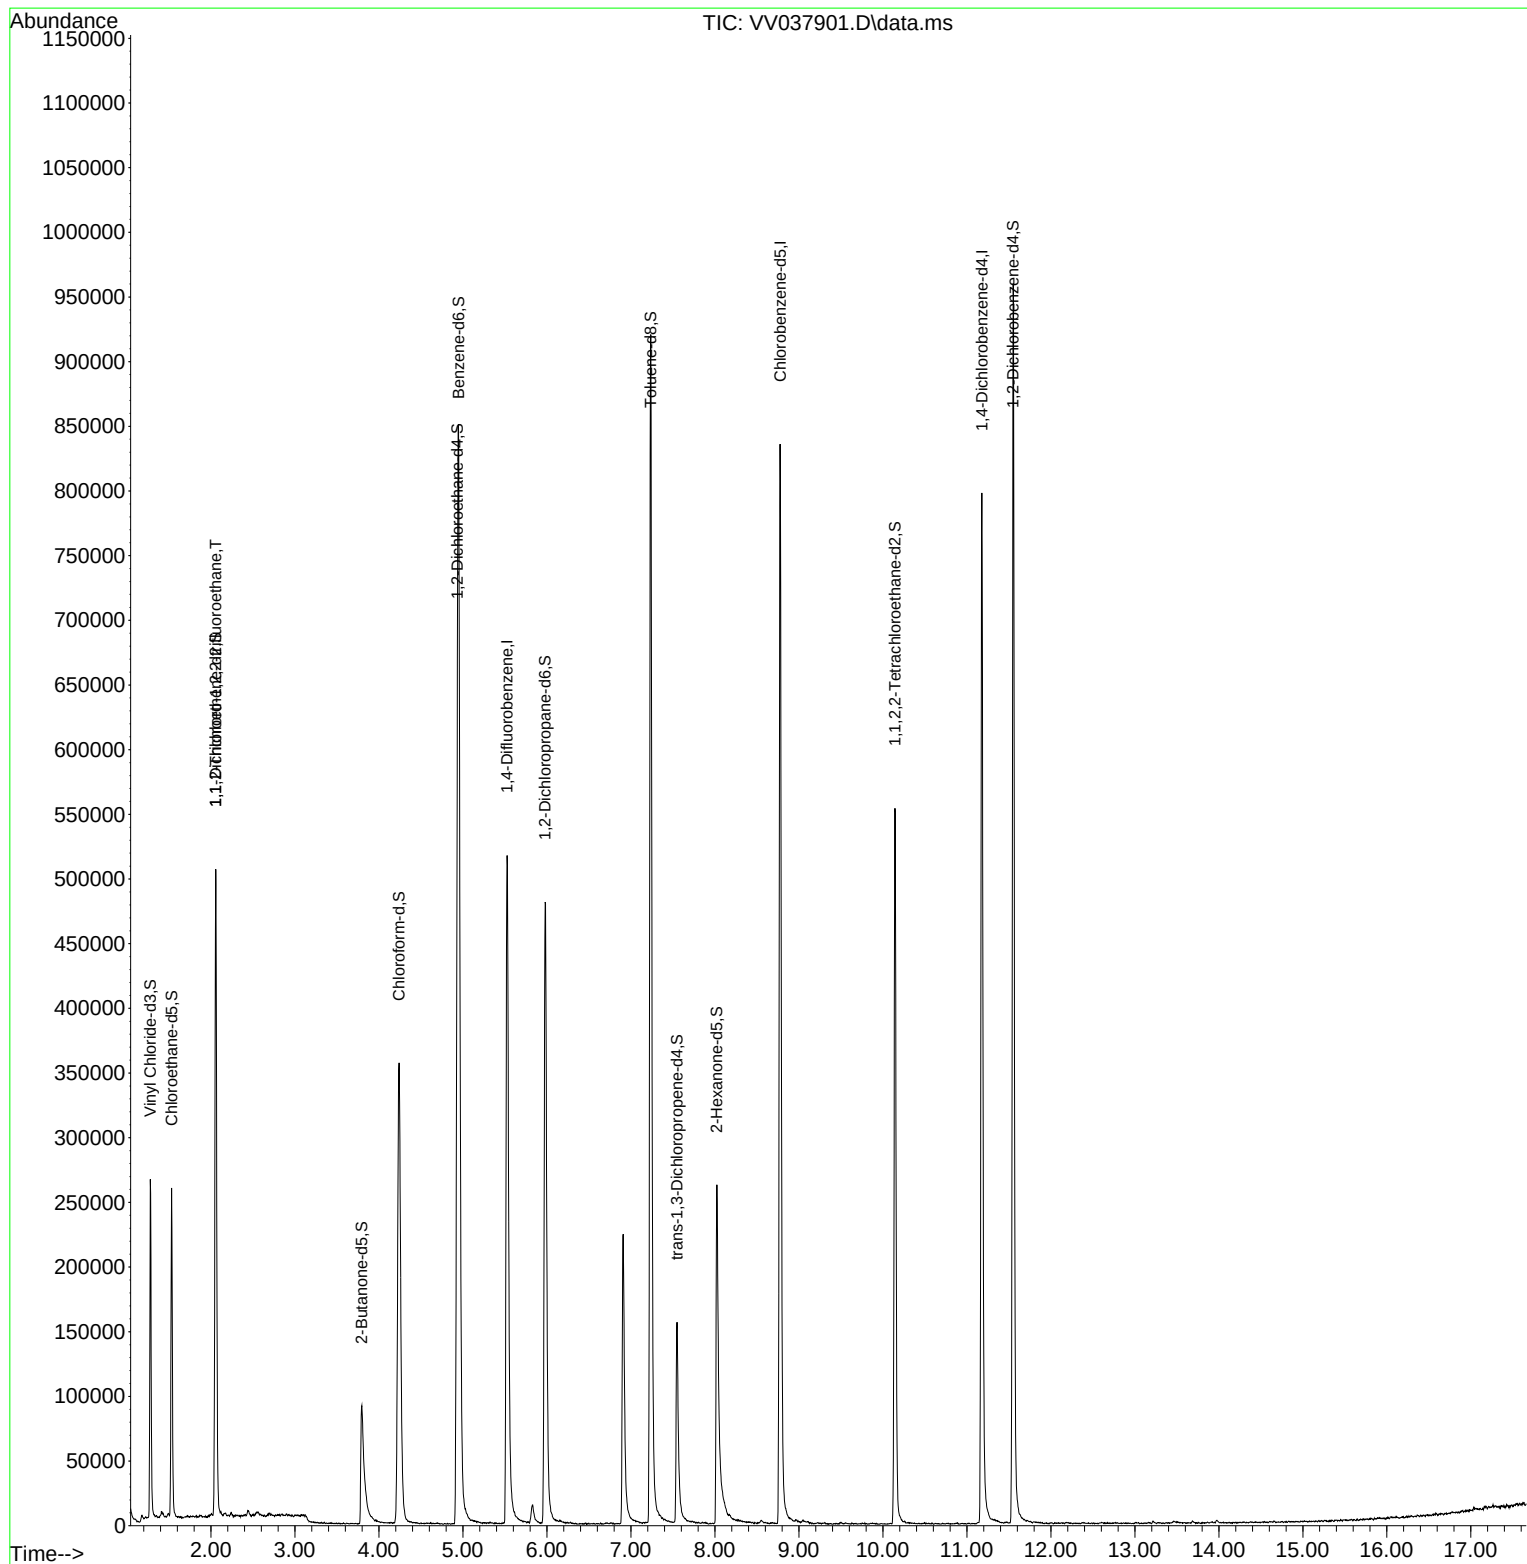

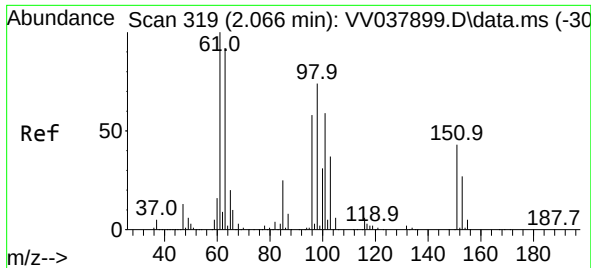

#10
 1,1,2-Trichloro-1,2,2-trifluoroethane
 Concen: 0.871 ug/L
 RT: 2.057 min Scan# 31
 Delta R.T. -0.010 min
 Lab File: VV037901.D
 Acq: 21 Oct 2024 14:03

Instrument :
 MSVOA_V
 ClientSampleId :

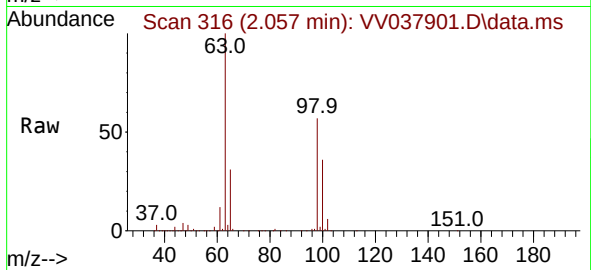

Tgt Ion:	101	Resp:	2925
Ion	Ratio	Lower	Upper
101	100		
85	1.6	34.6	52.0#
151	2.7	57.5	86.3#

