

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV102124\
 Data File : VV037904.D
 Acq On : 21 Oct 2024 17:24
 Operator : SY/MD
 Sample : P4429-12
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037904.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.175	36	42	46	rBV3	5206	6880	0.34%	0.045%
2	1.220	52	56	63	rBV3	4419	5261	0.26%	0.034%
3	1.278	67	74	87	rBV	243150	256900	12.55%	1.677%
4	1.532	145	153	166	rVB	216333	254684	12.44%	1.662%
5	2.056	307	316	330	rBV	439846	635046	31.03%	4.145%
6	3.275	693	695	704	rVB4	1105	1324	0.06%	0.009%
7	3.484	758	760	768	rVB3	884	569	0.03%	0.004%
8	3.577	783	789	790	rBV	625	558	0.03%	0.004%
9	3.799	850	858	891	rBV	104844	301733	14.74%	1.969%
10	4.002	918	921	923	rBV3	932	581	0.03%	0.004%
11	4.082	942	946	953	rVB6	572	545	0.03%	0.004%
12	4.137	959	963	965	rBV4	698	543	0.03%	0.004%
13	4.243	979	996	1024	rBV	346352	882906	43.14%	5.763%
14	4.426	1047	1053	1057	rVB4	876	962	0.05%	0.006%
15	4.468	1063	1066	1070	rBV4	521	520	0.03%	0.003%
16	4.542	1083	1089	1093	rVB6	992	1061	0.05%	0.007%
17	4.651	1118	1123	1125	rBV2	625	670	0.03%	0.004%
18	4.683	1128	1133	1137	rVB3	802	679	0.03%	0.004%
19	4.732	1142	1148	1153	rBV4	930	937	0.05%	0.006%
20	4.947	1199	1215	1258	rBV2	812903	2046825	100.00%	13.360%
21	5.220	1297	1300	1303	rBV3	782	481	0.02%	0.003%
22	5.275	1315	1317	1321	rVB4	1152	611	0.03%	0.004%
23	5.307	1321	1327	1328	rBV4	972	732	0.04%	0.005%
24	5.439	1366	1368	1373	rBV4	689	545	0.03%	0.004%
25	5.529	1384	1396	1425	rBV	628087	1313349	64.17%	8.573%
26	5.777	1471	1473	1475	rBV3	907	567	0.03%	0.004%
27	5.828	1479	1489	1502	rBV3	14694	32192	1.57%	0.210%
28	5.982	1524	1537	1576	rBV	459536	970743	47.43%	6.336%
29	6.143	1585	1587	1593	rBV4	1290	891	0.04%	0.006%
30	6.535	1707	1709	1715	rVB2	732	470	0.02%	0.003%
31	6.719	1763	1766	1768	rBV3	781	539	0.03%	0.004%
32	6.773	1782	1783	1788	rVB3	722	479	0.02%	0.003%
33	6.802	1788	1792	1797	rBV4	877	1197	0.06%	0.008%
34	6.908	1815	1825	1862	rBV	218183	434484	21.23%	2.836%
35	7.236	1914	1927	1956	rBV	843573	1518333	74.18%	9.911%
36	7.548	2016	2024	2056	rBV2	145960	285297	13.94%	1.862%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV102124\
 Data File : VV037904.D
 Acq On : 21 Oct 2024 17:24
 Operator : SY/MD
 Sample : P4429-12
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	7.712	2073	2075	2078	rBV4	783	528	0.03%	0.003%
38	7.751	2084	2087	2092	rVB7	1329	1109	0.05%	0.007%
39	7.793	2097	2100	2103	rBV4	735	577	0.03%	0.004%
40	7.857	2116	2120	2121	rBV2	1347	704	0.03%	0.005%
41	7.883	2126	2128	2132	rVB4	1035	666	0.03%	0.004%
42	8.024	2164	2172	2206	rBV2	305119	670113	32.74%	4.374%
43	8.381	2278	2283	2285	rBV4	941	750	0.04%	0.005%
44	8.494	2316	2318	2321	rBV2	700	537	0.03%	0.004%
45	8.545	2331	2334	2335	rBV3	1539	977	0.05%	0.006%
46	8.616	2350	2356	2359	rBV4	927	860	0.04%	0.006%
47	8.635	2360	2362	2367	rVB3	1030	744	0.04%	0.005%
48	8.674	2367	2374	2380	rVB7	1226	1679	0.08%	0.011%
49	8.712	2380	2386	2388	rBV4	807	743	0.04%	0.005%
50	8.780	2396	2407	2431	rBV	994430	1655506	80.88%	10.806%
51	9.101	2504	2507	2509	rBV3	1015	689	0.03%	0.004%
52	9.169	2524	2528	2531	rBV7	764	765	0.04%	0.005%
53	9.474	2619	2623	2627	rBV3	876	688	0.03%	0.004%
54	9.558	2646	2649	2653	rBV3	888	636	0.03%	0.004%
55	9.699	2689	2693	2697	rBV4	912	765	0.04%	0.005%
56	9.738	2701	2705	2708	rBV4	683	511	0.02%	0.003%
57	9.831	2729	2734	2738	rBV5	538	638	0.03%	0.004%
58	9.895	2750	2754	2761	rVB5	1338	1501	0.07%	0.010%
59	9.934	2761	2766	2769	rBV2	677	580	0.03%	0.004%
60	10.085	2808	2813	2817	rVB5	944	933	0.05%	0.006%
61	10.146	2817	2832	2854	rBV	596903	951382	46.48%	6.210%
62	10.320	2879	2886	2897	rVB6	4501	6790	0.33%	0.044%
63	10.458	2925	2929	2932	rBV3	773	560	0.03%	0.004%
64	10.622	2975	2980	2982	rBV2	773	592	0.03%	0.004%
65	10.741	3015	3017	3023	rBV2	575	579	0.03%	0.004%
66	10.841	3045	3048	3056	rVB4	1105	1297	0.06%	0.008%
67	10.882	3056	3061	3064	rVB2	602	516	0.03%	0.003%
68	10.905	3064	3068	3074	rBV2	768	1008	0.05%	0.007%
69	10.947	3078	3081	3085	rBV2	667	480	0.02%	0.003%
70	11.034	3106	3108	3116	rVB4	663	594	0.03%	0.004%
71	11.130	3135	3138	3142	rVB4	1233	796	0.04%	0.005%
72	11.178	3142	3153	3183	rBV	954163	1517238	74.13%	9.903%
73	11.439	3230	3234	3235	rBV2	953	499	0.02%	0.003%
74	11.477	3244	3246	3254	rVB5	717	666	0.03%	0.004%
75	11.551	3258	3269	3296	rBV	929281	1515381	74.04%	9.891%
76	11.905	3377	3379	3383	rVB4	937	554	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV102124\
 Data File : VV037904.D
 Acq On : 21 Oct 2024 17:24
 Operator : SY/MD
 Sample : P4429-12
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

77	12.284	3490	3497	3502	rBV5	1064	1383	0.07%	0.009%
78	12.339	3511	3514	3519	rVB4	863	645	0.03%	0.004%
79	12.477	3555	3557	3560	rBV3	755	482	0.02%	0.003%
80	12.664	3611	3615	3621	rVV4	852	1028	0.05%	0.007%
81	12.741	3635	3639	3646	rVB5	986	1220	0.06%	0.008%
82	12.780	3646	3651	3653	rBV2	918	899	0.04%	0.006%
83	12.796	3653	3656	3660	rVB2	1137	852	0.04%	0.006%
84	12.834	3665	3668	3670	rBV3	870	527	0.03%	0.003%
85	12.882	3681	3683	3687	rVB3	1120	745	0.04%	0.005%
86	13.124	3753	3758	3760	rVB3	932	804	0.04%	0.005%
87	13.143	3760	3764	3765	rBV4	820	575	0.03%	0.004%
88	13.223	3785	3789	3791	rVB5	854	590	0.03%	0.004%
89	13.239	3791	3794	3799	rBV4	911	679	0.03%	0.004%
90	13.316	3816	3818	3822	rVB4	1078	635	0.03%	0.004%
91	13.342	3822	3826	3828	rBV3	700	471	0.02%	0.003%
92	13.686	3930	3933	3940	rVB7	1296	1090	0.05%	0.007%
93	13.767	3955	3958	3959	rBV	919	488	0.02%	0.003%
94	13.821	3973	3975	3979	rVV4	781	634	0.03%	0.004%
95	13.902	3997	4000	4002	rBV	709	473	0.02%	0.003%
96	14.191	4086	4090	4093	rBV4	1349	1096	0.05%	0.007%
97	14.249	4104	4108	4109	rBV4	771	575	0.03%	0.004%
98	14.394	4149	4153	4155	rBV4	787	684	0.03%	0.004%
99	14.429	4160	4164	4168	rBV4	1420	1081	0.05%	0.007%
100	15.332	4443	4445	4447	rBV3	1281	561	0.03%	0.004%




Sum of corrected areas: 15320442

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV102124\
Data File : VV037904.D
Acq On : 21 Oct 2024 17:24
Operator : SY/MD
Sample : P4429-12
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

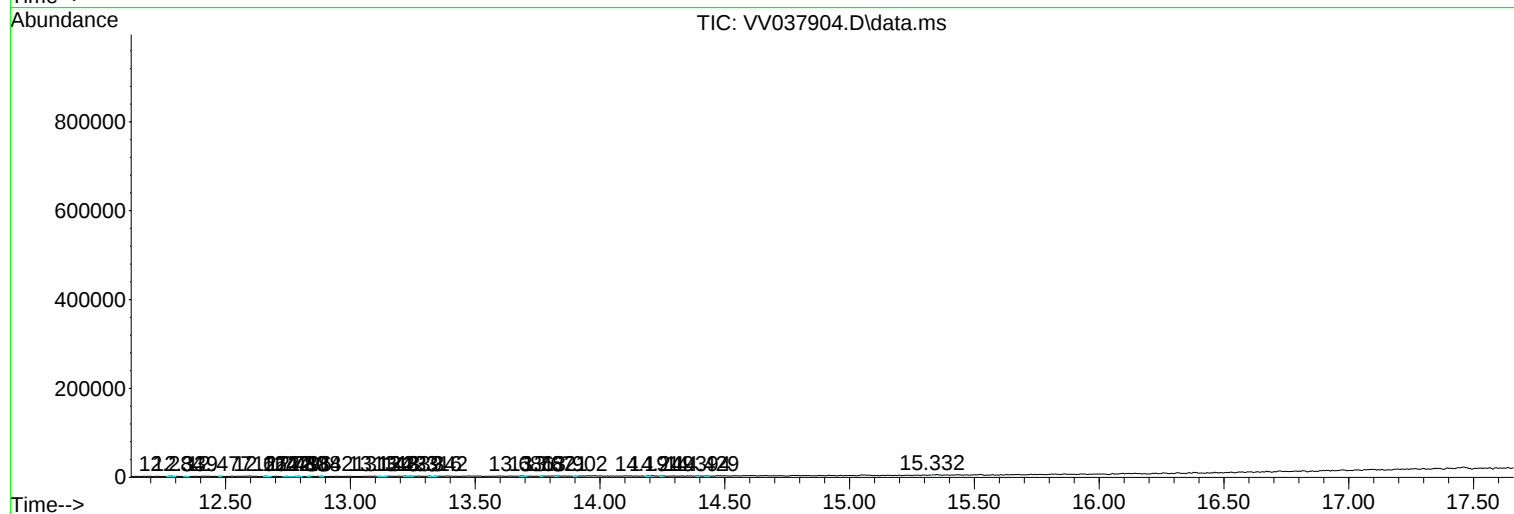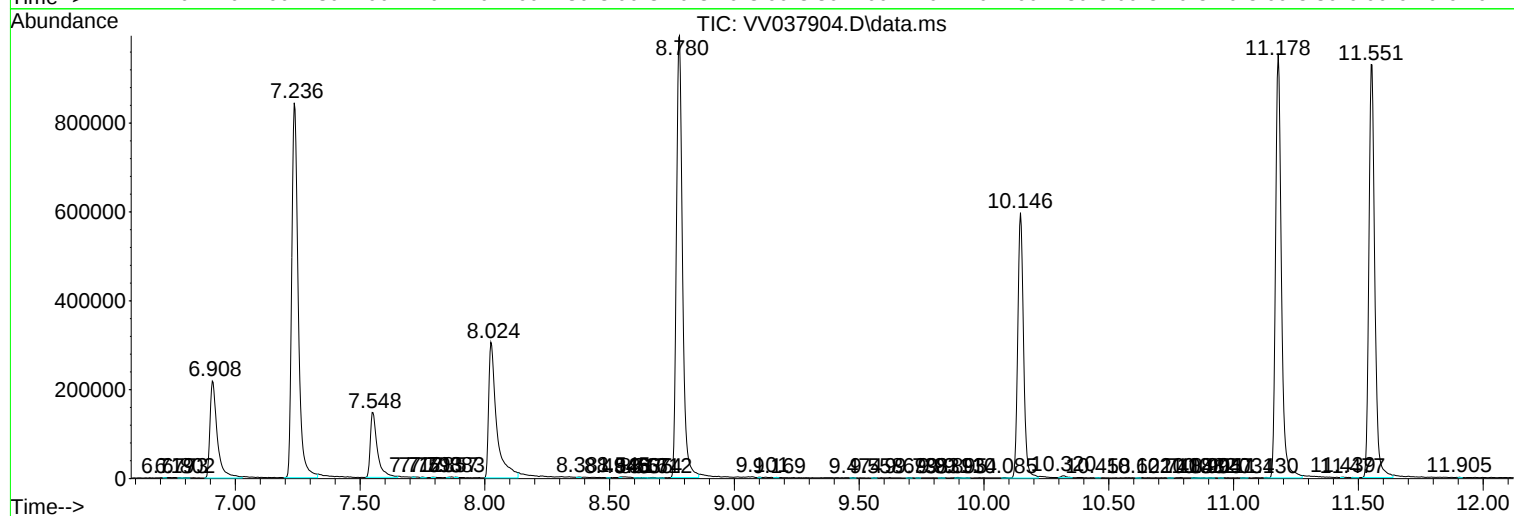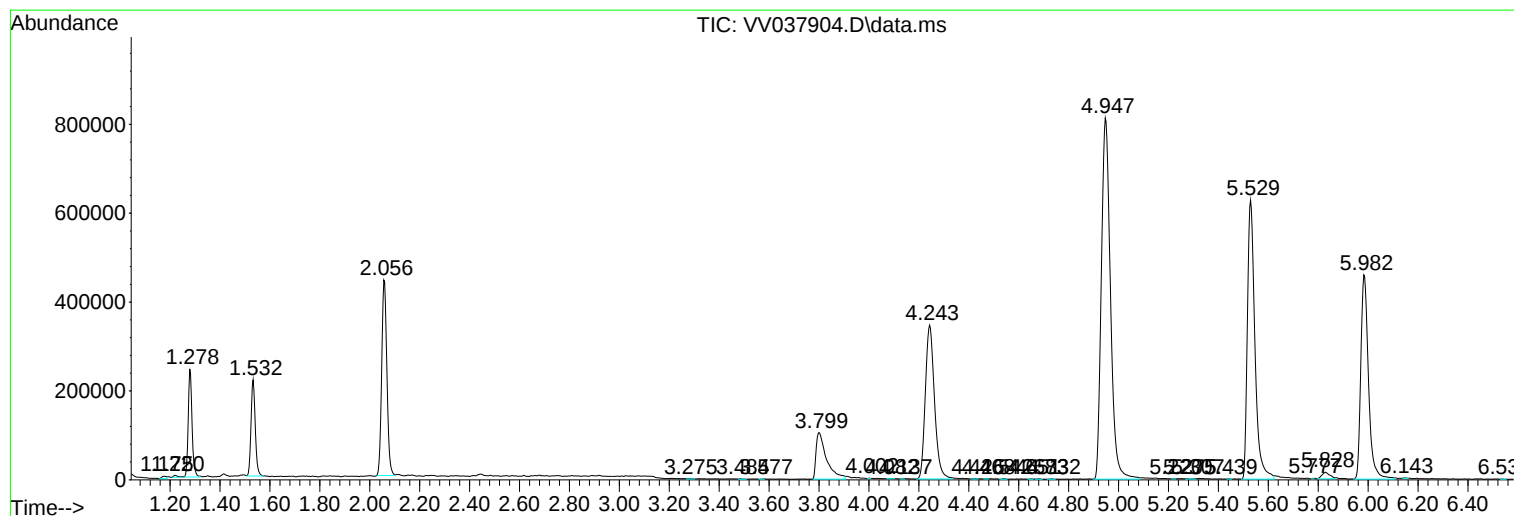

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV102124\
Data File : VV037904.D
Acq On : 21 Oct 2024 17:24
Operator : SY/MD
Sample : P4429-12
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV102124\
Data File : VV037904.D
Acq On : 21 Oct 2024 17:24
Operator : SY/MD
Sample : P4429-12
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc