

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV102125\
 Data File : VV039299.D
 Acq On : 21 Oct 2025 12:45
 Operator : SY/MD
 Sample : Q3390-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 4090

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\82V100725W.M
 Title : SW846 8260

Signal : TIC: VV039299.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.500	1059	1076	1095	rBV	580484	1533437	36.75%	6.616%
2	4.600	1095	1107	1151	rVB	845285	2312482	55.42%	9.977%
3	4.940	1201	1213	1241	rBV2	630528	1544285	37.01%	6.663%
4	5.532	1386	1397	1446	rBV	1318873	2995800	71.80%	12.925%
5	7.236	1916	1927	1970	rBV	2244290	4172664	100.00%	18.002%
6	8.773	2392	2405	2432	rBV	2070240	3502907	83.95%	15.113%
7	10.001	2775	2787	2824	rBV	1633734	2722977	65.26%	11.748%
8	11.172	3138	3151	3180	rBV	2007379	3222360	77.23%	13.902%
9	12.683	3598	3621	3634	rBV	32237	102631	2.46%	0.443%
10	13.053	3728	3736	3751	rBV8	36829	101464	2.43%	0.438%
11	14.046	4035	4045	4081	rBV2	184761	482043	11.55%	2.080%
12	14.554	4193	4203	4211	rBV2	23541	55359	1.33%	0.239%
13	14.992	4330	4339	4351	rBV2	176406	354047	8.48%	1.527%
14	15.889	4611	4618	4627	rBV8	40958	75928	1.82%	0.328%




Sum of corrected areas: 23178384

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV102125\
Data File : VV039299.D
Acq On : 21 Oct 2025 12:45
Operator : SY/MD
Sample : Q3390-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
4090

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\82V100725W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

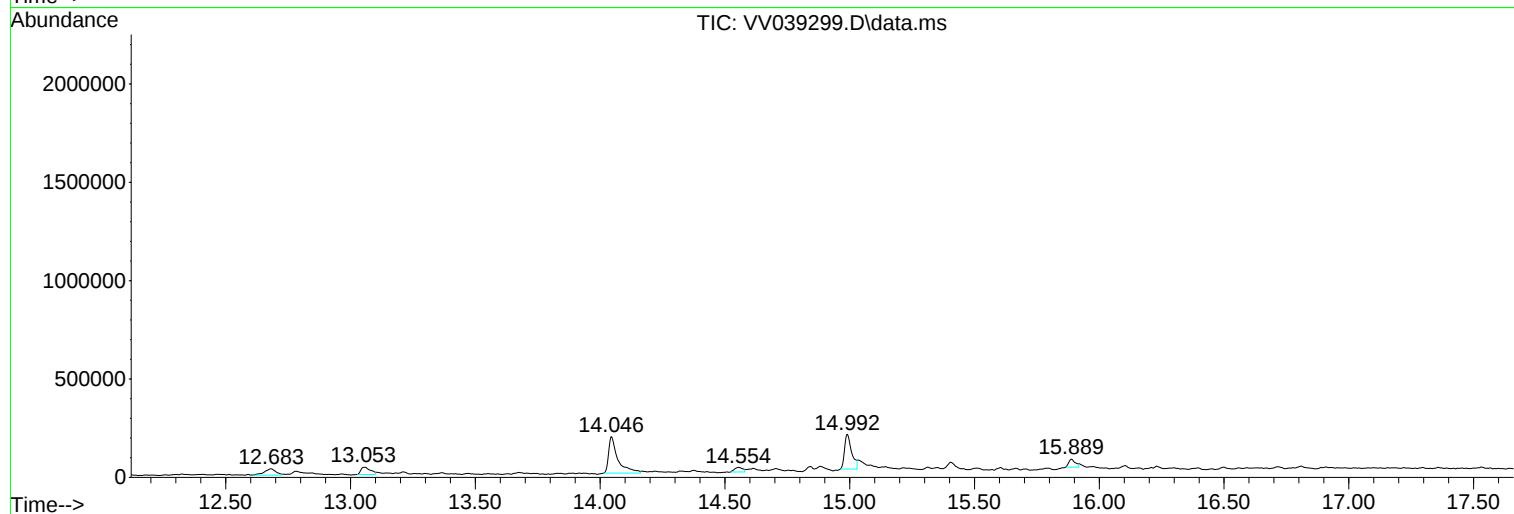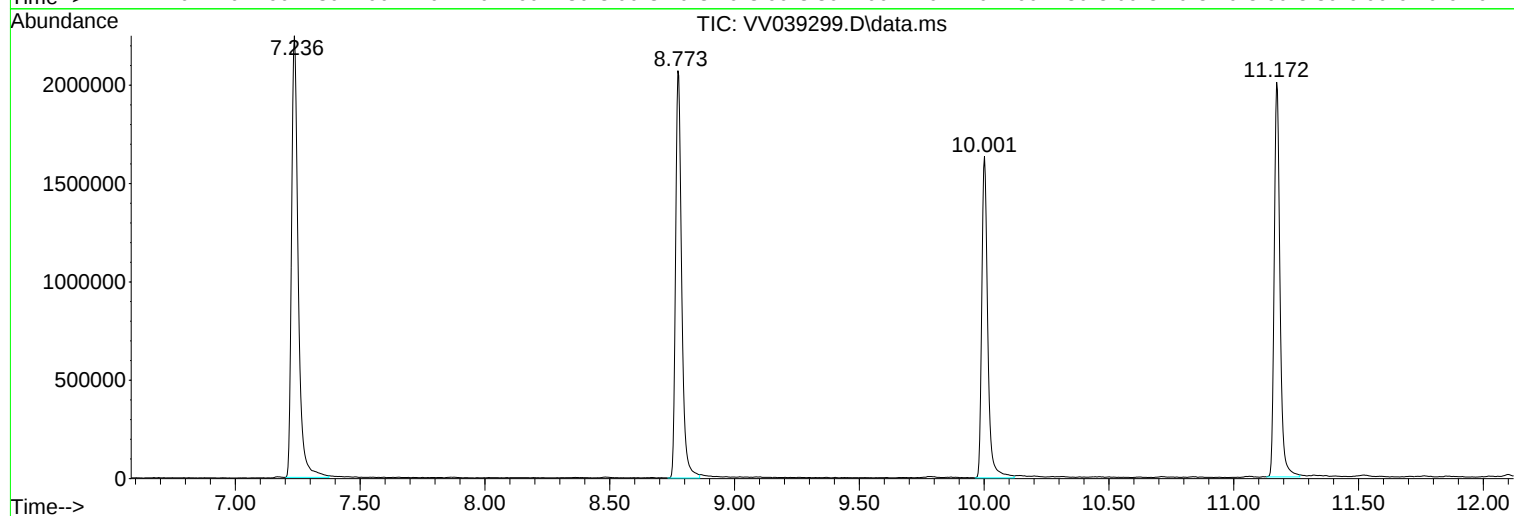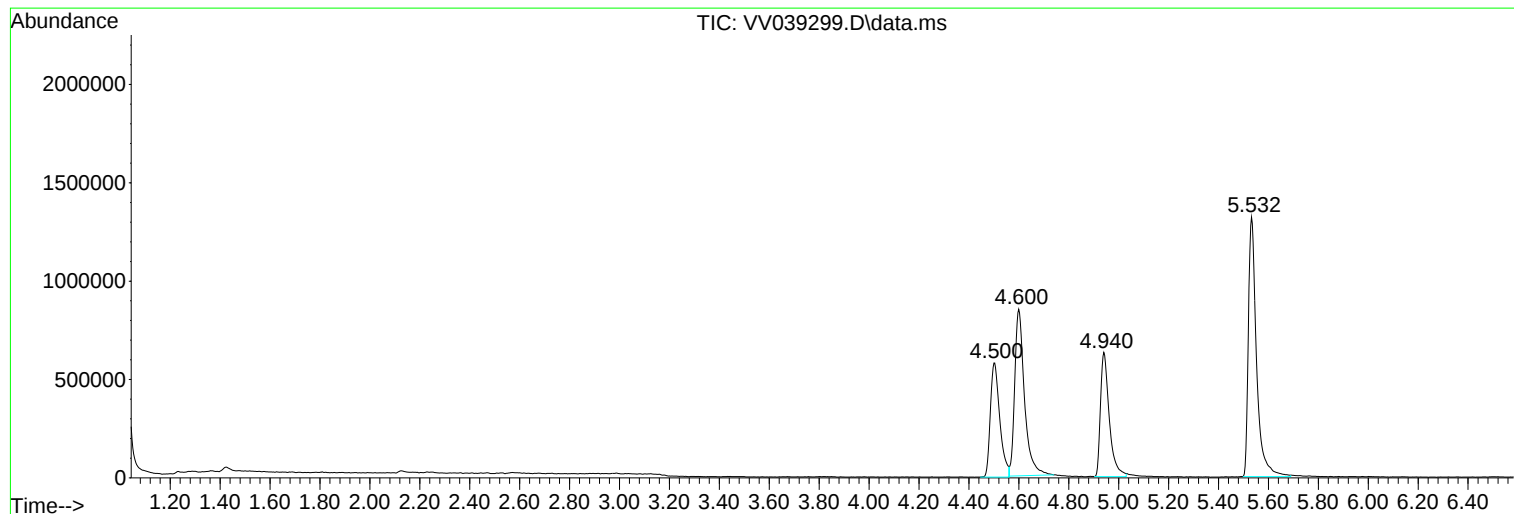

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV102125\
Data File : VV039299.D
Acq On : 21 Oct 2025 12:45
Operator : SY/MD
Sample : Q3390-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
4090










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\82V100725W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Cyclodecane Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.046	7.48 ug/l	482043	1,4-Dichlorobenzene-d4	11.172

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Cyclodecane	140	C10H20	000293-96-9	97
2			1-Decanol	158	C10H22O	000112-30-1	91
3			1-Dodecanol	186	C12H26O	000112-53-8	91
4			1-Undecanol	172	C11H24O	000112-42-5	91
5			1-Dodecene	168	C12H24	000112-41-4	90

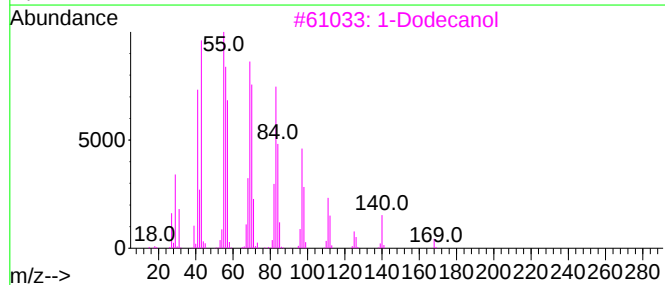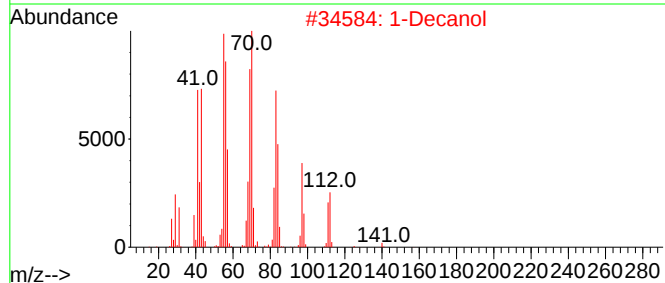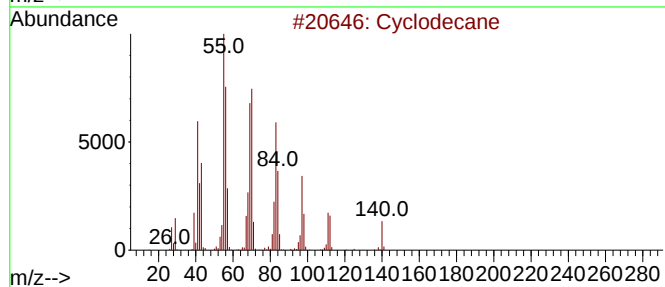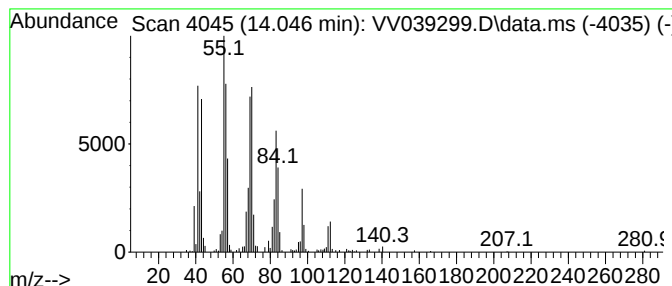

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV102125\
Data File : VV039299.D
Acq On : 21 Oct 2025 12:45
Operator : SY/MD
Sample : Q3390-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
4090










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\82V100725W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 1-Nonene Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.992	5.49 ug/l	354047	1,4-Dichlorobenzene-d4	11.172

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	1-Nonene			126	C9H18	000124-11-8	95
2	1-Undecanol			172	C11H24O	000112-42-5	91
3	1-Tetradecanol			214	C14H30O	000112-72-1	91
4	1-Dodecanol			186	C12H26O	000112-53-8	91
5	n-Tridecan-1-ol			200	C13H28O	000112-70-9	91

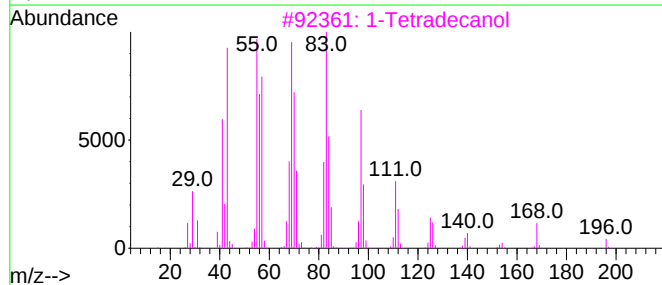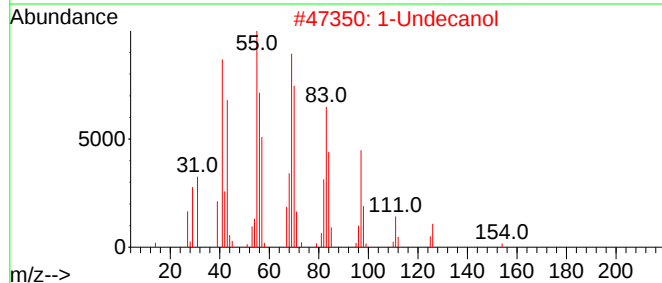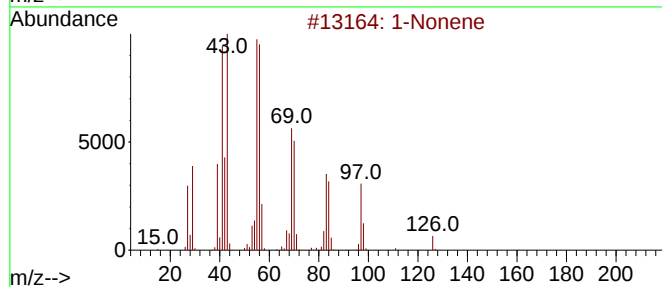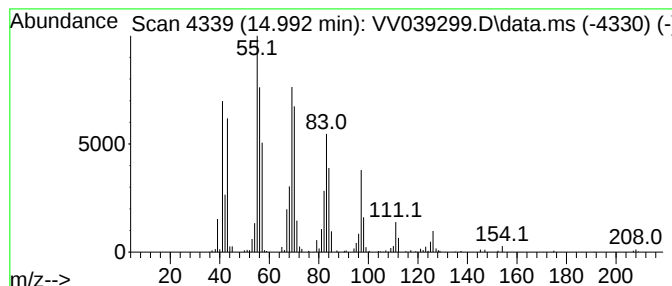

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV102125\
Data File : VV039299.D
Acq On : 21 Oct 2025 12:45
Operator : SY/MD
Sample : Q3390-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
4090

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\82V100725W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Cyclodecane	14.046	7.5	ug/l	482043	4	11.172	3222360	50.0
1-Nonene	14.992	5.5	ug/l	354047	4	11.172	3222360	50.0