
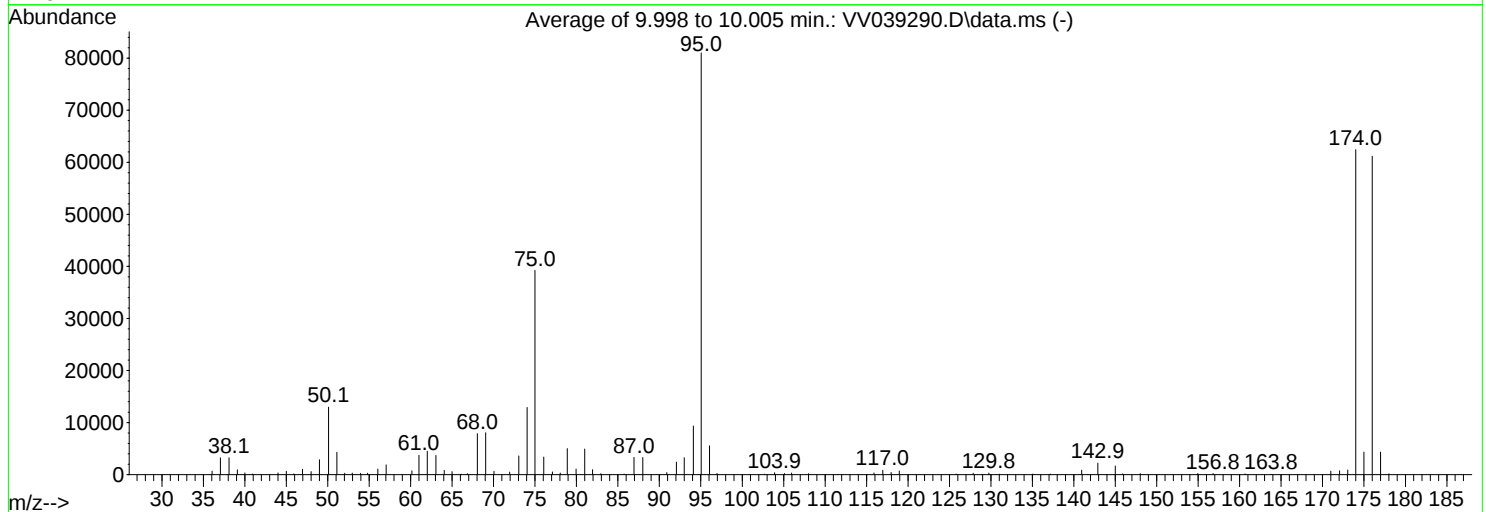


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV102125\
Data File : VV039290.D
Acq On : 21 Oct 2025 08:28
Operator : SY/MD
Sample : BFB
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\82V100725W.M
Title : SW846 8260
Last Update : Wed Oct 08 05:01:26 2025

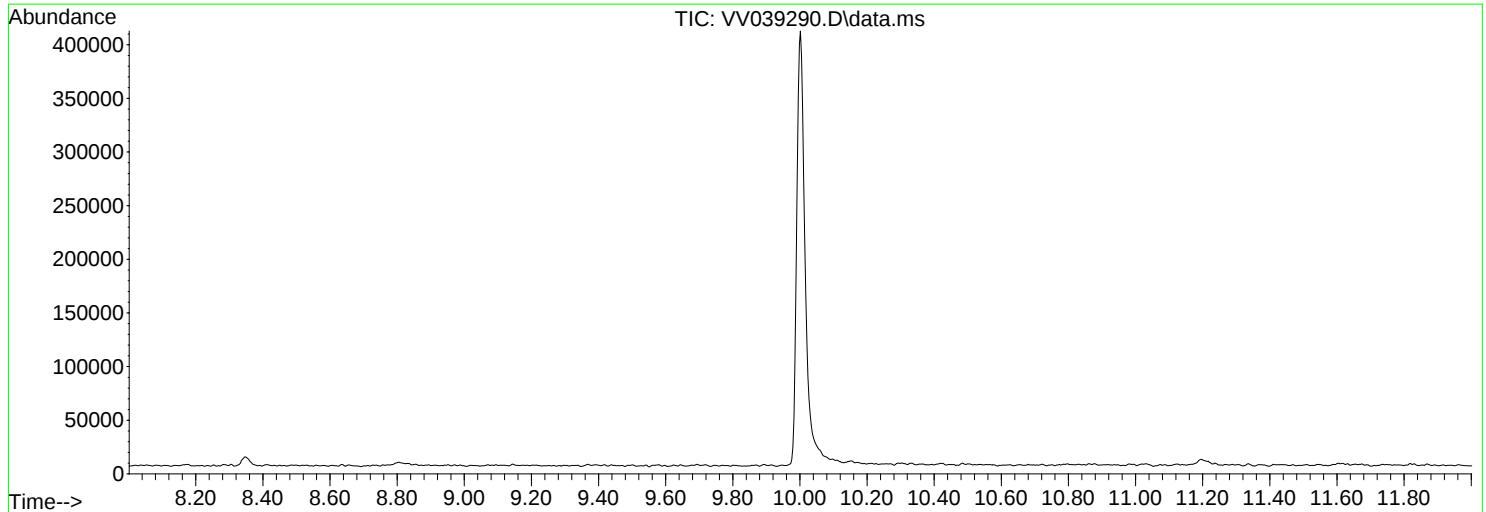

AutoFind: Scans 2786, 2787, 2788; Background Corrected with Scan 2774

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.0	12957	PASS
75	95	30	60	48.4	39240	PASS
95	95	100	100	100.0	81019	PASS
96	95	5	9	6.8	5537	PASS
173	174	0.00	2	1.4	897	PASS
174	95	50	100	77.1	62432	PASS
175	174	5	9	6.9	4330	PASS
176	174	95	101	98.0	61173	PASS
177	176	5	9	7.1	4321	PASS