

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102219\
 Data File : VV013280.D
 Acq On : 22 Oct 2019 15:35
 Operator : SY/MD
 Sample : VIBLK42
 Misc : 25.00ML/MSVOA V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK42

Quant Time: Oct 23 02:12:46 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR102119WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Oct 23 01:23:09 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	455458	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	487679	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	241120	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	182940	5.45	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	109.00%
7) Chloroethane-d5	1.58	69	151461	5.47	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	109.40%
11) 1,1-Dichloroethene-d2	2.13	63	224586	3.76	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	75.20%
20) 2-Butanone-d5	3.97	46	408814	63.40	ug/L	0.03
Spiked Amount	50.000	Range	40 - 130	Recovery	=	126.80%
24) Chloroform-d	4.40	84	391292	4.96	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.20%
26) 1,2-Dichloroethane-d4	5.08	65	184058	5.03	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.60%
32) Benzene-d6	5.10	84	780058	4.94	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.80%
36) 1,2-Dichloropropane-d6	6.12	67	236402	4.98	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	99.60%
41) Toluene-d8	7.36	98	641428	4.39	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.80%
43) trans-1,3-Dichloropropene-	7.66	79	76684	4.26	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	85.20%
46) 2-Hexanone-d5	8.14	63	244142	38.10	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	76.20%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	160119	4.67	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	93.40%
64) 1,2-Dichlorobenzene-d4	11.67	152	255158	5.44	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	108.80%


Target Compounds					Ovalue
16) Methylene chloride	2.53	84	10313	0.192 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV102219\
Data File : VV013280.D
Acq On : 22 Oct 2019 15:35
Operator : SY/MD
Sample : VIBLK42
Misc : 25.00ML/MSVOA V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK42

Quant Time: Oct 23 02:12:46 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR102119WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Oct 23 01:23:09 2019
Response via : Initial Calibration

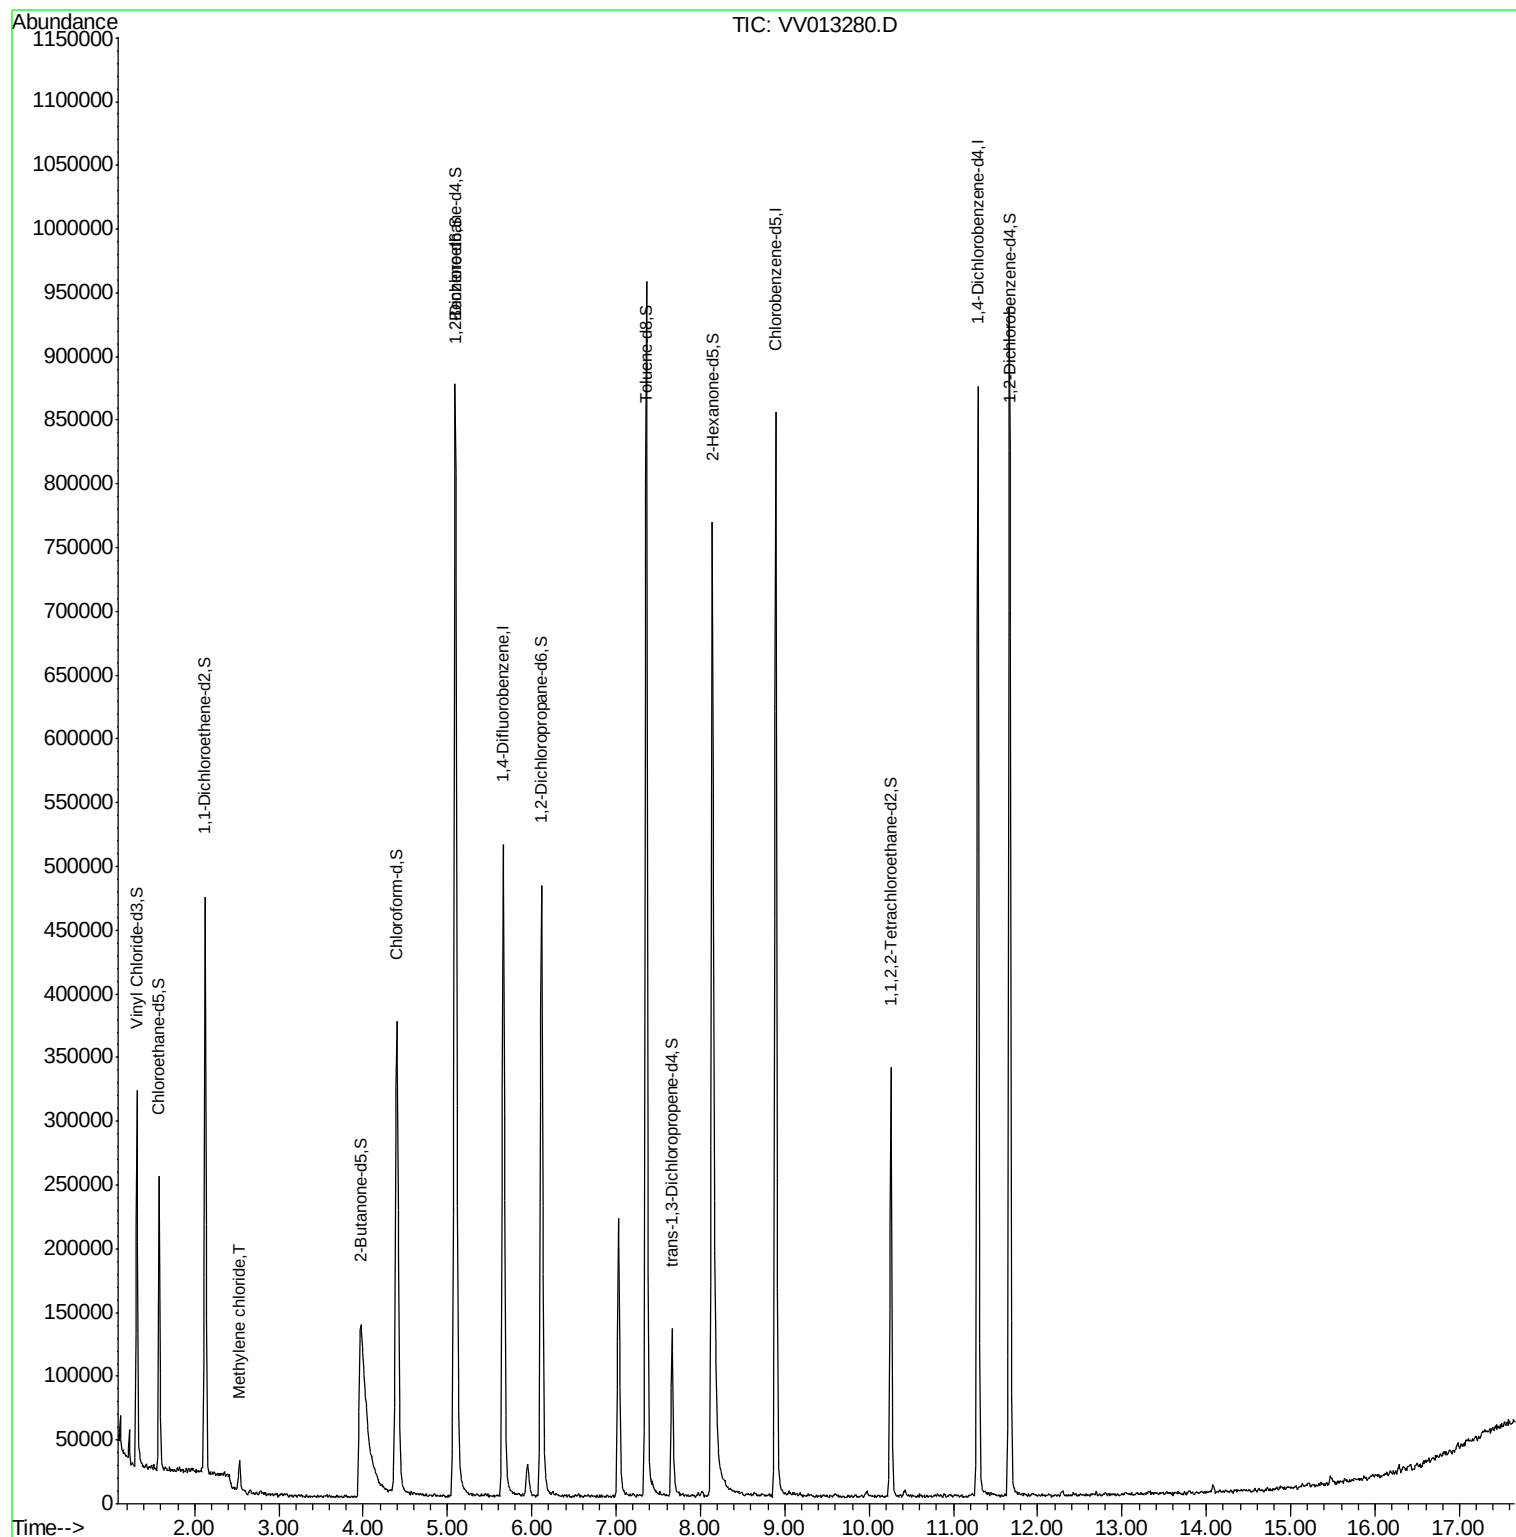

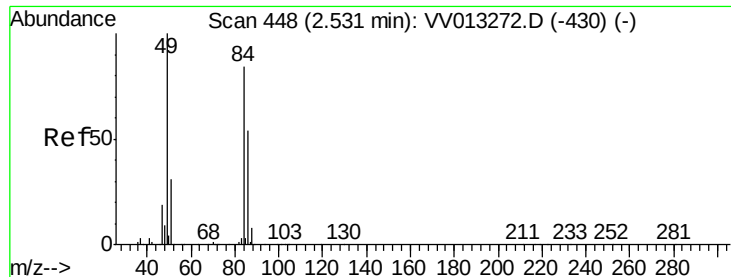

#16
 Methvlene chloride
 Concen: 0.192 ug/L
 RT: 2.53 min Scan# 448
 Delta R.T. 0.00 min
 Lab File: VV013280.D
 Acq: 22 Oct 2019 15:35

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK42

Tot Ion: 84 Resp: 10313
 Ion Ratio Lower Upper
 84 100
 86 63.1 46.2 85.8
 49 108.7 76.4 141.8

