

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102219\
 Data File : VV013287.D
 Acq On : 22 Oct 2019 19:07
 Operator : SY/MD
 Sample : K5404-01
 Misc : 25.00ML/MSVOA V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AA5

Quant Time: Oct 23 03:26:39 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR102119WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Oct 23 01:23:09 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	436600	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	478410	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	251537	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	171084	5.32	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	106.40%
7) Chloroethane-d5	1.58	69	148220	5.58	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	111.60%
11) 1,1-Dichloroethene-d2	2.13	63	217227	3.79	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	75.80%
20) 2-Butanone-d5	3.93	46	369201	59.73	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	119.46%
24) Chloroform-d	4.40	84	355946	4.70	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.00%
26) 1,2-Dichloroethane-d4	5.08	65	170723	4.87	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.40%
32) Benzene-d6	5.10	84	708254	4.57	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.40%
36) 1,2-Dichloropropane-d6	6.12	67	217789	4.68	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	93.60%
41) Toluene-d8	7.36	98	577615	4.03	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	80.60%
43) trans-1,3-Dichloropropene-	7.66	79	67862	3.85	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	77.00%
46) 2-Hexanone-d5	8.13	63	224992	35.80	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	71.60%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	150685	4.48	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	89.60%
64) 1,2-Dichlorobenzene-d4	11.67	152	252524	5.16	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	103.20%


Target Compounds				Ovalue
13) Acetone	2.19	43	43594	13.640 ug/L # 52


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV102219\
Data File : VV013287.D
Acq On : 22 Oct 2019 19:07
Operator : SY/MD
Sample : K5404-01
Misc : 25.00ML/MSVOA V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA5

Quant Time: Oct 23 03:26:39 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR102119WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Oct 23 01:23:09 2019
Response via : Initial Calibration

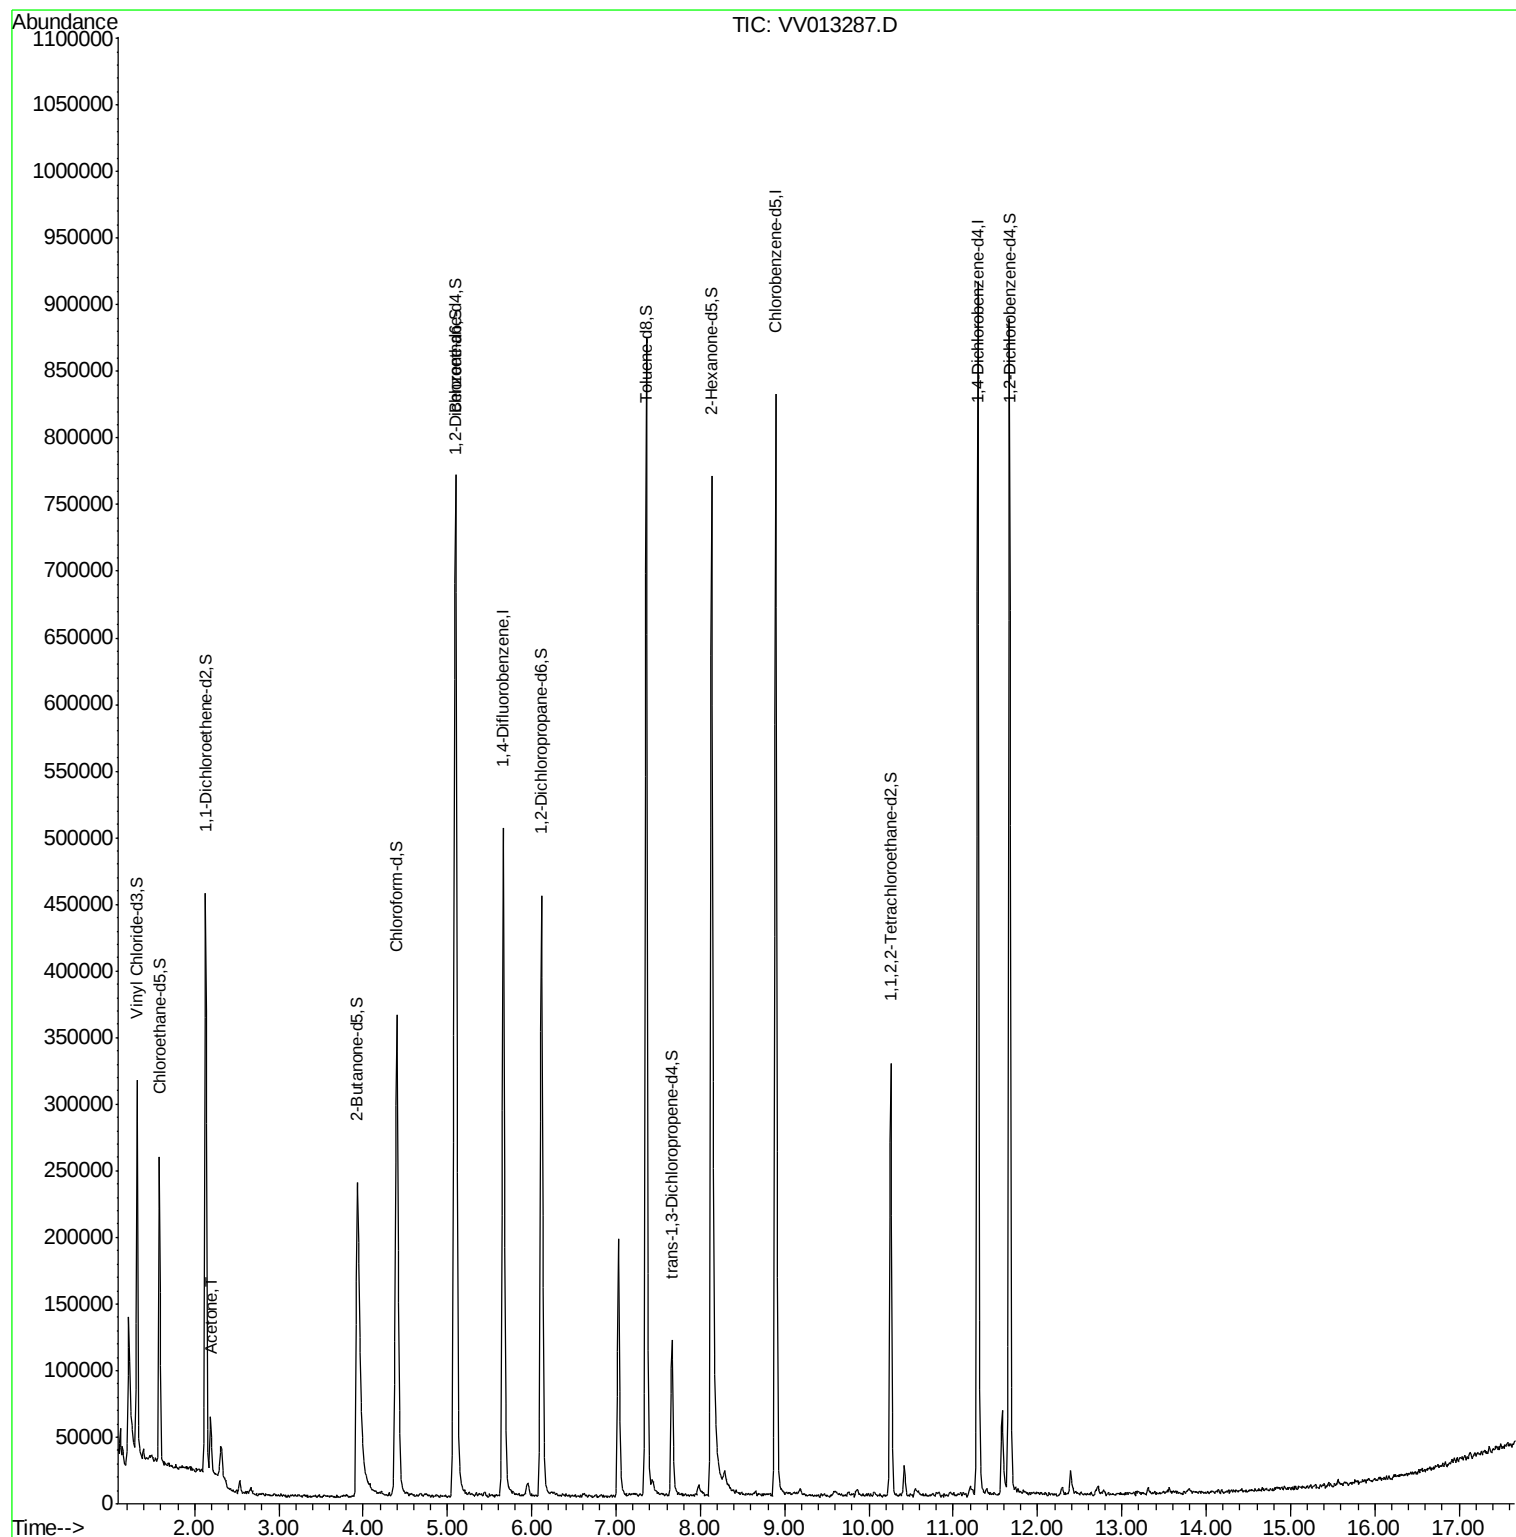

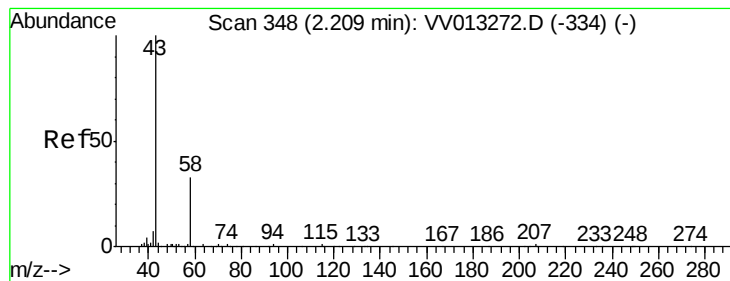

#13

Acetone

Concen: 13.640 ug/L

RT: 2.19 min Scan# 342

Delta R.T. -0.02 min

Lab File: VV013287.D

Acq: 22 Oct 2019 19:07

Instrument :
MSVOA_V
ClientSampleId :
C0AA5

Tot Ion: 43 Resp: 43594

Ion Ratio Lower Upper

43 100

58 32.4 0.0 26.2#

