


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV102219\
 Data File : VV013271.D
 Acq On : 22 Oct 2019 09:14
 Operator : SY/MD
 Sample : BFB46
 Misc : 25.00ML/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB46

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR102119WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Wed Oct 23 18:04:59 2019

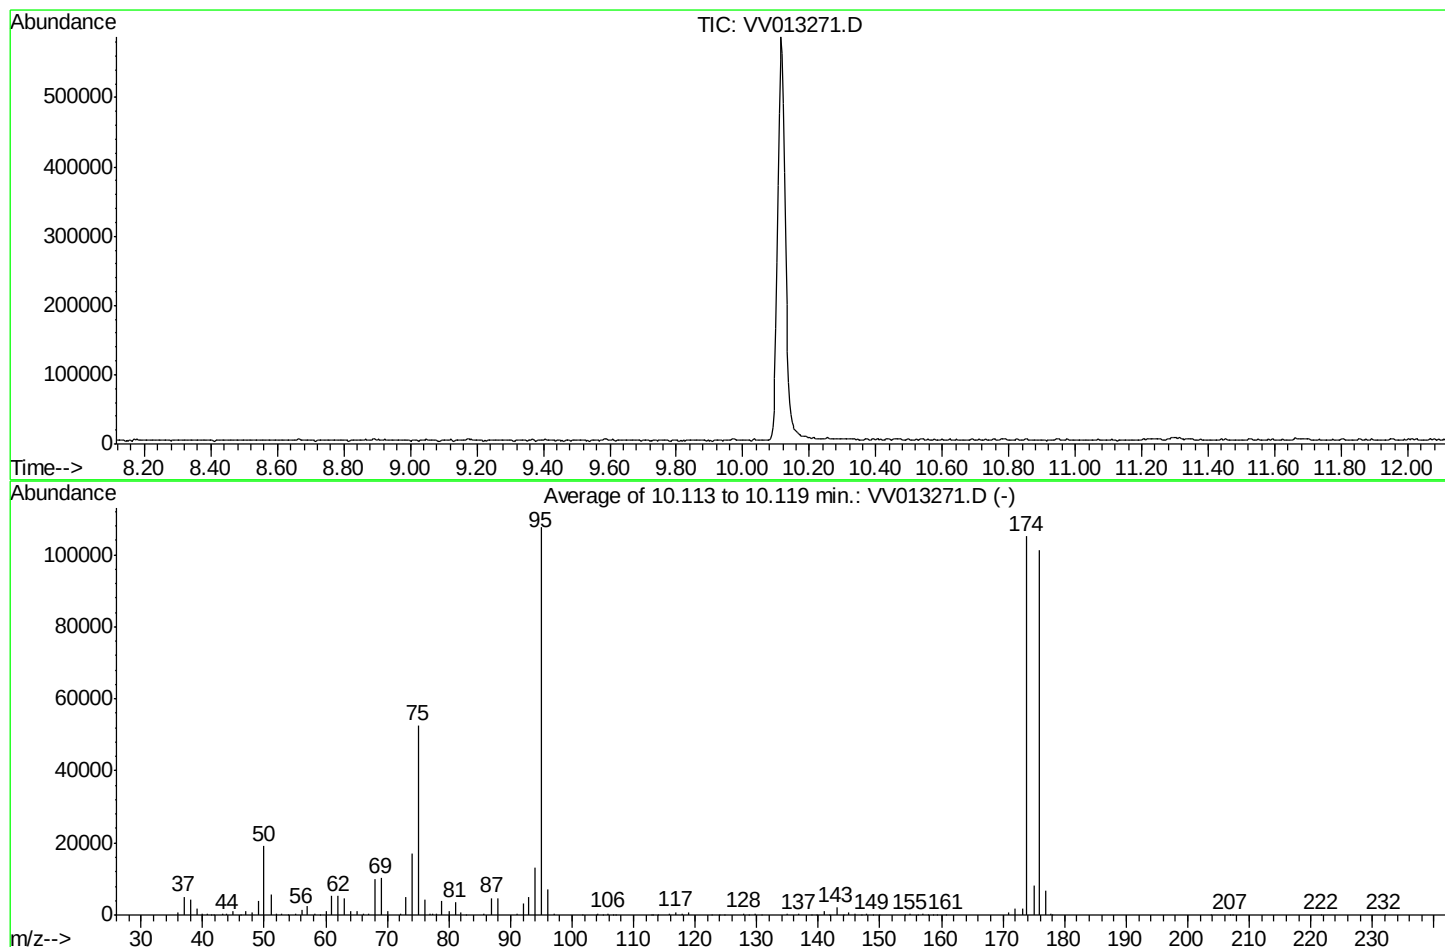

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2793

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.8	19157	PASS
75	95	30	80	48.8	52565	PASS
95	95	100	100	100.0	107632	PASS
96	95	5	9	6.7	7170	PASS
173	174	0.00	2	1.9	1962	PASS
174	95	50	120	97.6	105040	PASS
175	174	5	9	7.9	8289	PASS
176	174	95	101	96.4	101309	PASS
177	176	5	9	6.8	6853	PASS

m/z	Abundance
36.00	898.0
37.00	5162.0
38.00	4623.0
39.10	2064.0
39.90	1846.0
40.80	229.0
41.80	104.0
42.30	110.0
43.10	220.0
44.00	1943.0
45.00	1050.0
46.30	184.0
47.00	1025.0
48.10	788.0
49.00	4002.0
50.00	18904.0
51.10	5488.0
52.00	294.0
52.90	218.0
54.00	144.0
55.00	328.0
56.00	1413.0
57.00	2547.0
58.20	215.0
59.10	117.0
60.10	1098.0
61.00	5156.0
62.00	5172.0
63.00	4989.0
64.10	991.0
65.00	1117.0
66.10	261.0
67.00	350.0
68.00	10208.0
69.00	10081.0
70.00	891.0
72.10	458.0
73.00	4870.0
74.00	16536.0
75.00	51984.0
76.00	4198.0
76.90	534.0
77.30	403.0
78.00	379.0
78.90	3761.0
80.00	1046.0
81.00	3424.0
81.90	749.0
82.90	125.0
85.80	202.0
87.00	4418.0
88.00	4359.0
91.00	548.0
92.00	2966.0
93.00	4760.0
94.00	13344.0
95.00	104656.0
96.00	7385.0
97.00	214.0
101.60	109.0
103.90	473.0
105.00	129.0
105.80	555.0
106.70	140.0
115.70	410.0
116.90	897.0
117.80	433.0
118.80	744.0
122.70	147.0
123.80	111.0
124.80	108.0
127.90	572.0
128.80	168.0
129.60	304.0
130.80	143.0
134.90	254.0
136.90	370.0
140.90	1120.0
143.00	2078.0
144.10	181.0
144.80	847.0
145.90	255.0
147.00	156.0
147.80	356.0
149.90	125.0
154.90	323.0
156.00	104.0
156.90	170.0
159.10	101.0
170.90	527.0
171.90	1667.0
173.10	1824.0

Instrument :
MSVOA_V
ClientSampleId :
BFB46

173.90	100184.0
175.00	8605.0
175.90	97304.0
177.00	6696.0
177.80	320.0
206.90	216.0

Instrument :
MSVOA_V
ClientSampleId :
BFB46

m/z	Abundance
36.00	942.0
37.00	5400.0
38.00	4743.0
39.10	2192.0
39.90	1875.0
40.80	203.0
43.20	234.0
44.00	1808.0
44.90	940.0
46.20	141.0
47.00	1304.0
47.90	752.0
49.00	3926.0
50.00	19816.0
51.10	5676.0
52.00	305.0
52.80	234.0
54.00	192.0
55.00	435.0
56.10	1518.0
57.00	2731.0
58.20	219.0
59.10	111.0
60.00	1027.0
61.00	5589.0
62.00	5493.0
63.00	4936.0
64.00	932.0
65.00	1162.0
66.10	248.0
67.10	356.0
68.00	10404.0
69.00	10510.0
70.00	968.0
72.10	563.0
73.00	5126.0
74.00	17504.0
75.00	54512.0
76.00	4331.0
76.80	428.0
77.30	320.0
78.10	375.0
78.90	3856.0
79.90	1123.0
81.00	3539.0
81.90	736.0
82.80	140.0
85.70	221.0
87.00	4837.0
88.00	4911.0
91.00	464.0
92.00	3141.0
93.00	5197.0
94.00	13342.0
95.00	111384.0
96.00	7403.0
97.10	249.0
104.10	415.0
105.00	160.0
105.90	520.0
107.00	152.0
112.80	114.0
113.20	121.0
114.00	115.0
115.80	417.0
116.90	843.0
117.80	453.0
118.90	828.0
123.90	101.0
127.90	443.0
128.70	154.0
129.70	312.0
130.80	188.0
135.00	243.0
136.90	378.0
139.80	104.0
140.90	1128.0
141.70	140.0
143.00	2214.0
144.10	132.0
144.90	821.0
145.80	269.0
147.00	179.0
147.80	341.0
148.90	115.0
149.90	131.0
154.00	122.0
155.00	364.0
156.10	114.0
156.90	207.0
157.80	118.0
158.70	129.0

Instrument :
MSVOA_V
ClientSampleId :
BFB46

159.20	131.0
170.90	610.0
172.00	1761.0
173.10	2031.0
173.90	108672.0
175.00	8490.0
175.90	104760.0
177.00	7039.0
177.80	256.0
206.90	181.0
221.70	104.0

Instrument :
MSVOA_V
ClientSampleId :
BFB46

m/z	Abundance
36.00	898.0
37.00	4732.0
38.00	4119.0
39.00	2124.0
39.90	1794.0
40.80	169.0
41.40	128.0
42.20	107.0
43.20	219.0
44.00	1731.0
44.90	779.0
46.10	116.0
47.00	1457.0
47.90	681.0
49.00	3581.0
50.00	18752.0
51.10	5416.0
52.00	305.0
52.80	200.0
53.90	292.0
55.00	437.0
56.00	1498.0
57.00	2447.0
58.20	202.0
60.00	898.0
61.00	4981.0
62.00	5219.0
63.00	4495.0
63.90	896.0
65.00	1132.0
66.00	185.0
67.10	364.0
68.00	9751.0
69.00	10008.0
70.00	848.0
72.00	595.0
73.00	4677.0
74.00	17136.0
75.00	51200.0
76.00	4115.0
78.10	343.0
78.90	3872.0
79.90	1147.0
81.00	3482.0
81.90	722.0
82.80	121.0
85.60	184.0
87.00	4705.0
88.00	4951.0
91.00	395.0
92.00	3125.0
93.00	4849.0
94.00	12843.0
95.00	106856.0
96.00	6723.0
97.10	261.0
104.10	378.0
105.00	230.0
105.90	503.0
107.00	157.0
112.80	145.0
113.20	110.0
114.00	138.0
115.80	443.0
116.90	836.0
117.80	455.0
118.90	864.0
127.80	301.0
128.80	170.0
129.80	318.0
130.90	209.0
135.10	231.0
136.90	305.0
138.90	102.0
139.80	104.0
140.90	968.0
141.70	159.0
143.00	2034.0
144.90	906.0
145.80	285.0
146.90	164.0
147.80	298.0
148.80	138.0
149.90	112.0
154.00	125.0
155.00	404.0
156.10	108.0
157.00	228.0
157.80	122.0
158.70	129.0
159.20	134.0
160.80	112.0

Instrument :
MSVOA_V
ClientSampleId :
BFB46

170.90	604.0
172.00	1712.0
173.10	2031.0
173.90	106264.0
175.00	7773.0
175.90	101864.0
177.00	6824.0
178.00	183.0
203.70	104.0
206.90	101.0
207.30	111.0
232.00	109.0

Instrument :
MSVOA_V
ClientSampleId :
BFB46

m/z	Abundance
35.60	205.0
36.20	165.0
38.00	144.0
38.70	153.0
39.00	167.0
39.90	1354.0
42.10	130.0
43.90	1494.0
45.50	115.0
46.80	126.0
51.60	102.0
54.00	111.0
55.20	155.0
59.50	165.0
64.50	158.0
66.40	128.0
71.40	177.0
77.60	108.0
78.20	115.0
82.10	176.0
88.10	104.0
91.50	115.0
96.60	121.0
126.30	103.0
155.10	114.0
207.10	118.0
240.40	124.0

Instrument :
MSVOA_V
ClientSampleId :
BFB46