

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102220\
 Data File : VV019082.D
 Acq On : 22 Oct 2020 20:58
 Operator : SY/MD
 Sample : VIBLK67
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK67

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102220WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	83	rVB	201207	199981	15.17%	2.020%
2	1.579	146	152	167	rVB	175607	195652	14.84%	1.976%
3	2.122	312	321	354	rVB	342496	525061	39.83%	5.303%
4	2.434	415	418	419	rBV	496	235	0.02%	0.002%
5	2.881	554	557	561	rBV	432	427	0.03%	0.004%
6	3.434	727	729	734	rVV	254	166	0.01%	0.002%
7	3.473	737	741	744	rBV2	450	312	0.02%	0.003%
8	3.534	757	760	763	rBV	221	168	0.01%	0.002%
9	3.563	767	769	771	rBV	180	74	0.01%	0.001%
10	3.621	780	787	788	rBV2	291	283	0.02%	0.003%
11	3.646	793	795	799	rVB2	138	85	0.01%	0.001%
12	3.675	799	804	809	rBV2	246	312	0.02%	0.003%
13	3.724	816	819	820	rBV2	299	119	0.01%	0.001%
14	3.736	820	823	825	rVV	315	240	0.02%	0.002%
15	3.762	828	831	838	rBV	192	167	0.01%	0.002%
16	3.788	838	839	840	rBV	228	81	0.01%	0.001%
17	3.862	857	862	865	rBV3	352	364	0.03%	0.004%
18	3.923	870	881	921	rBV	82863	274483	20.82%	2.772%
19	4.376	1007	1022	1058	rVB	210693	518871	39.36%	5.240%
20	4.672	1109	1114	1115	rBV3	414	368	0.03%	0.004%
21	4.714	1125	1127	1129	rBV2	348	162	0.01%	0.002%
22	4.984	1206	1211	1214	rBV2	427	431	0.03%	0.004%
23	5.071	1221	1238	1270	rBV2	522006	1318267	100.00%	13.314%
24	5.296	1307	1308	1312	rVB2	430	275	0.02%	0.003%
25	5.376	1331	1333	1337	rVB3	452	299	0.02%	0.003%
26	5.470	1360	1362	1363	rBV	321	109	0.01%	0.001%
27	5.537	1380	1383	1385	rBV3	365	284	0.02%	0.003%
28	5.640	1403	1415	1440	rBV	373282	745870	56.58%	7.533%
29	5.933	1500	1506	1507	rBV3	1420	1373	0.10%	0.014%
30	6.023	1533	1534	1535	rBV3	239	74	0.01%	0.001%
31	6.093	1543	1556	1588	rBV2	293110	597057	45.29%	6.030%
32	6.495	1679	1681	1682	rBV	444	177	0.01%	0.002%
33	6.537	1691	1694	1698	rBV3	283	238	0.02%	0.002%
34	6.585	1707	1709	1711	rBV2	164	70	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102220\
 Data File : VV019082.D
 Acq On : 22 Oct 2020 20:58
 Operator : SY/MD
 Sample : VIBLK67
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK67

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102220WMA.M
 Title : VOC Analysis

35	6.598	1711	1713	1715	rBV	173	76	0.01%	0.001%
36	6.656	1729	1731	1733	rBV	206	124	0.01%	0.001%
37	6.701	1740	1745	1748	rBV2	433	484	0.04%	0.005%
38	6.775	1764	1768	1776	rVB3	352	504	0.04%	0.005%
39	6.817	1779	1781	1788	rVB3	446	263	0.02%	0.003%
40	7.006	1829	1840	1867	rBV	162165	297706	22.58%	3.007%
41	7.338	1930	1943	1970	rBV	601835	1025567	77.80%	10.358%
42	7.601	2022	2025	2028	rBV3	378	281	0.02%	0.003%
43	7.643	2028	2038	2066	rVV	123081	211190	16.02%	2.133%
44	7.949	2130	2133	2136	rBV2	328	192	0.01%	0.002%
45	7.990	2143	2146	2147	rBV2	370	212	0.02%	0.002%
46	8.029	2155	2158	2160	rBV	336	235	0.02%	0.002%
47	8.109	2172	2183	2223	rBV	349163	614747	46.63%	6.209%
48	8.569	2321	2326	2330	rBV2	369	423	0.03%	0.004%
49	8.820	2402	2404	2407	rBV2	293	189	0.01%	0.002%
50	8.871	2408	2420	2444	rBV	578506	940418	71.34%	9.498%
51	9.039	2470	2472	2476	rBV4	399	143	0.01%	0.001%
52	9.151	2504	2507	2510	rBV	214	146	0.01%	0.001%
53	9.167	2510	2512	2514	rBV	209	94	0.01%	0.001%
54	9.193	2518	2520	2528	rVV2	455	546	0.04%	0.006%
55	9.289	2547	2550	2553	rBV2	277	211	0.02%	0.002%
56	9.338	2563	2565	2569	rBV2	319	171	0.01%	0.002%
57	9.389	2579	2581	2582	rBV	172	61	0.00%	0.001%
58	9.598	2644	2646	2647	rBV	160	67	0.01%	0.001%
59	9.762	2693	2697	2700	rBV2	296	281	0.02%	0.003%
60	9.794	2704	2707	2708	rBV	181	80	0.01%	0.001%
61	9.907	2739	2742	2743	rBV2	380	225	0.02%	0.002%
62	10.135	2810	2813	2815	rBV	204	92	0.01%	0.001%
63	10.148	2815	2817	2820	rVV	278	138	0.01%	0.001%
64	10.238	2833	2845	2865	rBV	381728	595947	45.21%	6.019%
65	10.405	2891	2897	2899	rBV3	667	567	0.04%	0.006%
66	10.521	2931	2933	2937	rVB	542	263	0.02%	0.003%
67	10.817	3022	3025	3028	rBV2	352	269	0.02%	0.003%
68	11.067	3100	3103	3106	rBV	266	177	0.01%	0.002%
69	11.087	3106	3109	3110	rBV2	456	217	0.02%	0.002%
70	11.164	3131	3133	3137	rBV2	465	340	0.03%	0.003%
71	11.206	3142	3146	3148	rBV4	580	508	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102220\
Data File : VV019082.D
Acq On : 22 Oct 2020 20:58
Operator : SY/MD
Sample : VIBLK67
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK67

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102220WMA.M
Title : VOC Analysis

72	11.270	3154	3166	3193	rBV	564870	873794	66.28%	8.825%
73	11.553	3249	3254	3257	rBV	526	494	0.04%	0.005%
74	11.591	3263	3266	3267	rBV2	418	253	0.02%	0.003%
75	11.646	3271	3283	3309	rVV	601394	937248	71.10%	9.466%
76	12.582	3572	3574	3577	rBV	390	203	0.02%	0.002%
77	12.691	3606	3608	3611	rBV	353	227	0.02%	0.002%
78	12.836	3651	3653	3655	rBV	227	131	0.01%	0.001%
79	13.286	3788	3793	3802	rVB4	5128	6987	0.53%	0.071%
80	13.543	3871	3873	3874	rBV4	571	290	0.02%	0.003%
81	13.768	3938	3943	3957	rVB7	3584	5864	0.44%	0.059%
82	13.820	3957	3959	3965	rBV	529	563	0.04%	0.006%


Sum of corrected areas: 9901343

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV102220\
Data File : VV019082.D
Acq On : 22 Oct 2020 20:58
Operator : SY/MD
Sample : VIBLK67
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK67

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102220WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

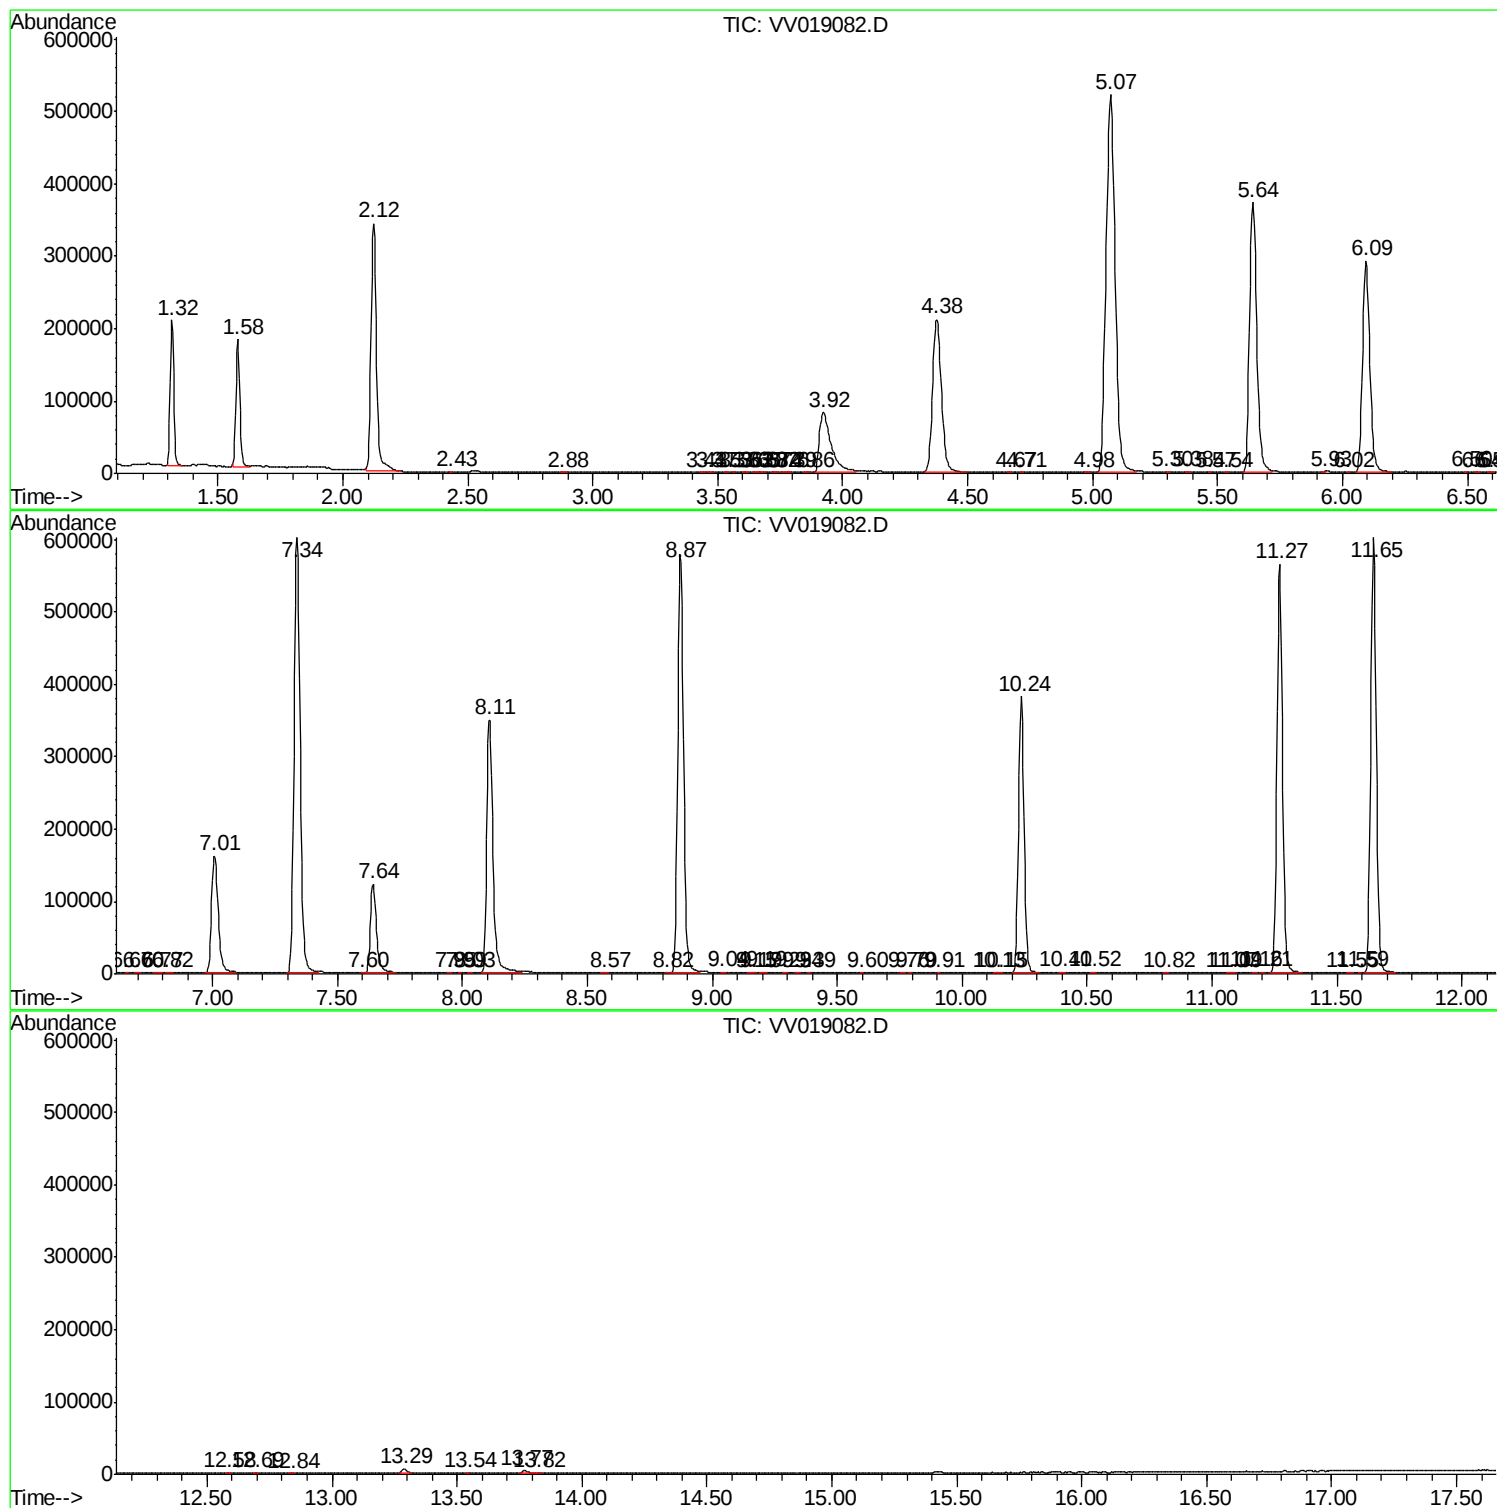

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV102220\
Data File : VV019082.D
Acq On : 22 Oct 2020 20:58
Operator : SY/MD
Sample : VIBLK67
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK67

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102220WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV102220\
Data File : VV019082.D
Acq On : 22 Oct 2020 20:58
Operator : SY/MD
Sample : VIBLK67
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK67

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102220WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc