


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV102220\
 Data File : VV019063.D
 Acq On : 22 Oct 2020 10:54
 Operator : SY/MD
 Sample : BFB80
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB80

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM101420WMA.M
 Title : VOC Analysis
 Last Update : Fri Oct 23 11:29:18 2020

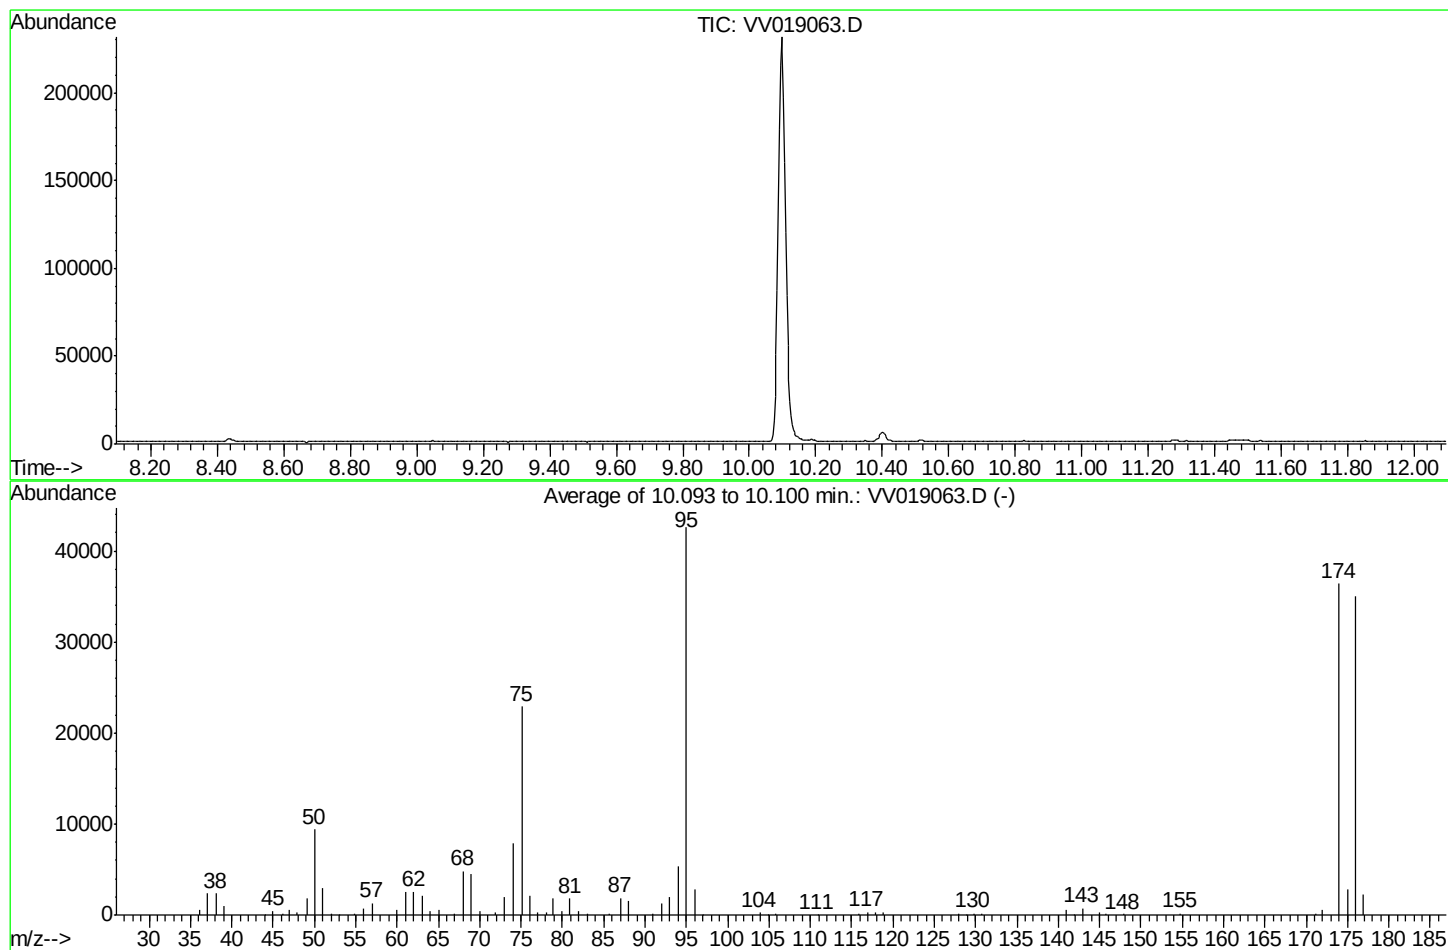

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2790

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.0	9375	PASS
75	95	30	80	53.7	22874	PASS
95	95	100	100	100.0	42605	PASS
96	95	5	9	6.7	2847	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	85.5	36418	PASS
175	174	5	9	7.7	2813	PASS
176	174	95	101	96.1	34984	PASS
177	176	5	9	6.6	2316	PASS

m/z	Abundance
36.00	522.0
37.10	2319.0
38.00	2241.0
39.00	1057.0
39.90	292.0
44.00	1145.0
45.00	455.0
46.00	165.0
47.00	520.0
47.90	330.0
49.00	1863.0
50.00	9158.0
51.00	2902.0
52.00	138.0
54.90	193.0
56.00	844.0
57.00	1301.0
60.00	547.0
61.00	2535.0
62.00	2515.0
63.00	2090.0
64.00	362.0
65.00	546.0
66.90	146.0
68.00	4744.0
69.00	4341.0
70.00	365.0
71.90	303.0
73.00	1980.0
74.00	7659.0
75.10	22296.0
76.00	2085.0
77.10	282.0
78.00	274.0
78.90	1902.0
79.90	452.0
80.90	1710.0
81.90	435.0
83.10	123.0
87.00	1931.0
88.00	1485.0
90.90	156.0
92.00	1280.0
93.00	2005.0
94.00	5149.0
95.00	40896.0
96.00	2845.0
96.90	110.0
103.90	190.0
105.80	182.0
110.90	112.0
115.80	159.0
116.90	365.0
117.80	232.0
118.80	264.0
128.00	204.0
128.90	107.0
129.80	190.0
130.80	125.0
140.90	462.0
141.80	104.0
142.90	719.0
144.90	237.0
145.70	102.0
147.80	101.0
154.80	154.0
171.20	112.0
171.90	507.0
174.00	34520.0
175.00	2744.0
176.00	33008.0
177.00	2171.0

Instrument :
MSVOA_V
ClientSampleId :
BFB80

m/z	Abundance
36.00	536.0
37.10	2457.0
38.10	2495.0
39.00	1068.0
39.90	299.0
44.00	1185.0
45.00	463.0
46.10	173.0
47.00	504.0
47.90	321.0
49.10	1935.0
50.00	9725.0
51.00	3015.0
52.00	174.0
54.90	197.0
56.00	749.0
57.00	1318.0
60.00	583.0
61.00	2690.0
62.00	2708.0
63.00	2167.0
64.00	362.0
65.00	583.0
66.90	134.0
68.00	5024.0
69.00	4736.0
70.00	413.0
71.90	276.0
73.00	2053.0
74.00	8214.0
75.10	23584.0
76.00	2179.0
77.00	251.0
78.10	230.0
78.90	1991.0
79.90	489.0
80.90	1846.0
81.90	488.0
83.10	110.0
85.70	106.0
87.00	1943.0
88.00	1643.0
91.00	170.0
92.00	1347.0
93.00	2024.0
94.00	5547.0
95.00	43992.0
96.00	2946.0
97.00	105.0
103.90	222.0
105.80	215.0
115.90	175.0
116.90	352.0
117.80	231.0
118.80	291.0
127.90	196.0
128.90	109.0
129.80	215.0
130.80	130.0
140.90	545.0
141.90	104.0
142.90	745.0
145.00	225.0
145.80	135.0
147.90	131.0
154.80	173.0
171.20	150.0
171.90	553.0
174.00	37696.0
175.00	2921.0
176.00	36320.0
176.90	2383.0

Instrument :
MSVOA_V
ClientSampleId :
BFB80

m/z	Abundance
36.10	496.0
37.00	2307.0
38.10	2439.0
39.00	967.0
39.90	353.0
44.00	1280.0
45.00	424.0
46.20	185.0
47.00	504.0
48.00	291.0
49.10	1819.0
50.00	9242.0
51.10	2859.0
52.00	169.0
53.00	108.0
54.90	169.0
56.00	637.0
57.00	1228.0
60.00	519.0
61.00	2410.0
62.00	2450.0
63.00	2100.0
63.90	356.0
65.00	561.0
67.00	113.0
68.00	4774.0
69.00	4572.0
70.00	395.0
71.80	250.0
73.00	1966.0
74.00	7859.0
75.10	22744.0
76.00	2109.0
77.00	240.0
78.00	194.0
78.90	1811.0
80.00	505.0
80.90	1834.0
81.90	470.0
85.70	135.0
87.00	1725.0
88.00	1672.0
91.00	188.0
92.00	1362.0
93.00	1887.0
94.10	5272.0
95.00	42928.0
96.00	2750.0
103.90	244.0
104.90	105.0
105.80	224.0
115.90	210.0
116.90	302.0
117.80	213.0
118.80	302.0
127.90	158.0
129.80	215.0
130.80	110.0
140.90	561.0
142.90	688.0
145.00	242.0
145.80	110.0
147.90	137.0
154.80	141.0
171.10	146.0
171.90	557.0
174.00	37040.0
175.00	2774.0
176.00	35624.0
176.90	2394.0

Instrument :
MSVOA_V
ClientSampleId :
BFB80

Scan 2790 (10.061 min): VV019063.D
BFB80

m/z	Abundance
40.00	346.0
44.00	1132.0

Instrument :
MSVOA_V
ClientSampleId :
BFB80