


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102221\
Data File : VV022973.D
Acq On : 21 Oct 2021 22:49
Operator : SY/MD
Sample : M4265-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB7J4

Manual IntegrationsAPPROVED

Quant Time: Oct 22 04:59:16 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Oct 22 04:55:17 2021
Response via : Initial Calibration

Reviewed By : John Carlone 10/25/2021
Supervised By : Mahesh Dadoda 10/25/2021

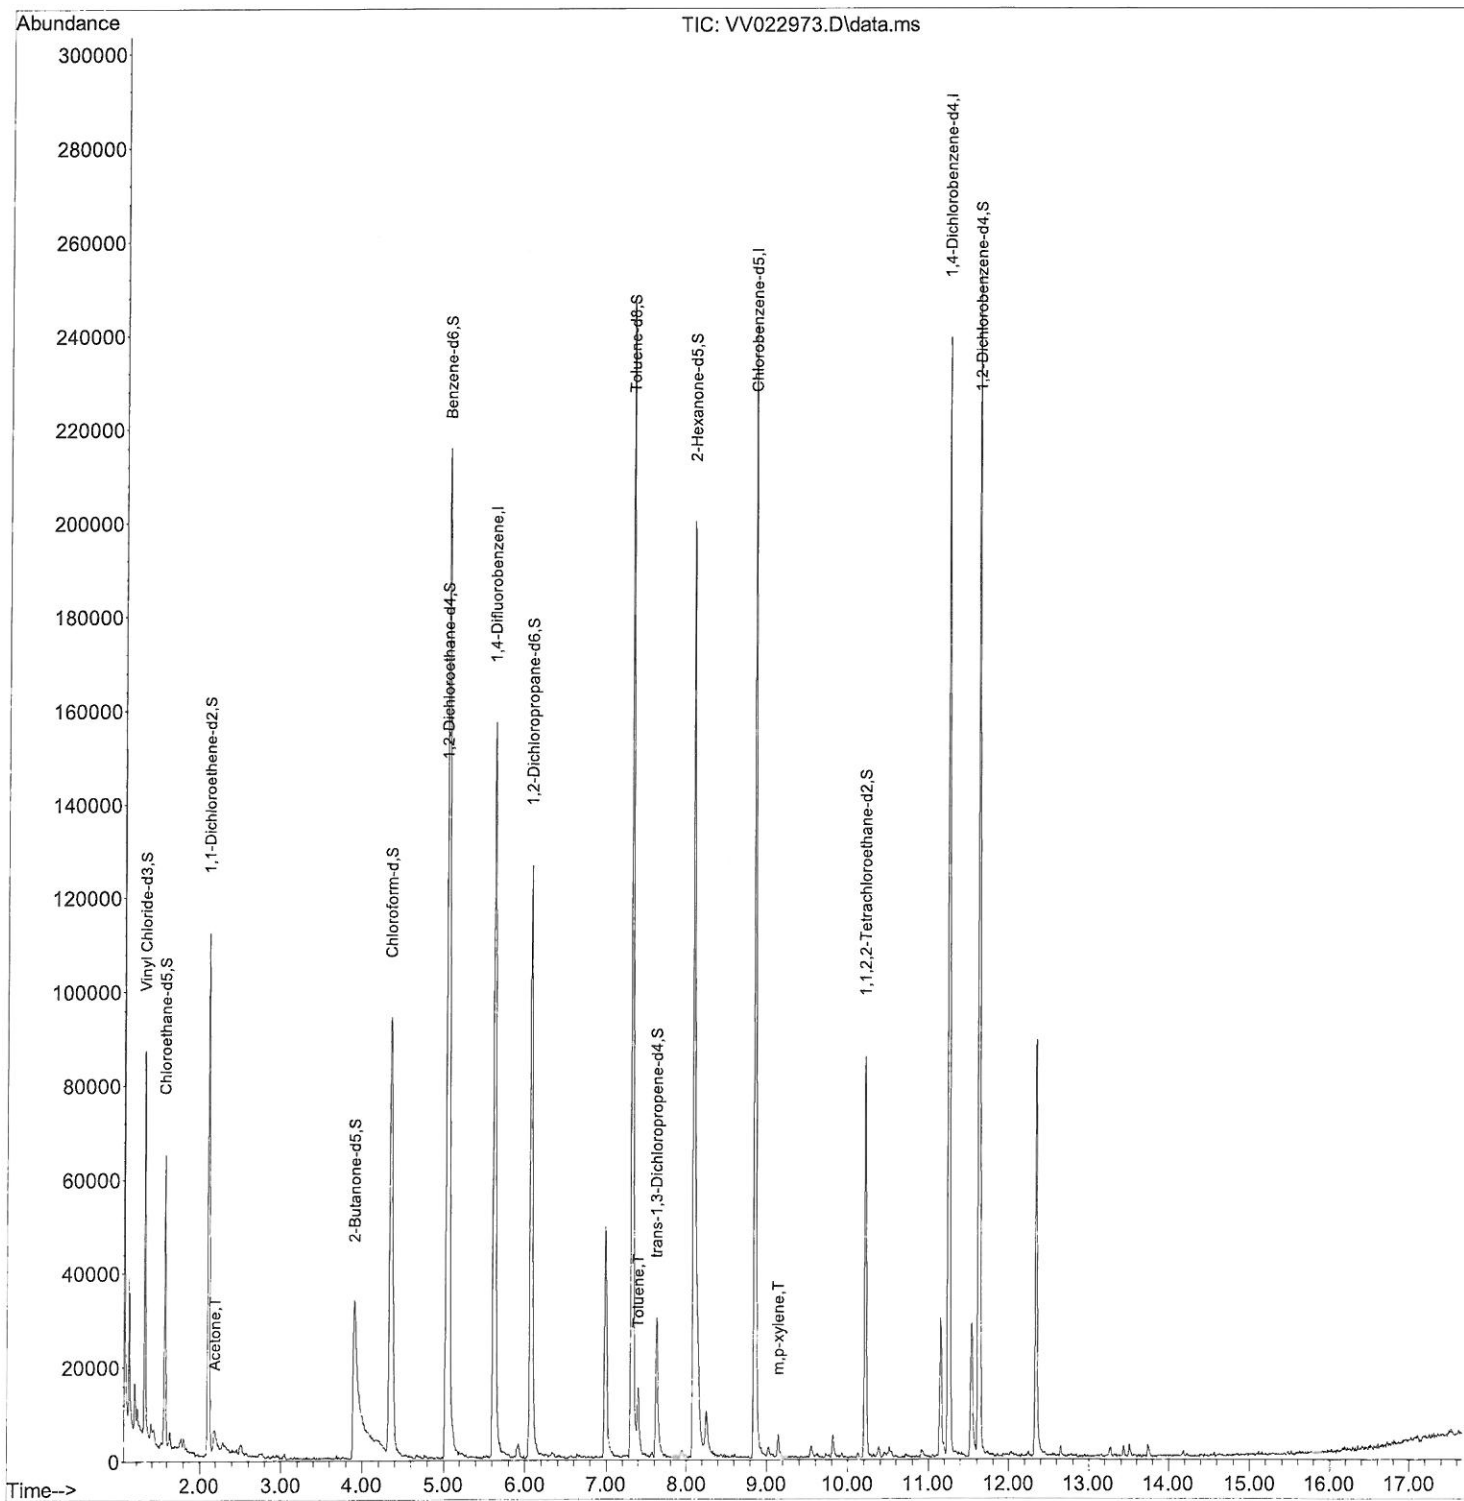

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102221\
 Data File : VV022973.D
 Acq On : 21 Oct 2021 22:49
 Operator : SY/MD
 Sample : M4265-12
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB7J4

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 10/25/2021
 Supervised By :Mahesh Dadoda 10/25/2021

Quant Time: Oct 22 04:59:16 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Oct 22 04:55:17 2021
 Response via : Initial Calibration

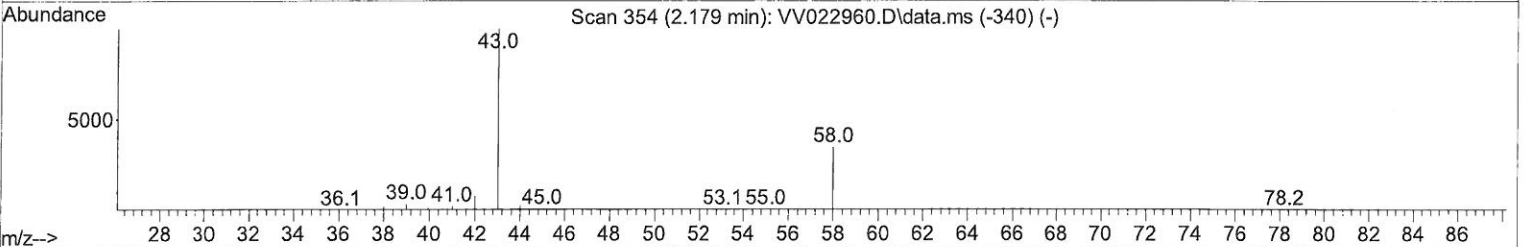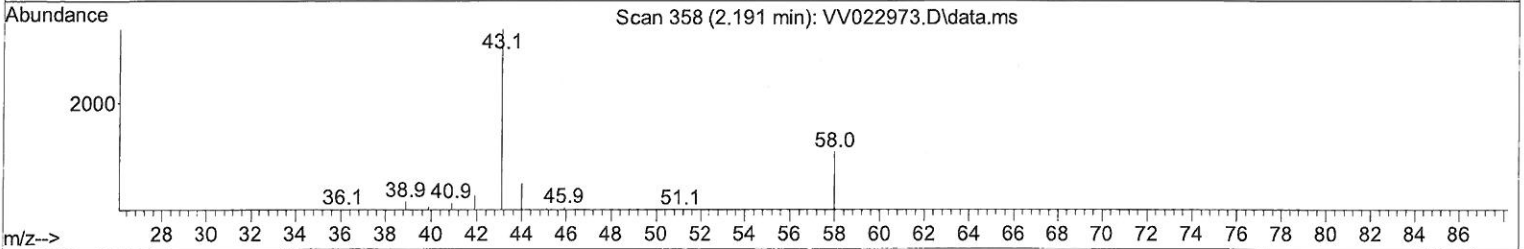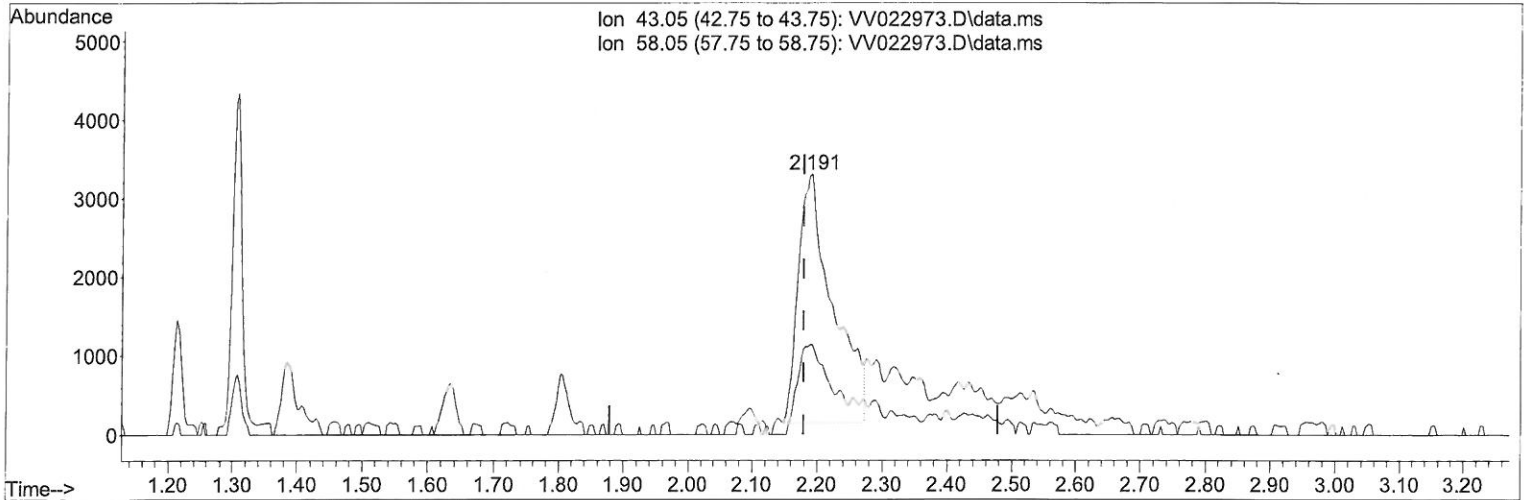

TIC: VV022973.D\data.ms

(13) Acetone (T)

2.191min (+ 0.013) 8.13 ug/L

response 11651

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	12.10	29.77#
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102221\
 Data File : VV022973.D
 Acq On : 21 Oct 2021 22:49
 Operator : SY/MD
 Sample : M4265-12
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB7J4

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 10/25/2021
 Supervised By :Mahesh Dadoda 10/25/2021

Quant Time: Oct 22 04:59:16 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Oct 22 04:55:17 2021
 Response via : Initial Calibration

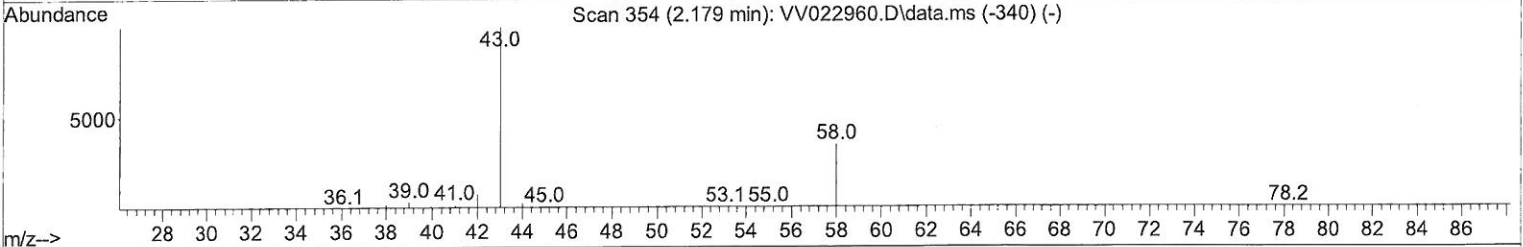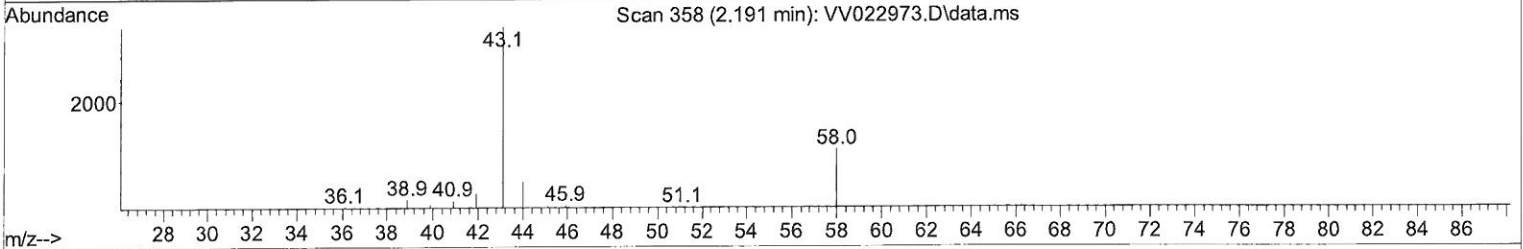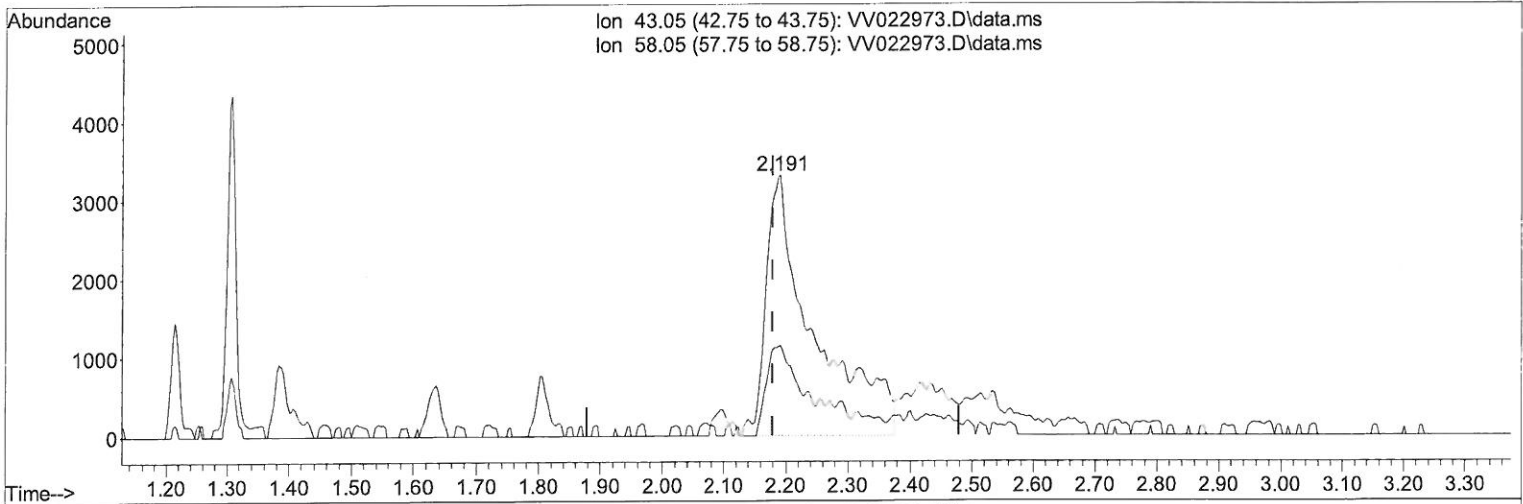

TIC: VV022973.D\data.ms

(13) Acetone (T)

2.191min (+ 0.013) 12.20 ug/L m

response 17483

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	12.10	19.84
0.00	0.00	0.00
0.00	0.00	0.00

> MD
 10/26/21

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102221\
 Data File : VV022973.D
 Acq On : 21 Oct 2021 22:49
 Operator : SY/MD
 Sample : M4265-12
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB7J4

Manual Integrations APPROVED

Reviewed By : John Carlone 10/25/2021
 Supervised By : Mahesh Dadoda 10/25/2021

Quant Time: Oct 22 04:59:16 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Oct 22 04:55:17 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	142468	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	140569	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	65045	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	44642	4.554	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery =	91.000%		
7) Chloroethane-d5	1.568	69	36920	4.191	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery =	83.800%		
11) 1,1-Dichloroethene-d2	2.108	63	58151	3.024	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery =	60.400%		
20) 2-Butanone-d5	3.902	46	79618	30.978	ug/L	0.01
Spiked Amount 50.000	Range 40 - 130		Recovery =	61.960%		
24) Chloroform-d	4.349	84	98669	4.885	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	97.600%		
26) 1,2-Dichloroethane-d4	5.034	65	45365	4.627	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	92.600%		
32) Benzene-d6	5.053	84	200092	4.782	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	95.600%		
36) 1,2-Dichloropropane-d6	6.072	67	63069	5.089	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery =	101.800%		
41) Toluene-d8	7.317	98	167280	4.624	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	92.400%		
43) trans-1,3-Dichloroprop...	7.625	79	18992	4.620	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery =	92.400%		
46) 2-Hexanone-d5	8.091	63	83691	50.516	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery =	101.040%		
56) 1,1,2,2-Tetrachloroeth...	10.217	84	42518	5.065	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery =	101.200%		
66) 1,2-Dichlorobenzene-d4	11.625	152	66909	5.548	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery =	111.000%		
Target Compounds						
13) Acetone	2.191	43	17483m	12.199	ug/L	Qvalue
42) Toluene	7.397	91	10552	0.275	ug/L	97
53) m,p-xylene	9.143	106	1558	0.102	ug/L	90

(#) = qualifier out of range (m) = manual integration (+) = signals summed