


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102221\
Data File : VV022976.D
Acq On : 22 Oct 2021 00:00
Operator : SY/MD
Sample : M4265-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB7J7

Manual IntegrationsAPPROVED

Quant Time: Oct 22 05:00:00 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Oct 22 04:55:17 2021
Response via : Initial Calibration

Reviewed By :John Carlone 10/25/2021
Supervised By :Mahesh Dadoda 10/25/2021

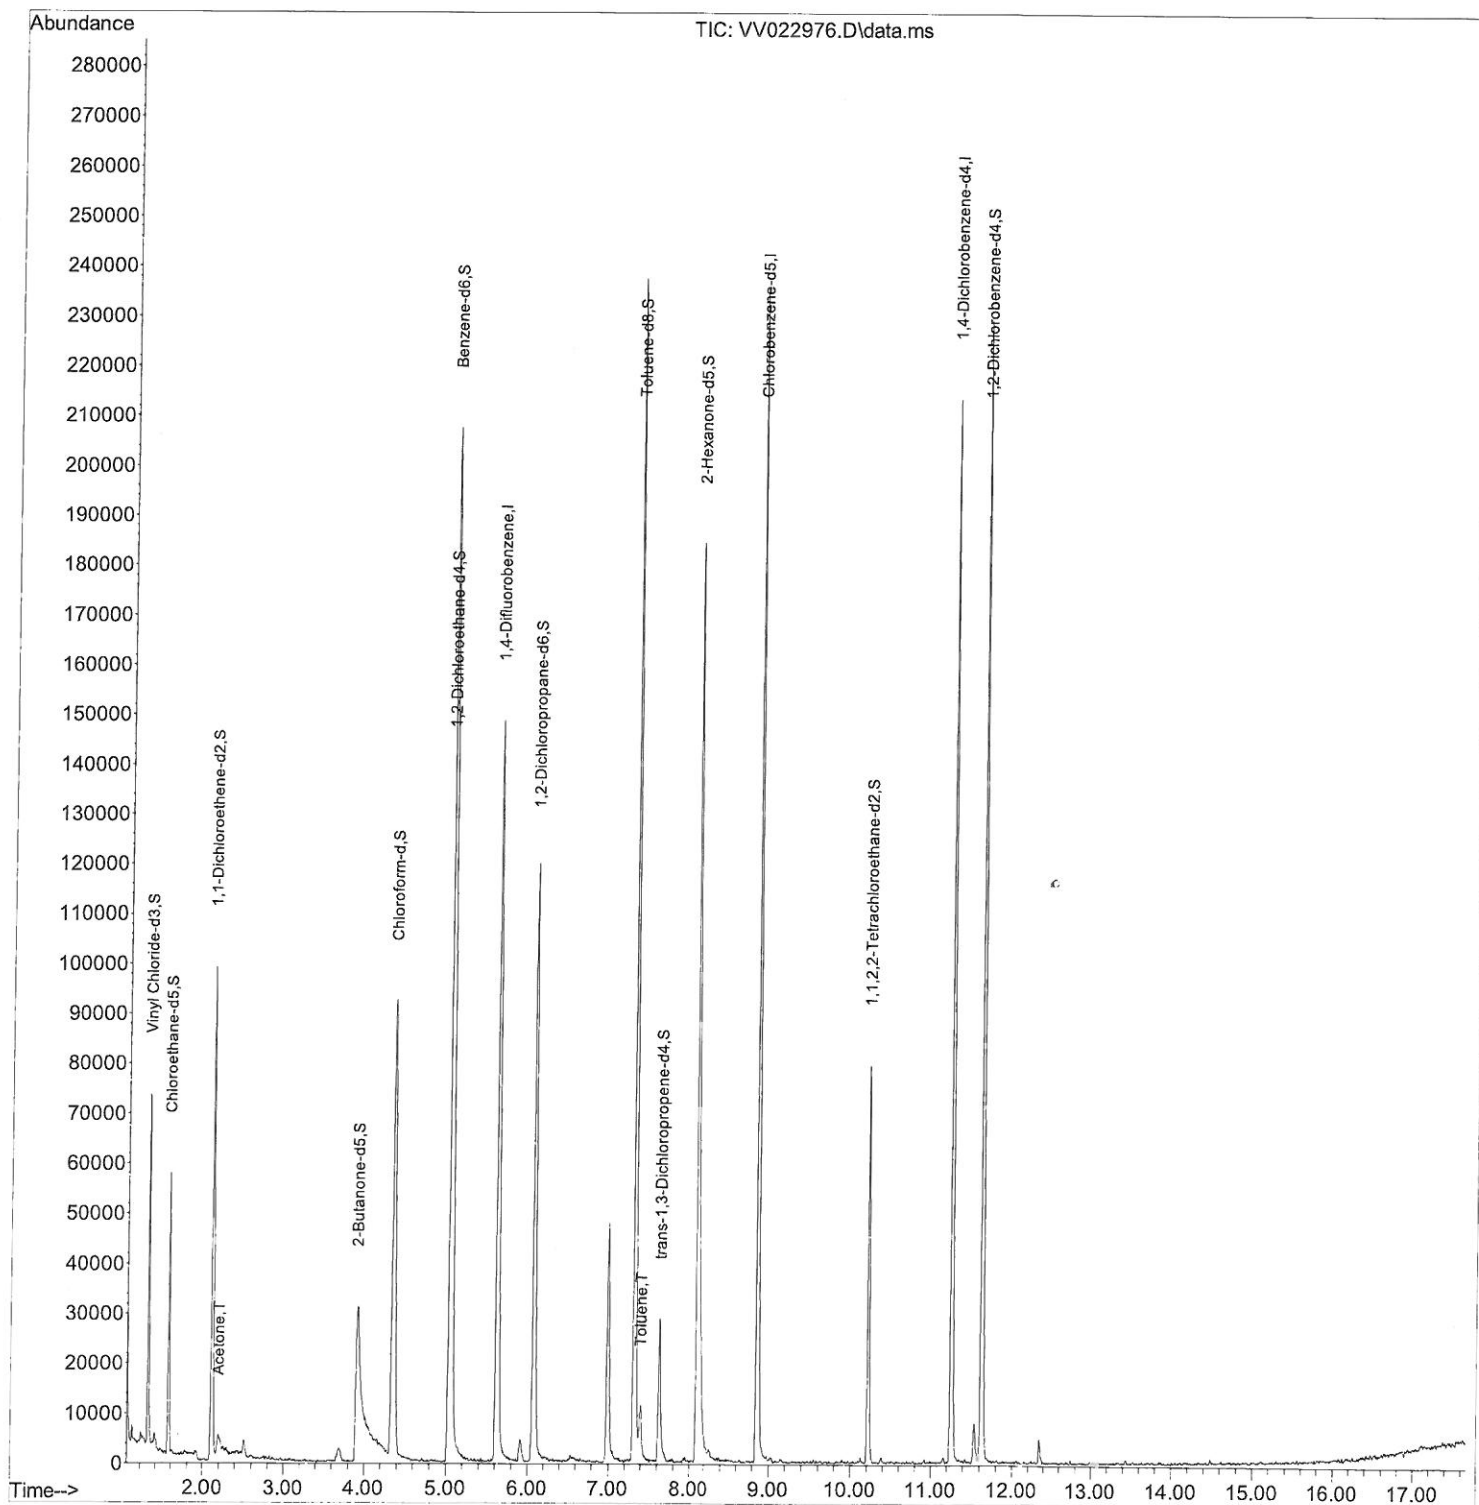

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102221\
 Data File : VV022976.D
 Acq On : 22 Oct 2021 00:00
 Operator : SY/MD
 Sample : M4265-15
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB7J7

Manual IntegrationsAPPROVED

Quant Time: Oct 22 05:00:00 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Oct 22 04:55:17 2021
 Response via : Initial Calibration

Reviewed By :John Carlone 10/25/2021
 Supervised By :Mahesh Dadoda 10/25/2021

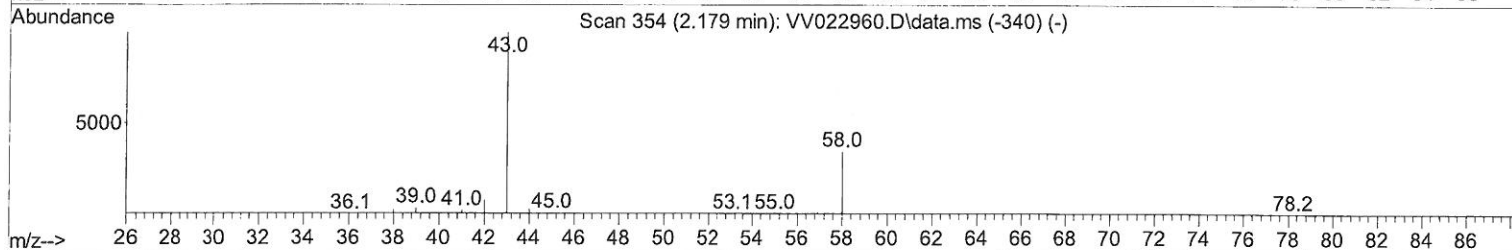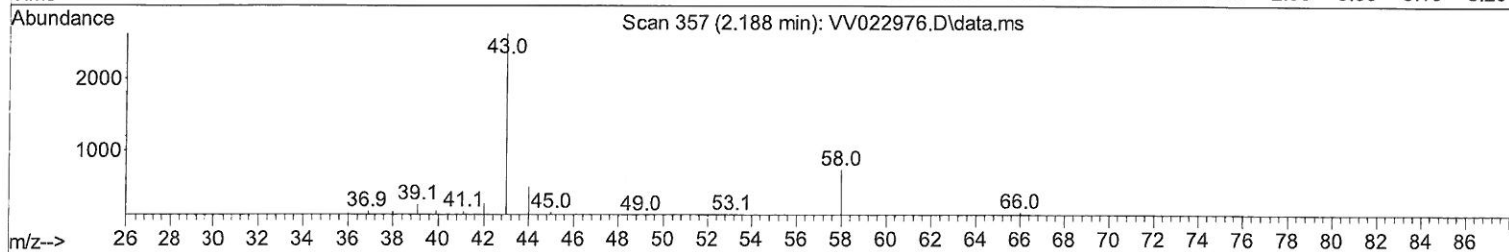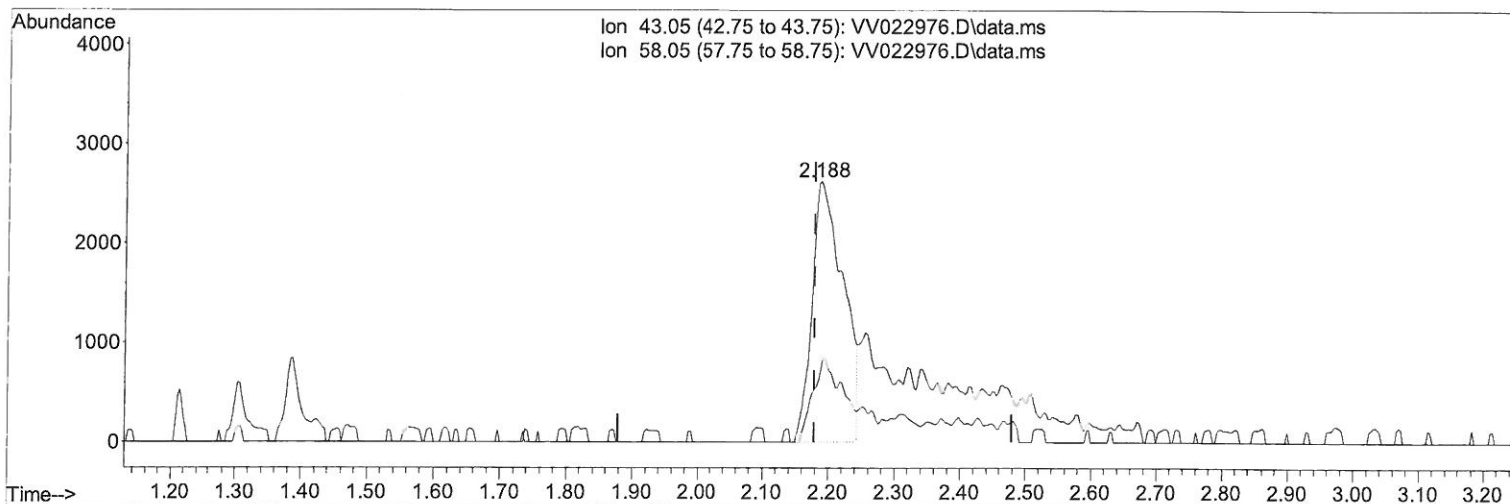

TIC: VV022976.D\data.ms

(13) Acetone (T)

2.188min (+ 0.009) 6.33 ug/L

response 8573

| Ion | Exp% | Act% |
|-------|--------|--------|
| 43.05 | 100.00 | 100.00 |
| 58.05 | 12.10 | 21.88 |
| 0.00 | 0.00 | 0.00 |
| 0.00 | 0.00 | 0.00 |

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102221\
 Data File : VV022976.D
 Acq On : 22 Oct 2021 00:00
 Operator : SY/MD
 Sample : M4265-15
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 Client Sample Id :
 GB7J7

Manual Integrations APPROVED

Quant Time: Oct 22 05:00:00 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Oct 22 04:55:17 2021
 Response via : Initial Calibration

Reviewed By : John Carlone 10/25/2021
 Supervised By : Mahesh Dadoda 10/25/2021

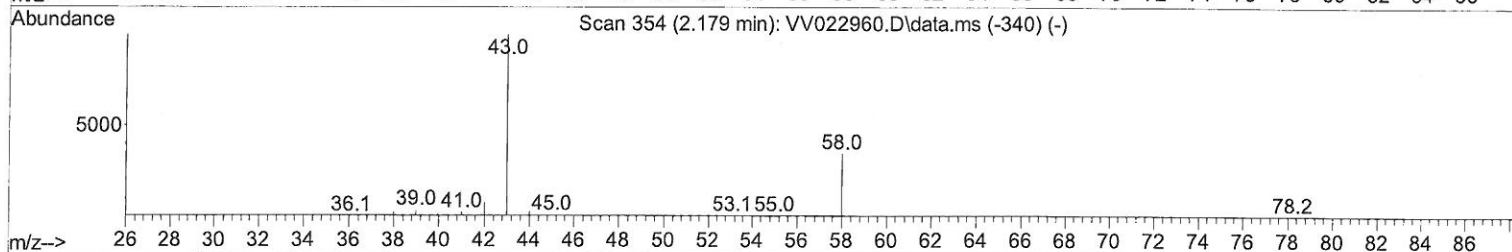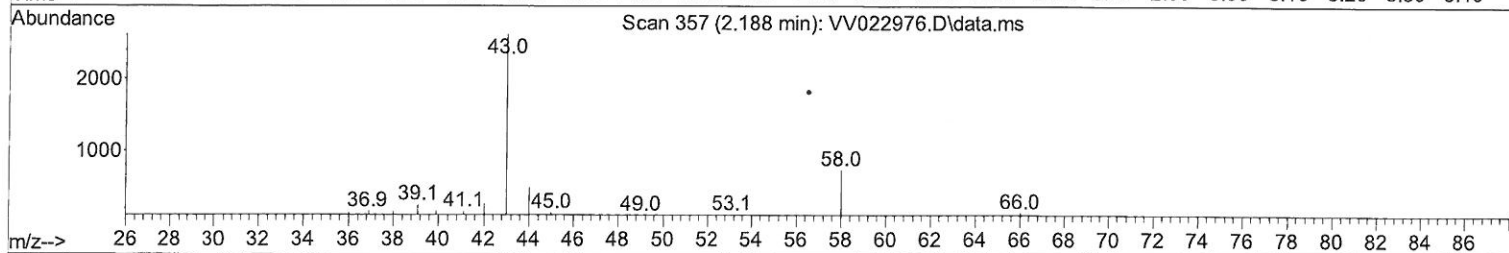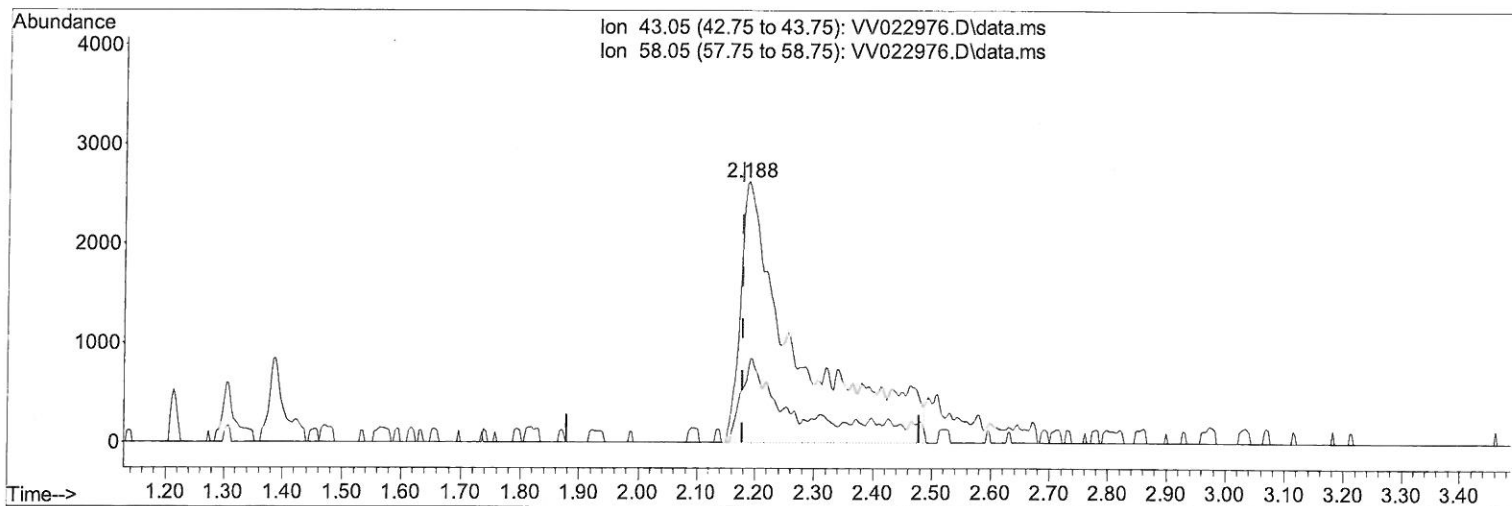

TIC: VV022976.D\data.ms

(13) Acetone (T)

2.188min (+ 0.009) 12.96 ug/L m

response 17556

Ion Exp% Act%

43.05 100.00 100.00

58.05 12.10 10.69

0.00 0.00 0.00

0.00 0.00 0.00

7 MD
10/26/21

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102221\
 Data File : VV022976.D
 Acq On : 22 Oct 2021 00:00
 Operator : SY/MD
 Sample : M4265-15
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB7J7

Manual Integrations APPROVED

Reviewed By : John Carlone 10/25/2021
 Supervised By : Mahesh Dadoda 10/25/2021

Quant Time: Oct 22 05:00:00 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Oct 22 04:55:17 2021
 Response via : Initial Calibration

| Compound | R.T. | QIon | Response | Conc | Units | Dev(Min) |
|-------------------------------|----------------|------|------------|----------|-------|----------|
| Internal Standards | | | | | | |
| 1) 1,4-Difluorobenzene | 5.619 | 114 | 134656 | 5.000 | ug/L | 0.00 |
| 28) Chlorobenzene-d5 | 8.854 | 117 | 134745 | 5.000 | ug/L | 0.00 |
| 58) 1,4-Dichlorobenzene-d4 | 11.249 | 152 | 57363 | 5.000 | ug/L | 0.00 |
| System Monitoring Compounds | | | | | | |
| 4) Vinyl Chloride-d3 | 1.304 | 65 | 43321 | 4.676 | ug/L | 0.00 |
| Spiked Amount 5.000 | Range 40 - 130 | | Recovery = | 93.600% | | |
| 7) Chloroethane-d5 | 1.568 | 69 | 34880 | 4.190 | ug/L | 0.00 |
| Spiked Amount 5.000 | Range 65 - 130 | | Recovery = | 83.800% | | |
| 11) 1,1-Dichloroethene-d2 | 2.108 | 63 | 51442 | 2.831 | ug/L | 0.00 |
| Spiked Amount 5.000 | Range 60 - 125 | | Recovery = | 56.600%# | | |
| 20) 2-Butanone-d5 | 3.908 | 46 | 72412 | 29.809 | ug/L | 0.02 |
| Spiked Amount 50.000 | Range 40 - 130 | | Recovery = | 59.620% | | |
| 24) Chloroform-d | 4.352 | 84 | 97977 | 5.132 | ug/L | 0.00 |
| Spiked Amount 5.000 | Range 70 - 125 | | Recovery = | 102.600% | | |
| 26) 1,2-Dichloroethane-d4 | 5.034 | 65 | 44414 | 4.793 | ug/L | 0.00 |
| Spiked Amount 5.000 | Range 70 - 130 | | Recovery = | 95.800% | | |
| 32) Benzene-d6 | 5.050 | 84 | 189192 | 4.717 | ug/L | 0.00 |
| Spiked Amount 5.000 | Range 70 - 125 | | Recovery = | 94.400% | | |
| 36) 1,2-Dichloropropane-d6 | 6.069 | 67 | 60750 | 5.114 | ug/L | 0.00 |
| Spiked Amount 5.000 | Range 60 - 140 | | Recovery = | 102.200% | | |
| 41) Toluene-d8 | 7.317 | 98 | 162135 | 4.676 | ug/L | 0.00 |
| Spiked Amount 5.000 | Range 70 - 130 | | Recovery = | 93.600% | | |
| 43) trans-1,3-Dichloroprop... | 7.628 | 79 | 18368 | 4.661 | ug/L | 0.00 |
| Spiked Amount 5.000 | Range 55 - 130 | | Recovery = | 93.200% | | |
| 46) 2-Hexanone-d5 | 8.095 | 63 | 75048 | 47.257 | ug/L | 0.00 |
| Spiked Amount 50.000 | Range 45 - 130 | | Recovery = | 94.520% | | |
| 56) 1,1,2,2-Tetrachloroeth... | 10.217 | 84 | 39334 | 4.888 | ug/L | 0.00 |
| Spiked Amount 5.000 | Range 65 - 120 | | Recovery = | 97.800% | | |
| 66) 1,2-Dichlorobenzene-d4 | 11.625 | 152 | 61471 | 5.780 | ug/L | 0.00 |
| Spiked Amount 5.000 | Range 80 - 120 | | Recovery = | 115.600% | | |
| Target Compounds | | | | | | |
| 13) Acetone | 2.188 | 43 | 17556m | 12.961 | ug/L | Qvalue |
| 42) Toluene | 7.394 | 91 | 8036 | 0.218 | ug/L | 88 |

(#) = qualifier out of range (m) = manual integration (+) = signals summed