


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102221\
Data File : VV022996.D
Acq On : 22 Oct 2021 18:53
Operator : SY/MD
Sample : M4265-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
Client Sample Id :
GB7J0

Manual Integrations APPROVED

Reviewed By : John Carlone 10/25/2021
Supervised By : Mahesh Dadoda 10/25/2021

Quant Time: Oct 23 01:30:59 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Oct 23 01:14:46 2021
Response via : Initial Calibration

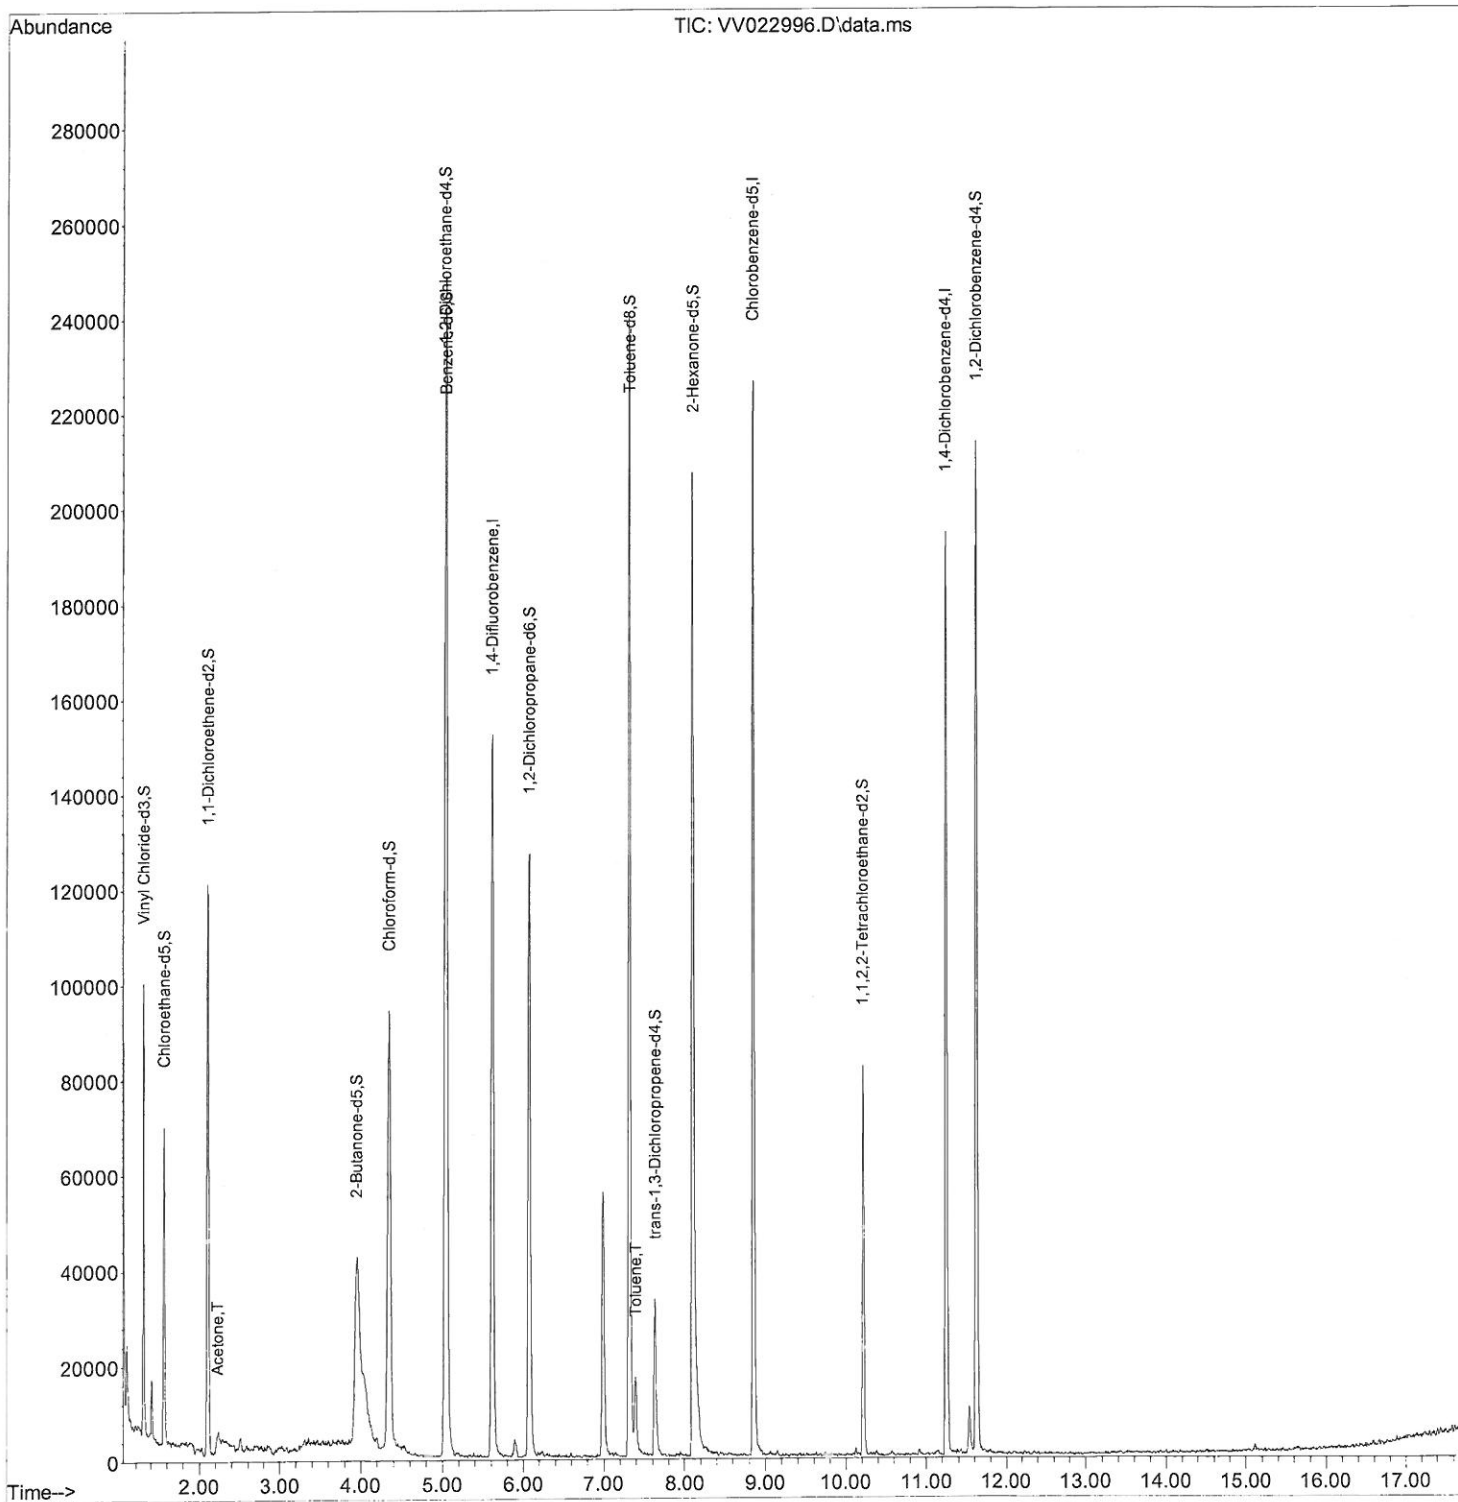

Quantitation Report (Qedit)


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102221\
 Data File : VV022996.D
 Acq On : 22 Oct 2021 18:53
 Operator : SY/MD
 Sample : M4265-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB7J0

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 10/25/2021
 Supervised By :Mahesh Dadoda 10/25/2021

Quant Time: Oct 23 01:30:59 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Oct 23 01:14:46 2021
 Response via : Initial Calibration

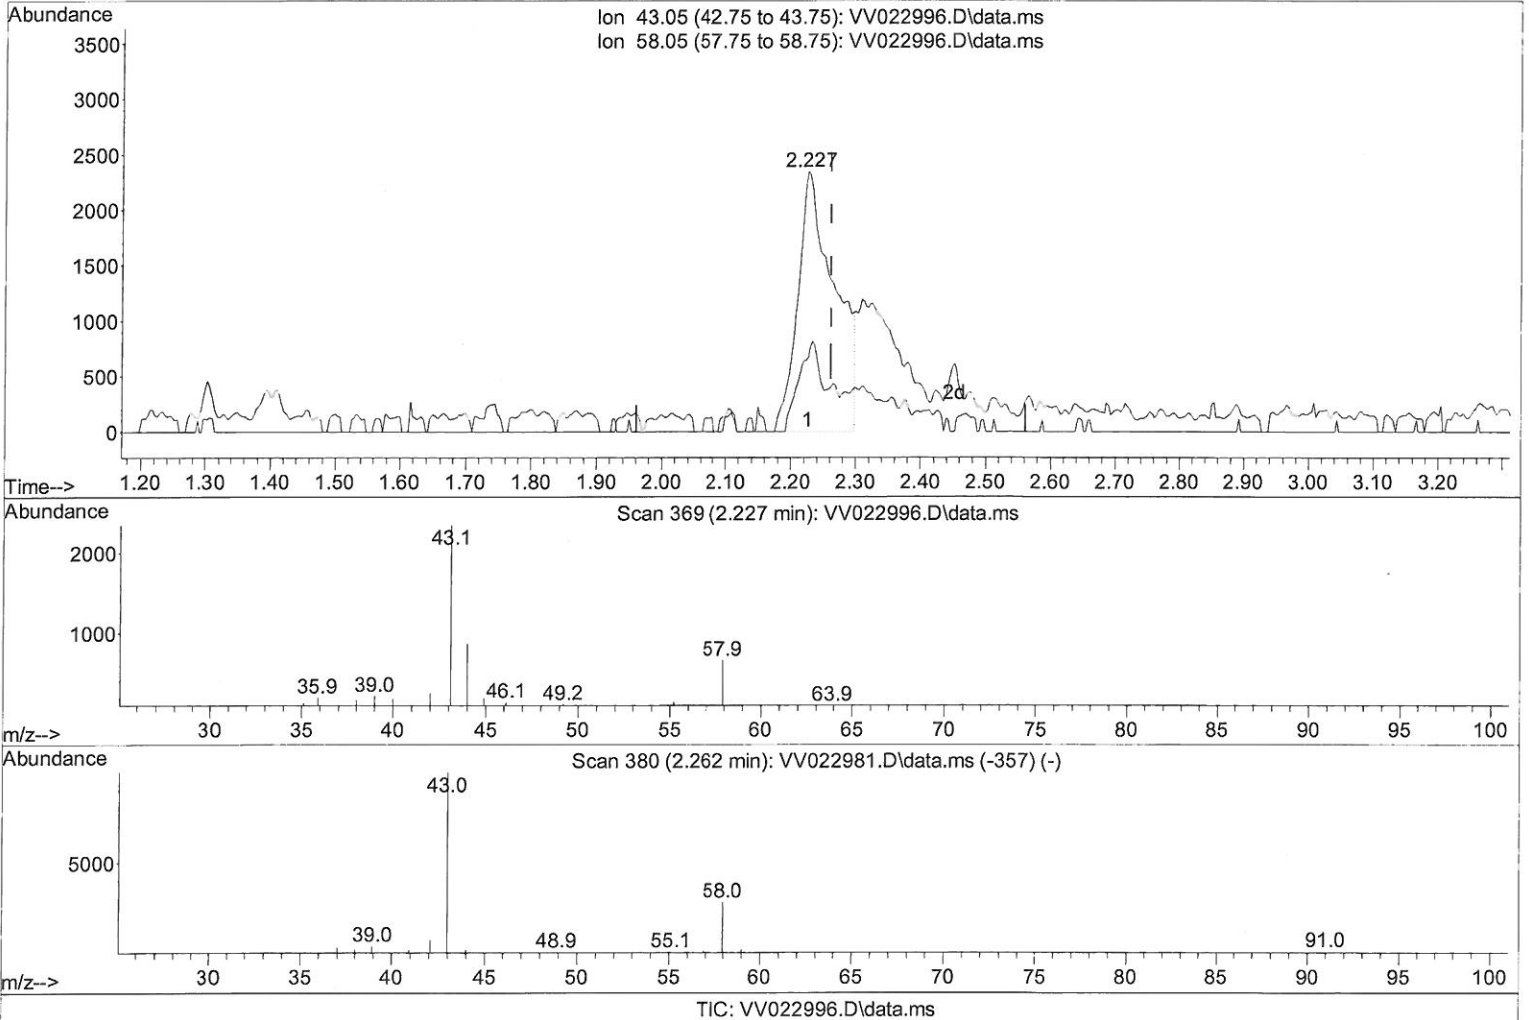

(13) Acetone (T)

2.227min (-0.035) 10.39 ug/L

response 9212

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	27.70	20.04
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102221\
Data File : VV022996.D
Acq On : 22 Oct 2021 18:53
Operator : SY/MD
Sample : M4265-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :

MSVOA_V

ClientSampleId :




GB7J0

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 10/25/2021

Supervised By :Mahesh Dadoda 10/25/2021

Quant Time: Oct 23 01:30:59 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Oct 23 01:14:46 2021
Response via : Initial Calibration

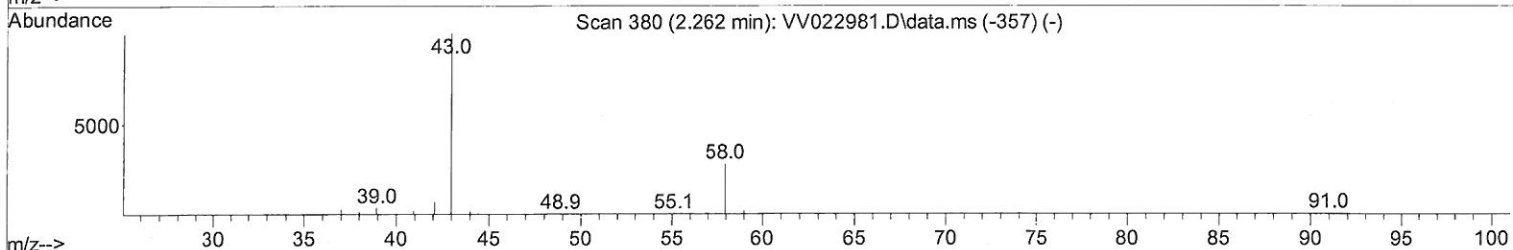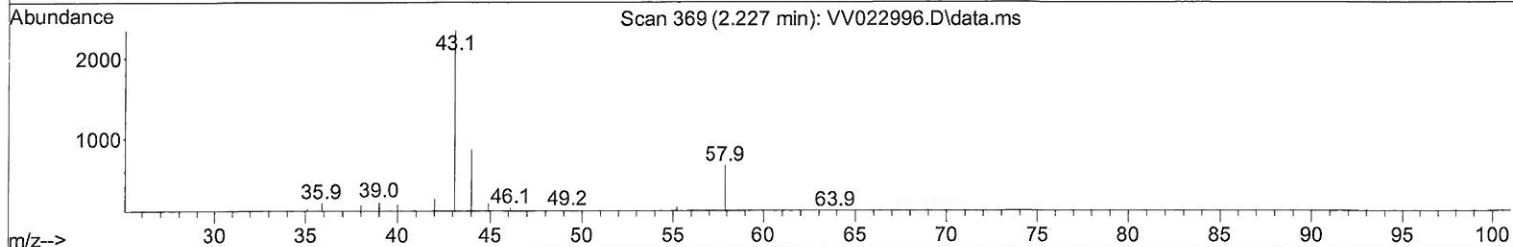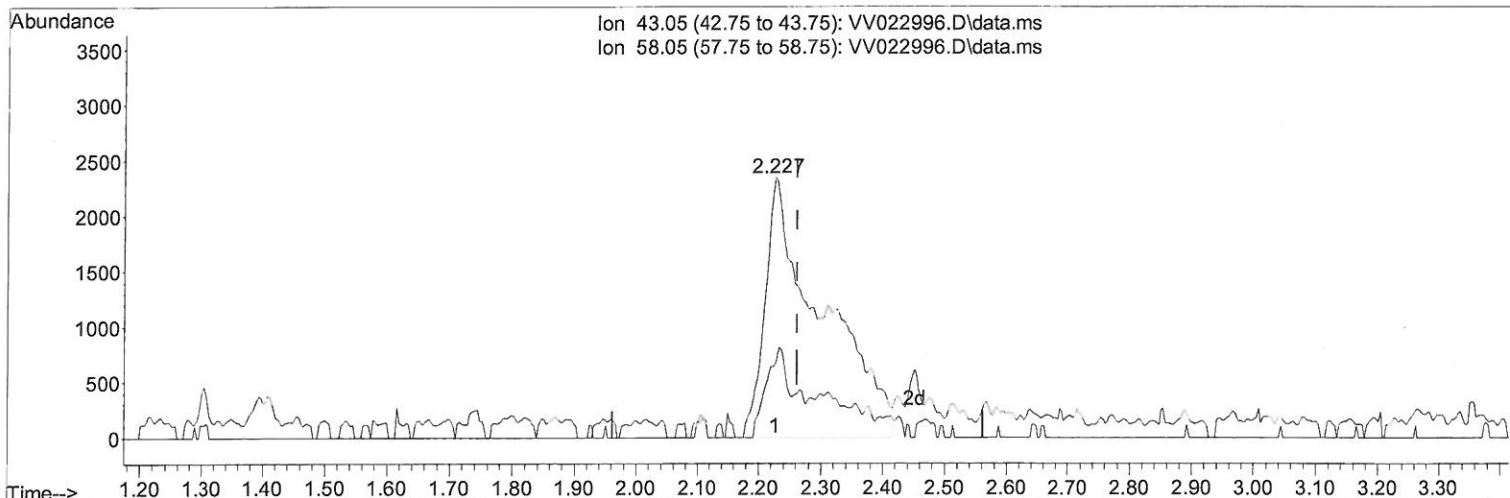

TIC: VV022996.D\data.ms

(13) Acetone (T)

2.227min (-0.035) 16.68 ug/L m

response 14783

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	27.70	12.49
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (QT Review)

Instrument :

MSVOA_V

Client Sample Id :

GB7J0

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW102221\

Data File : VW022996.D

Acq On : 22 Oct 2021 18:53

Operator : SY/MD

Sample : M4265-06

Misc : 25.0mL/MSVOA_V/WATER

ALS Vial : 39 Sample Multiplier: 1

Manual Integrations APPROVED

Reviewed By : John Carlone 10/25/2021

Supervised By : Mahesh Dadoda 10/25/2021

Quant Time: Oct 23 01:30:59 2021

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M

Quant Title : TRACE VOA SFAM1.0

QLast Update : Sat Oct 23 01:14:46 2021

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	128862	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	126764	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	51881	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	55881	4.963	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery =	99.200%		
7) Chloroethane-d5	1.561	69	38774	5.567	ug/L	-0.02
Spiked Amount 5.000	Range 65 - 130		Recovery =	111.400%		
11) 1,1-Dichloroethene-d2	2.101	63	61955	3.814	ug/L	-0.02
Spiked Amount 5.000	Range 60 - 125		Recovery =	76.200%		
20) 2-Butanone-d5	3.953	46	118891	65.820	ug/L	0.00
Spiked Amount 50.000	Range 40 - 130		Recovery =	131.640%#		
24) Chloroform-d	4.346	84	91982	5.025	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	100.400%		
26) 1,2-Dichloroethane-d4	5.034	65	47613	5.518	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	110.400%		
32) Benzene-d6	5.043	84	206631	5.583	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	111.600%		
36) 1,2-Dichloropropane-d6	6.072	67	62487	5.485	ug/L	-0.01
Spiked Amount 5.000	Range 60 - 140		Recovery =	109.600%		
41) Toluene-d8	7.317	98	159485	4.797	ug/L	-0.01
Spiked Amount 5.000	Range 70 - 130		Recovery =	96.000%		
43) trans-1,3-Dichloroprop...	7.628	79	19855	4.974	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery =	99.400%		
46) 2-Hexanone-d5	8.104	63	69851	47.265	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery =	94.520%		
56) 1,1,2,2-Tetrachloroeth...	10.217	84	39917	5.074	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery =	101.400%		
66) 1,2-Dichlorobenzene-d4	11.625	152	56947	6.152	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery =	123.000%#		
Target Compounds						
13) Acetone	2.227	43	14783m	16.681	ug/L	Qvalue
42) Toluene	7.391	91	12020	0.348	ug/L	91

(#)= qualifier out of range (m)= manual integration (+)= signals summed