

Quantitation Report (QT Review)


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102221\
Data File : VV022998.D
Acq On : 22 Oct 2021 19:41
Operator : SY/MD
Sample : M4265-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB7J7

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 10/25/2021
Supervised By :Mahesh Dadoda 10/25/2021

Quant Time: Oct 23 01:31:21 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Oct 23 01:14:46 2021
Response via : Initial Calibration

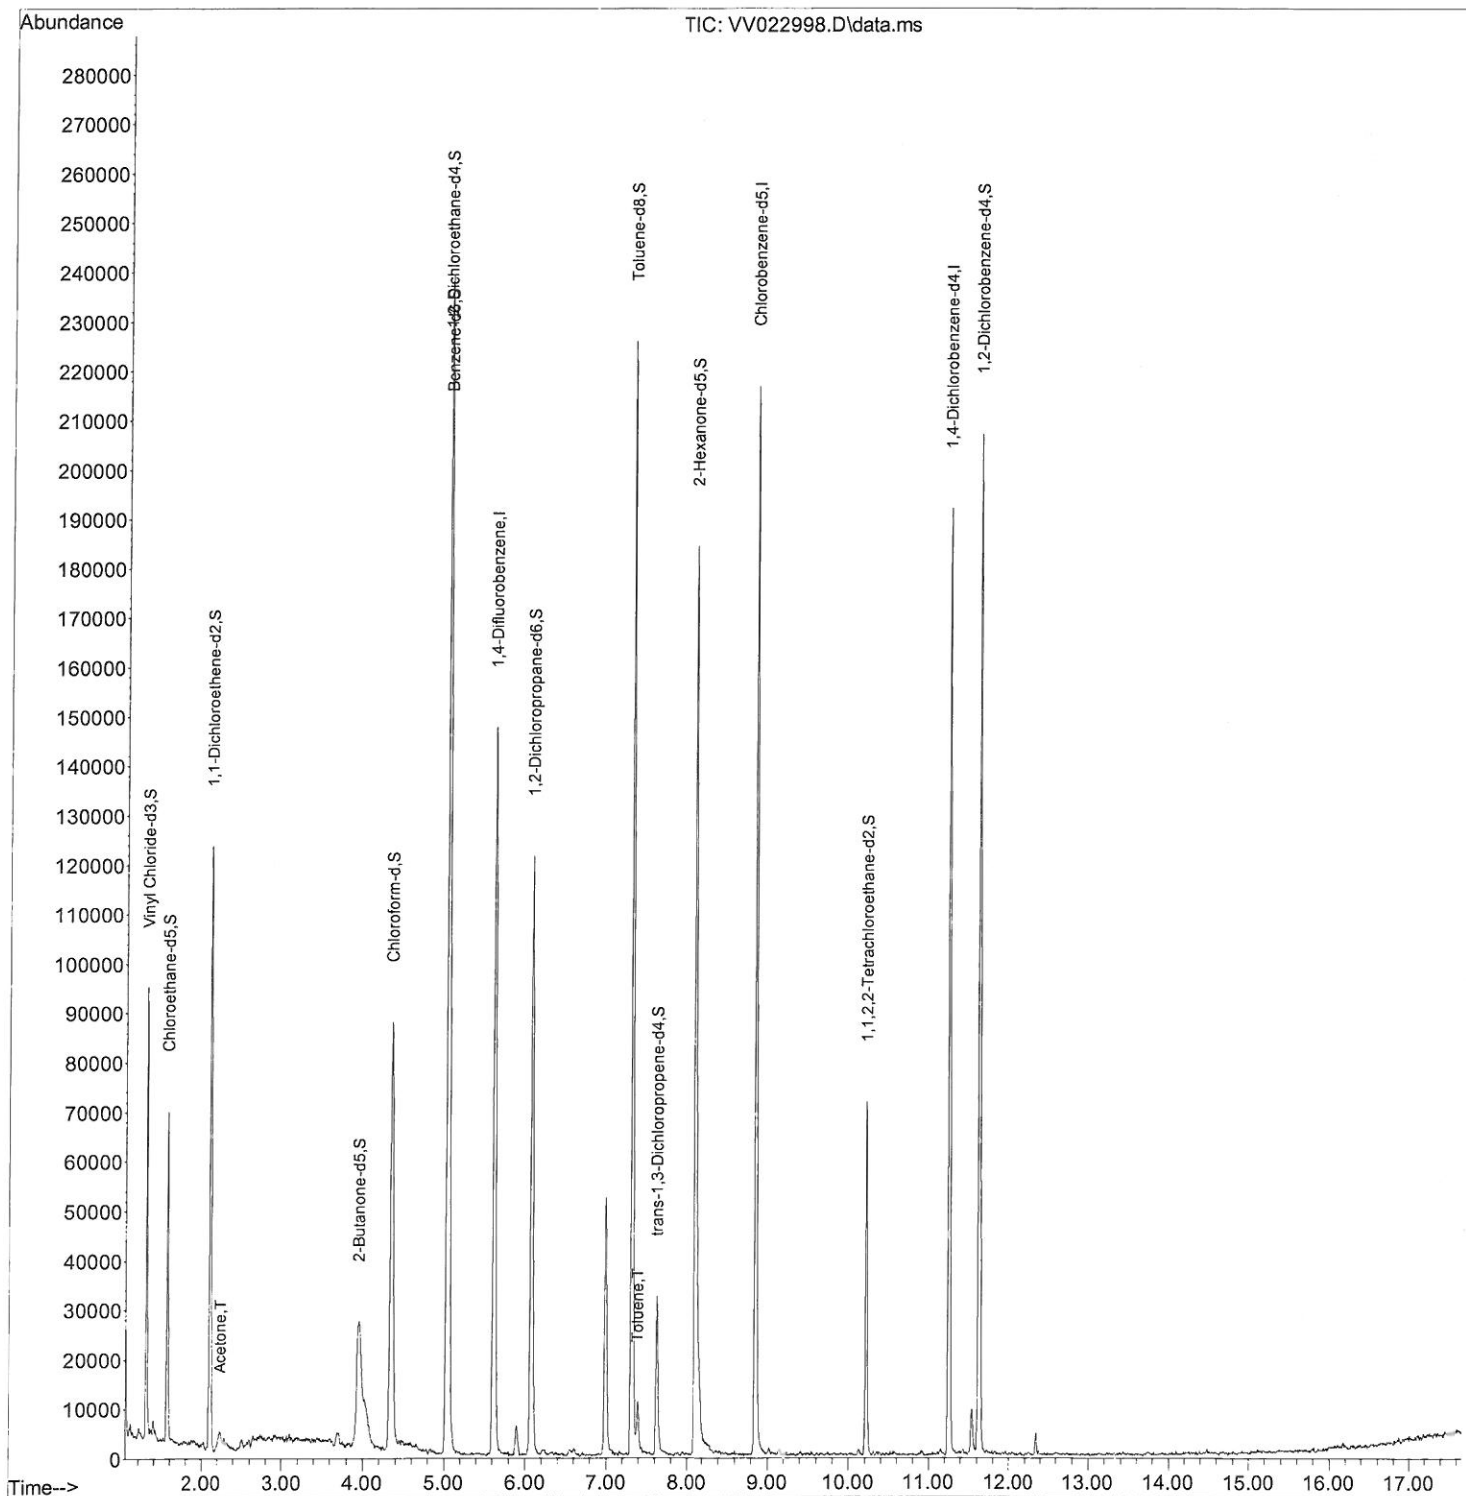

Quantitation Report (Qedit)


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102221\
 Data File : VV022998.D
 Acq On : 22 Oct 2021 19:41
 Operator : SY/MD
 Sample : M4265-15
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB7J7

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 10/25/2021
 Supervised By :Mahesh Dadoda 10/25/2021

Quant Time: Oct 23 01:31:21 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Oct 23 01:14:46 2021
 Response via : Initial Calibration

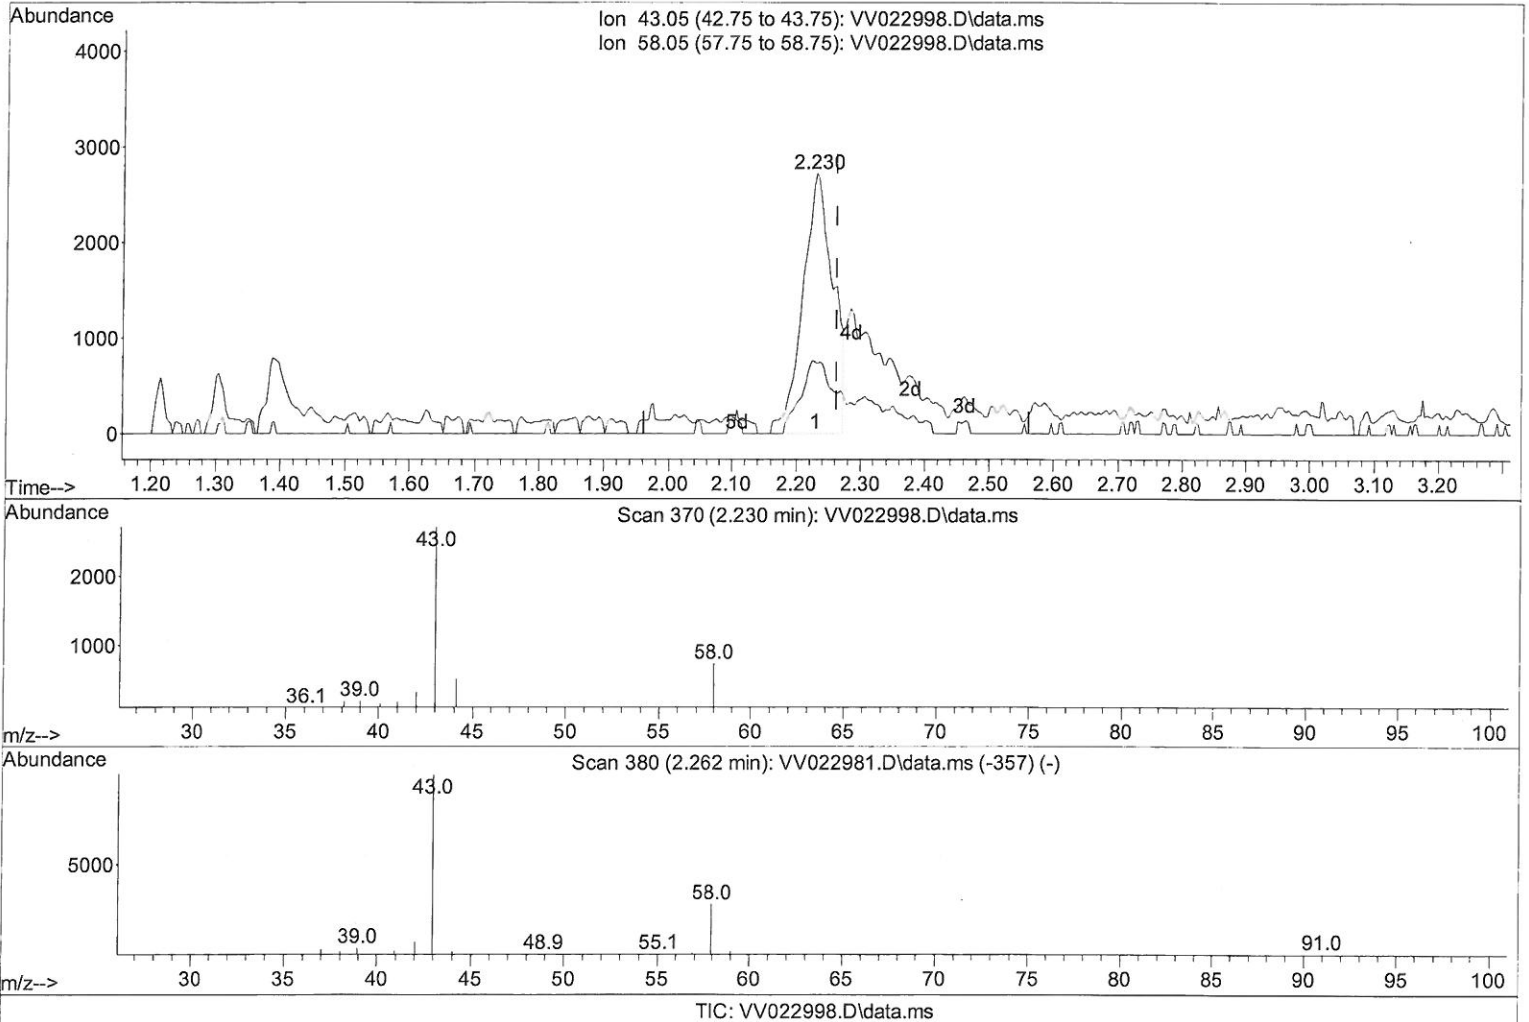

(13) Acetone (T)

2.230min (-0.032) 10.18 ug/L

response 8844

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	27.70	27.34
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102221\
 Data File : VV022998.D
 Acq On : 22 Oct 2021 19:41
 Operator : SY/MD
 Sample : M4265-15
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB7J7

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 10/25/2021
 Supervised By :Mahesh Dadoda 10/25/2021

Quant Time: Oct 23 01:31:21 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Oct 23 01:14:46 2021
 Response via : Initial Calibration

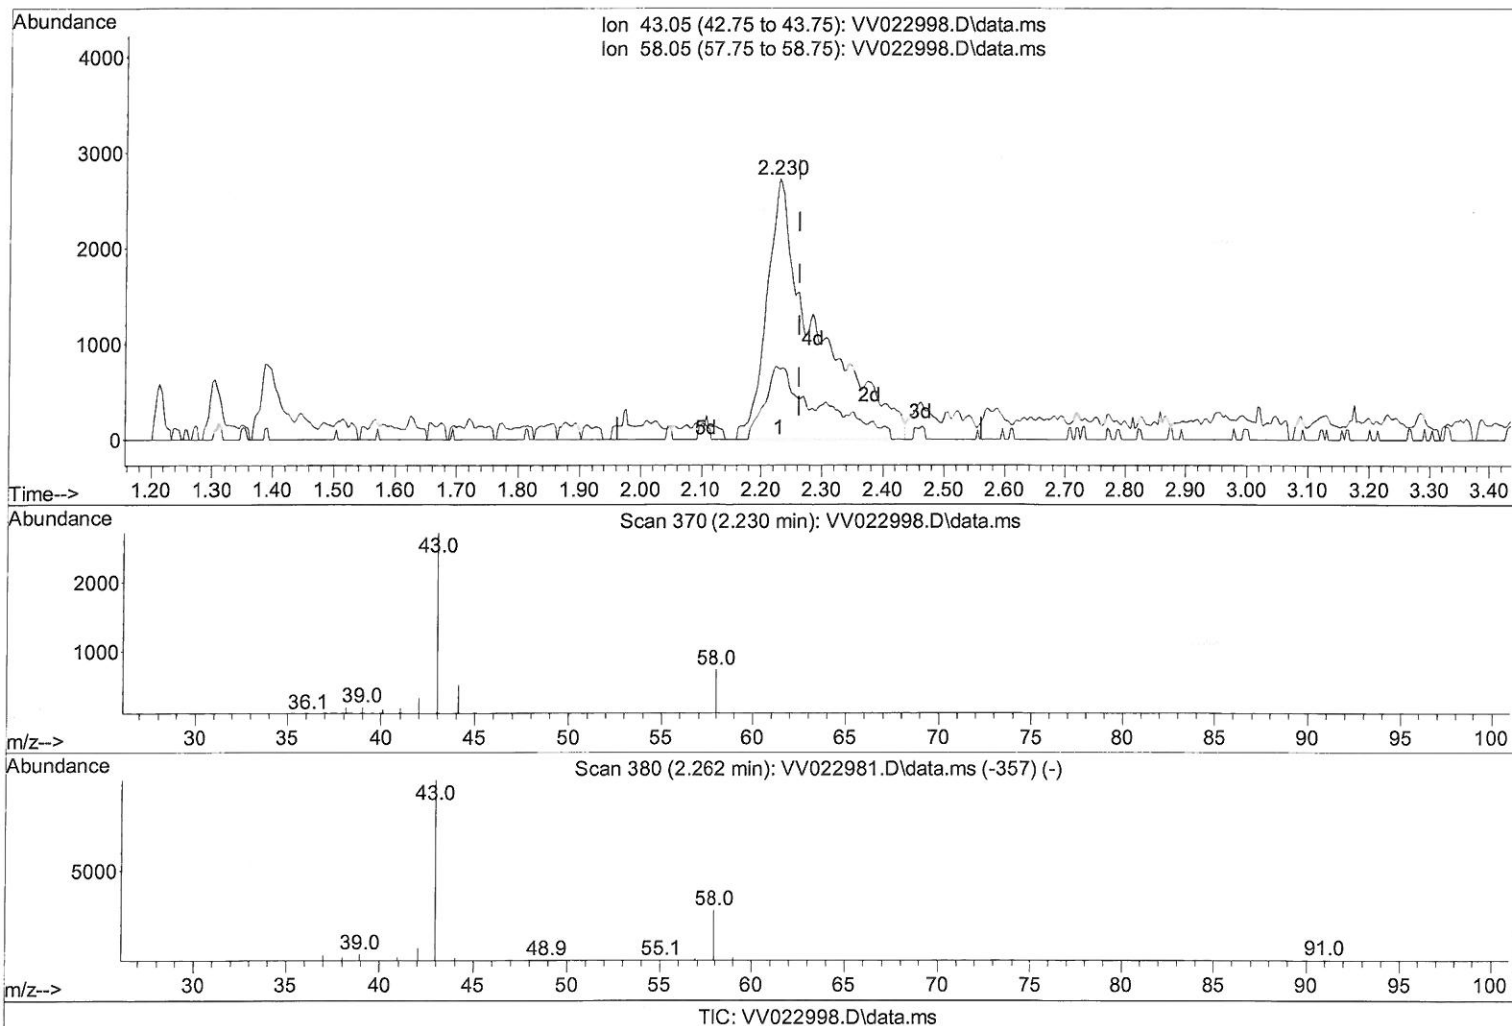

(13) Acetone (T)

2.230min (-0.032) 17.92 ug/L m

response 15572

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	27.70	15.53
0.00	0.00	0.00
0.00	0.00	0.00

SYMD
 10/27/21

Quantitation Report (QT Review)

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW102221\
 Data File : VW022998.D
 Acq On : 22 Oct 2021 19:41
 Operator : SY/MD
 Sample : M4265-15
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 Client Sample Id :
 GB7J7

Manual Integrations APPROVED

Reviewed By : John Carlone 10/25/2021
 Supervised By : Mahesh Dadoda 10/25/2021

Quant Time: Oct 23 01:31:21 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Oct 23 01:14:46 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	126366	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	123392	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	50665	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	55390	5.016	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery = 100.400%			
7) Chloroethane-d5	1.561	69	39064	5.719	ug/L	-0.02
Spiked Amount 5.000	Range 65 - 130		Recovery = 114.400%			
11) 1,1-Dichloroethene-d2	2.101	63	62704	3.936	ug/L	-0.02
Spiked Amount 5.000	Range 60 - 125		Recovery = 78.800%			
20) 2-Butanone-d5	3.953	46	79126	44.671	ug/L	0.00
Spiked Amount 50.000	Range 40 - 130		Recovery = 89.340%			
24) Chloroform-d	4.346	84	86215	4.803	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery = 96.000%			
26) 1,2-Dichloroethane-d4	5.034	65	45870	5.421	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery = 108.400%			
32) Benzene-d6	5.043	84	200297	5.560	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery = 111.200%			
36) 1,2-Dichloropropane-d6	6.072	67	59218	5.340	ug/L	-0.01
Spiked Amount 5.000	Range 60 - 140		Recovery = 106.800%			
41) Toluene-d8	7.317	98	147966	4.573	ug/L	-0.01
Spiked Amount 5.000	Range 70 - 130		Recovery = 91.400%			
43) trans-1,3-Dichloroprop...	7.625	79	18350	4.723	ug/L	-0.01
Spiked Amount 5.000	Range 55 - 130		Recovery = 94.400%			
46) 2-Hexanone-d5	8.104	63	61472	42.732	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery = 85.460%			
56) 1,1,2,2-Tetrachloroeth...	10.220	84	34402	4.493	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery = 89.800%			
66) 1,2-Dichlorobenzene-d4	11.625	152	52607	5.819	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery = 116.400%			
Target Compounds						
13) Acetone	2.230	43	15572m	17.919	ug/L	Qvalue
42) Toluene	7.391	91	6807	0.202	ug/L	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed