

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW102221\
 Data File : VW022970.D
 Acq On : 21 Oct 2021 21:37
 Operator : SY/MD
 Sample : M4265-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB7J3

Quant Time: Oct 22 04:58:03 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Oct 22 04:55:17 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	133418	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	136991	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	58004	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	43580	4.748	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	95.000%
7) Chloroethane-d5	1.568	69	36133	4.380	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	87.600%
11) 1,1-Dichloroethene-d2	2.108	63	55400	3.077	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	61.600%
20) 2-Butanone-d5	3.892	46	99886	41.501	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	83.000%
24) Chloroform-d	4.352	84	98157	5.189	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.800%
26) 1,2-Dichloroethane-d4	5.034	65	44395	4.835	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.800%
32) Benzene-d6	5.053	84	190135	4.662	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.200%
36) 1,2-Dichloropropane-d6	6.072	67	61781	5.116	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	102.400%
41) Toluene-d8	7.316	98	157016	4.454	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	89.000%
43) trans-1,3-Dichloroprop...	7.625	79	16923	4.224	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	84.400%
46) 2-Hexanone-d5	8.091	63	76260	47.233	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	94.460%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	41138	5.028	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	100.600%
66) 1,2-Dichlorobenzene-d4	11.625	152	60121	5.590	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	111.800%
Target Compounds						
					Qvalue	
13) Acetone	2.182	43	18242	13.592	ug/L	# 45
42) Toluene	7.400	91	7454	0.199	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102221\
Data File : VV022970.D
Acq On : 21 Oct 2021 21:37
Operator : SY/MD
Sample : M4265-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB7J3

Quant Time: Oct 22 04:58:03 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Oct 22 04:55:17 2021
Response via : Initial Calibration

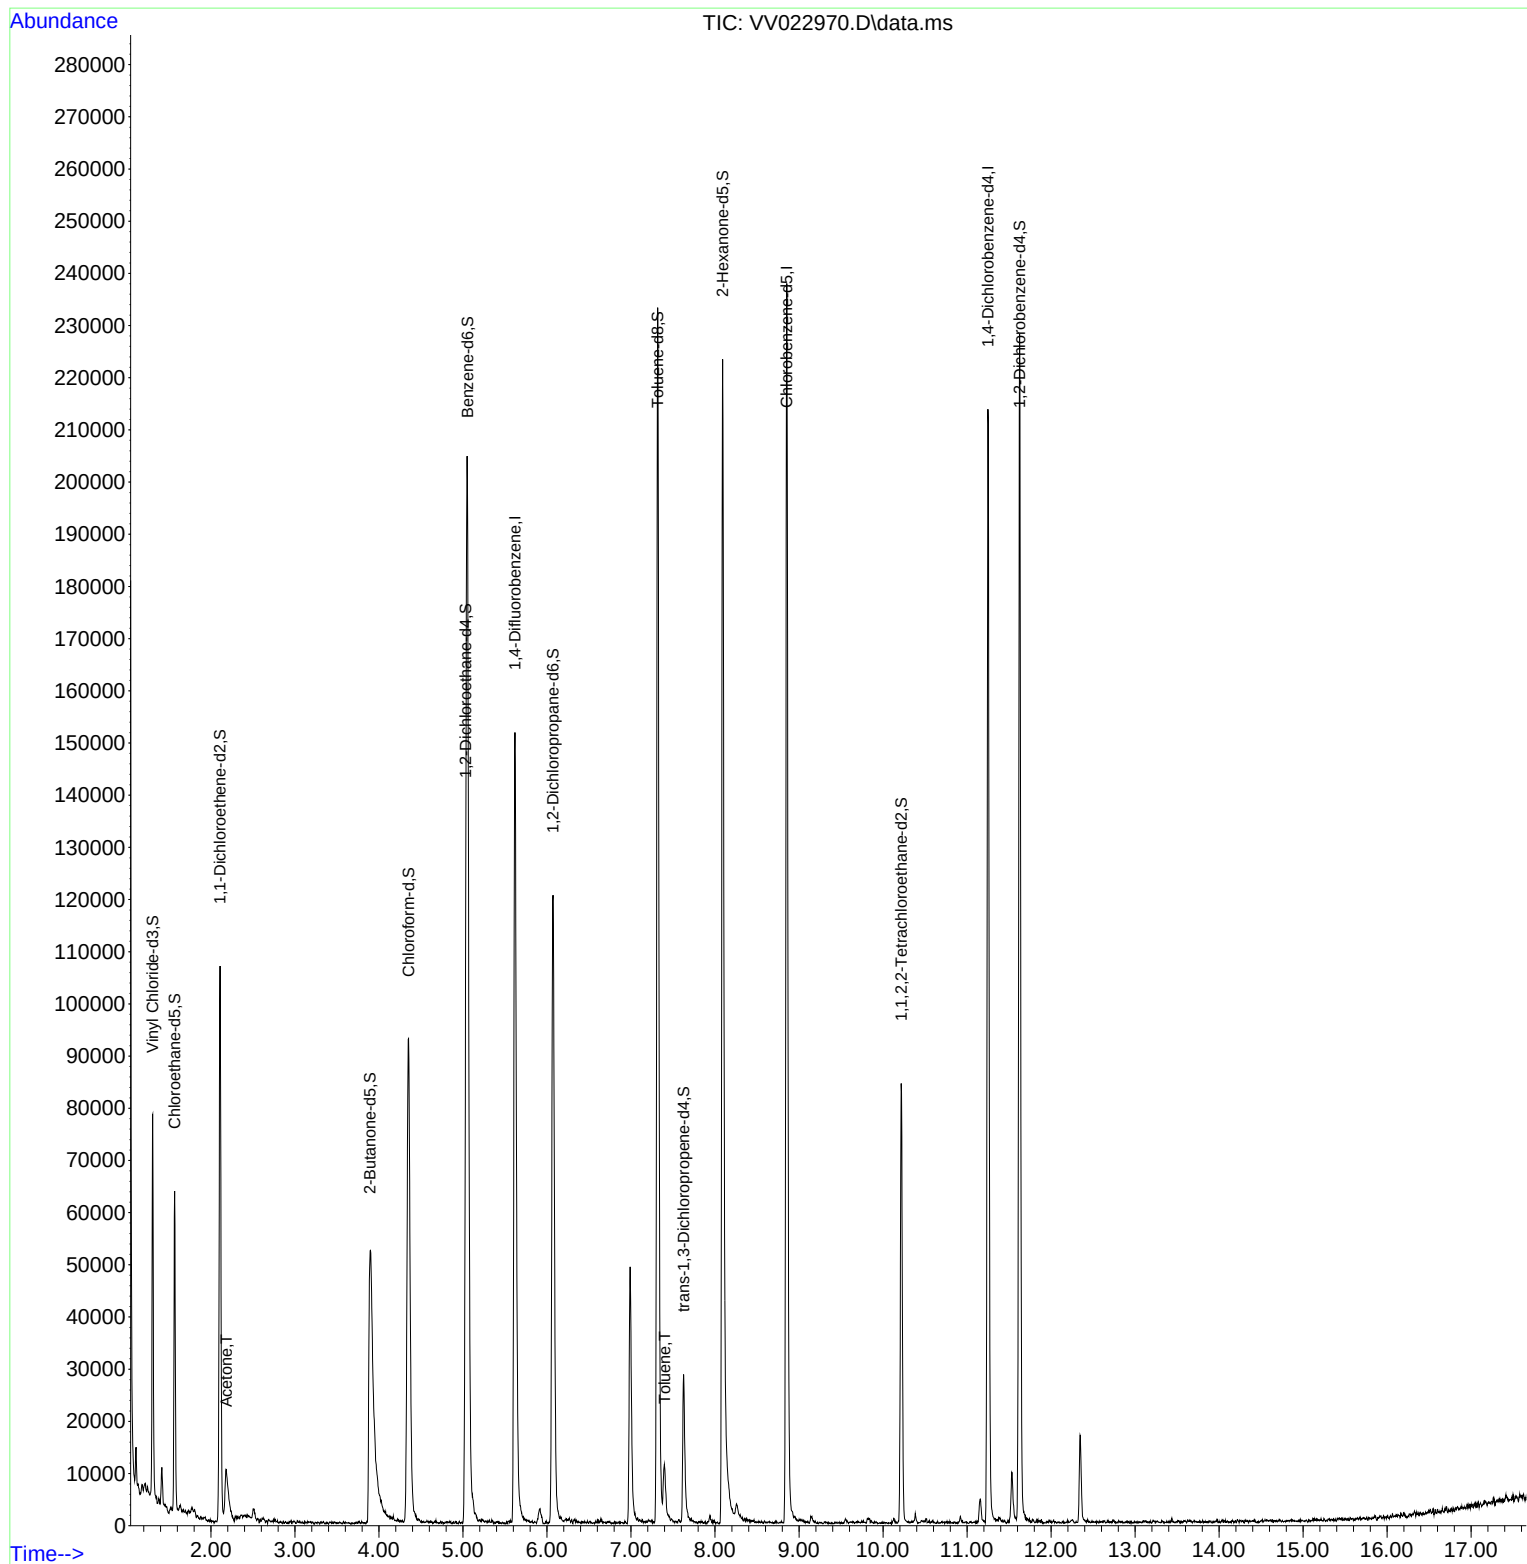

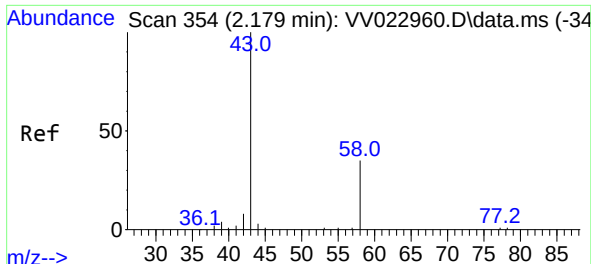

#13

Acetone

Concen: 13.592 ug/L

RT: 2.182 min Scan# 31

Delta R.T. 0.003 min

Lab File: VV022970.D

Acq: 21 Oct 2021 21:37

Instrument :

MSVOA_V

ClientSampleId :





GB7J3

Tgt Ion: 43 Resp: 18242

Ion Ratio Lower Upper

43 100

58 33.5 0.0 24.2#

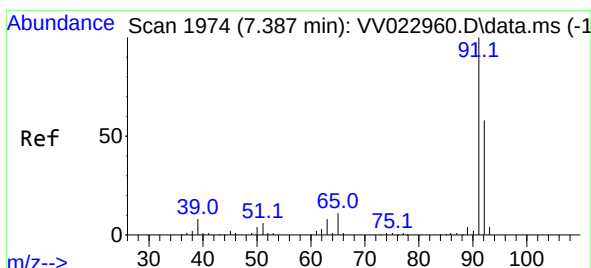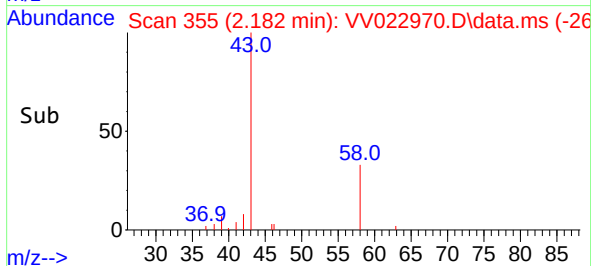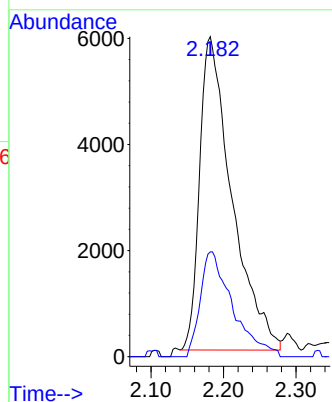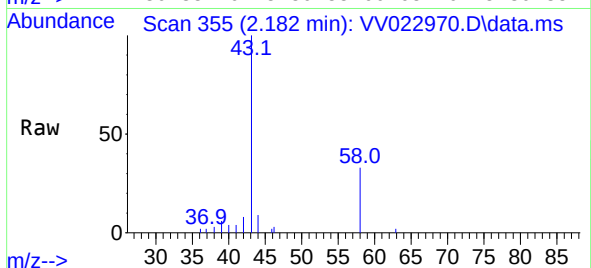

#42

Toluene

Concen: 0.199 ug/L

RT: 7.400 min Scan# 1978

Delta R.T. 0.013 min

Lab File: VV022970.D

Acq: 21 Oct 2021 21:37

Tgt Ion: 91 Resp: 7454

Ion Ratio Lower Upper

91 100

92 60.6 40.7 75.7

