

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102221\
 Data File : VV022961.D
 Acq On : 21 Oct 2021 18:02
 Operator : SY/MD
 Sample : VV1022WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK229

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV022961.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	73	82	99	rVB	101235	102409	19.90%	2.584%
2	1.561	155	162	170	rBV	53419	58711	11.41%	1.481%
3	2.101	317	330	342	rBV	127805	181461	35.26%	4.578%
4	2.500	447	454	465	rVB2	7575	12380	2.41%	0.312%
5	3.941	887	902	936	rBV	30672	145567	28.28%	3.672%
6	4.342	1011	1027	1063	rBV	93836	259296	50.38%	6.541%
7	5.040	1229	1244	1273	rBV3	221168	514664	100.00%	12.984%
8	5.612	1409	1422	1448	rBV	161425	328349	63.80%	8.283%
9	5.899	1501	1511	1524	rVB4	4171	8392	1.63%	0.212%
10	6.069	1551	1564	1592	rBV	115004	235416	45.74%	5.939%
11	6.989	1839	1850	1872	rBV	52599	102346	19.89%	2.582%
12	7.313	1938	1951	1971	rBV	237736	418739	81.36%	10.564%
13	7.391	1971	1975	1984	rVB7	3362	5847	1.14%	0.148%
14	7.625	2037	2048	2063	rBV2	31820	57779	11.23%	1.458%
15	7.940	2135	2146	2153	rBV2	3433	5934	1.15%	0.150%
16	8.098	2183	2195	2229	rBV	174036	360365	70.02%	9.091%
17	8.854	2419	2430	2445	rBV	232782	381993	74.22%	9.637%
18	10.217	2843	2854	2873	rBV	67807	109357	21.25%	2.759%
19	10.384	2897	2906	2916	rVB4	6127	9997	1.94%	0.252%
20	11.249	3164	3175	3193	rBV	221159	340734	66.21%	8.596%
21	11.625	3281	3292	3310	rBV	205074	324195	62.99%	8.179%




Sum of corrected areas: 3963931

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102221\
Data File : VV022961.D
Acq On : 21 Oct 2021 18:02
Operator : SY/MD
Sample : VV1022WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK229

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

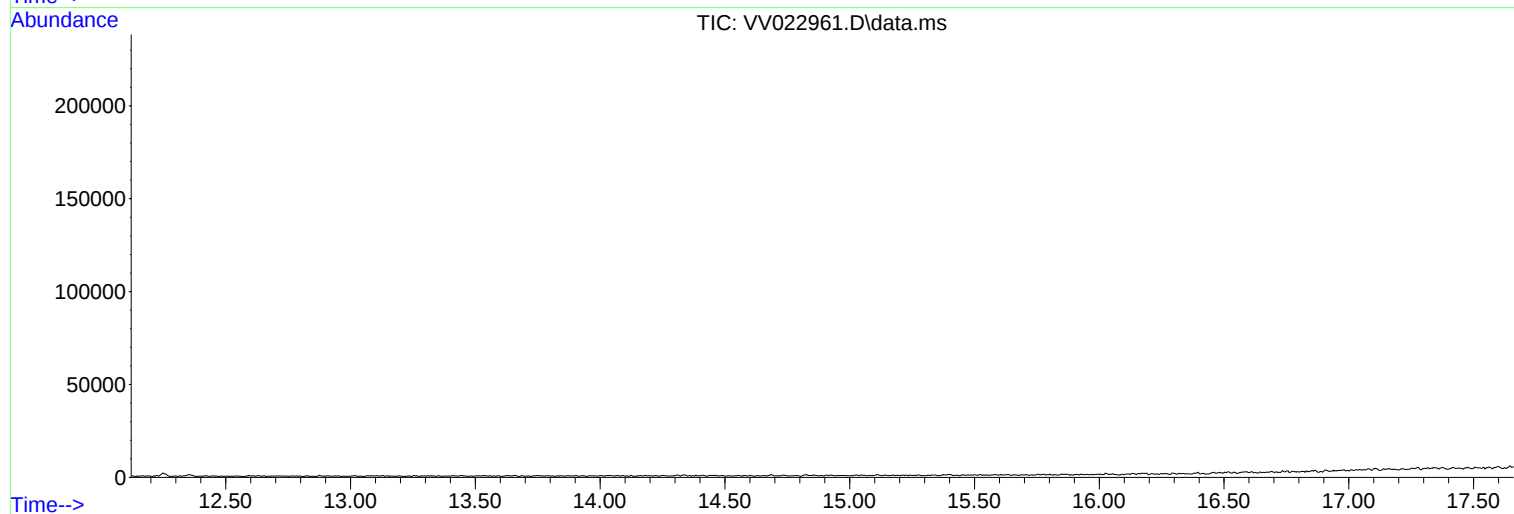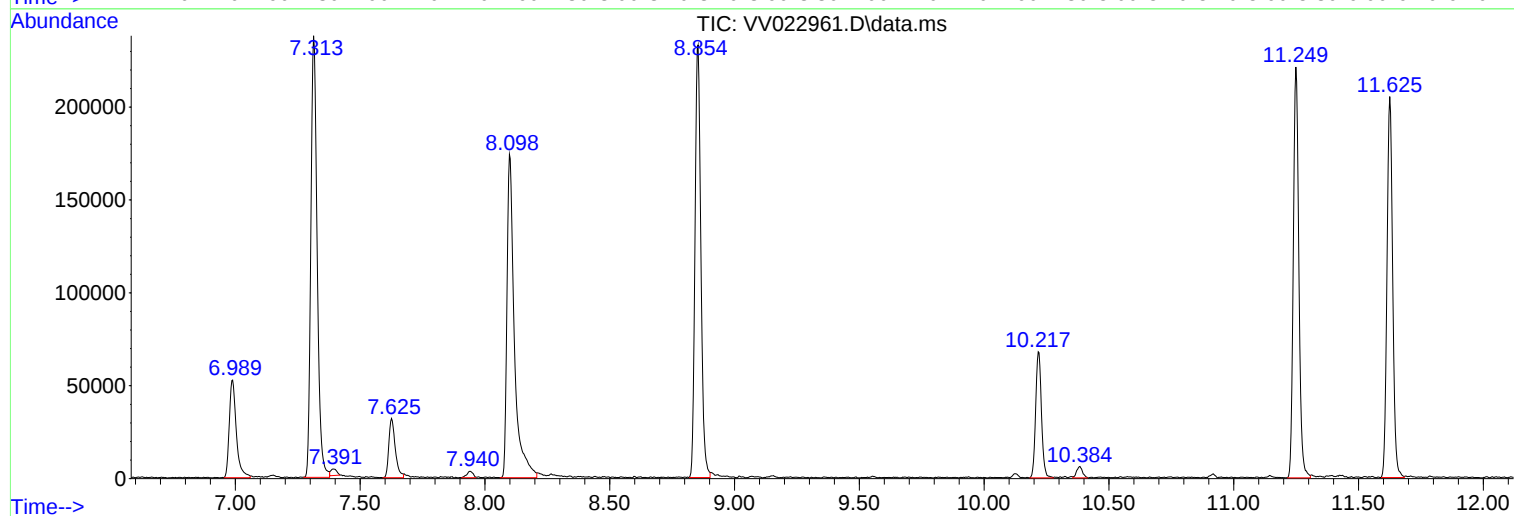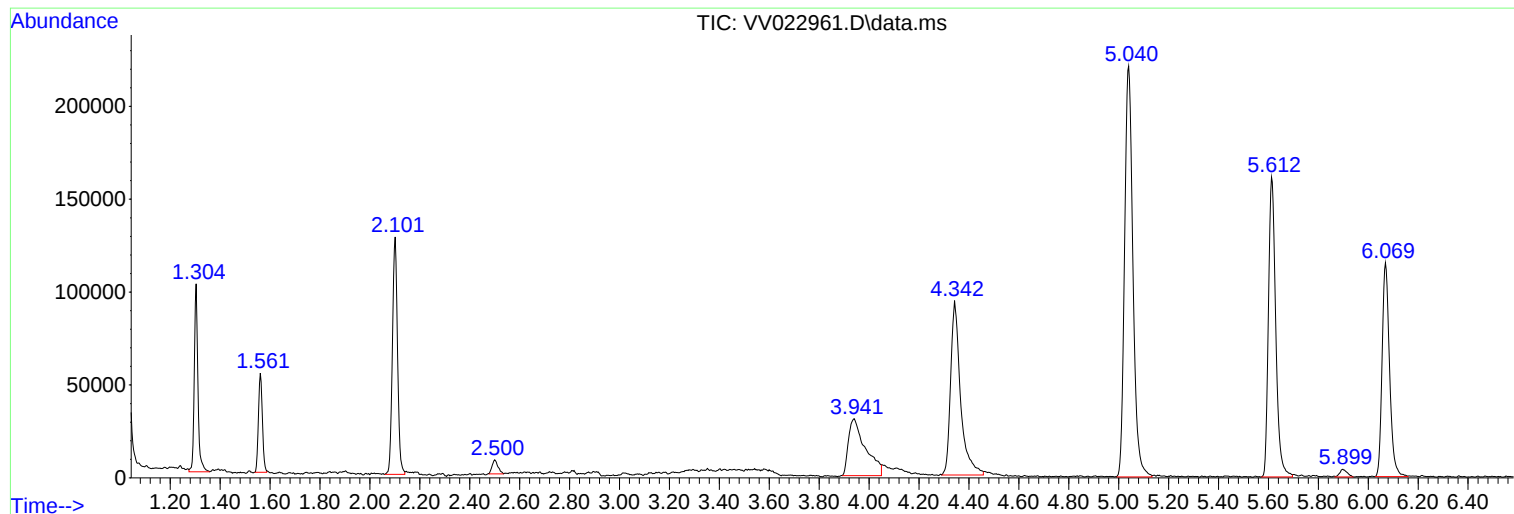

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102221\
Data File : VV022961.D
Acq On : 21 Oct 2021 18:02
Operator : SY/MD
Sample : VV1022WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK229

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102221\
Data File : VV022961.D
Acq On : 21 Oct 2021 18:02
Operator : SY/MD
Sample : VV1022WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK229

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc