

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102221\
 Data File : VV022962.D
 Acq On : 21 Oct 2021 18:26
 Operator : SY/MD
 Sample : M4200-11
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV022962.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	97	rVB	100059	106138	20.08%	2.650%
2	1.568	156	164	174	rBV	59206	67248	12.72%	1.679%
3	2.105	319	331	344	rBV	122061	175288	33.17%	4.377%
4	3.931	883	899	932	rBV	32761	137543	26.03%	3.435%
5	4.208	973	985	986	rBV8	3954	5395	1.02%	0.135%
6	4.346	1013	1028	1054	rVB	95794	244623	46.29%	6.108%
7	5.040	1229	1244	1274	rBV2	230346	528501	100.00%	13.197%
8	5.616	1409	1423	1441	rBV	168127	337315	63.82%	8.423%
9	6.072	1551	1565	1588	rBV	116238	244683	46.30%	6.110%
10	6.989	1836	1850	1871	rBV	57018	106043	20.06%	2.648%
11	7.317	1939	1952	1971	rBV	241521	425201	80.45%	10.618%
12	7.397	1973	1977	1986	rVB8	3666	5950	1.13%	0.149%
13	7.625	2038	2048	2064	rBV	34109	60263	11.40%	1.505%
14	8.101	2186	2196	2209	rBV	174269	335862	63.55%	8.387%
15	8.854	2413	2430	2451	rBV	247742	407888	77.18%	10.185%
16	10.220	2841	2855	2868	rBV	76220	123277	23.33%	3.078%
17	10.381	2899	2905	2916	rVB4	3910	6383	1.21%	0.159%
18	11.249	3165	3175	3191	rBV	223613	349401	66.11%	8.725%
19	11.625	3280	3292	3315	rBV	213537	337686	63.90%	8.432%




Sum of corrected areas: 4004688

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102221\
Data File : VV022962.D
Acq On : 21 Oct 2021 18:26
Operator : SY/MD
Sample : M4200-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

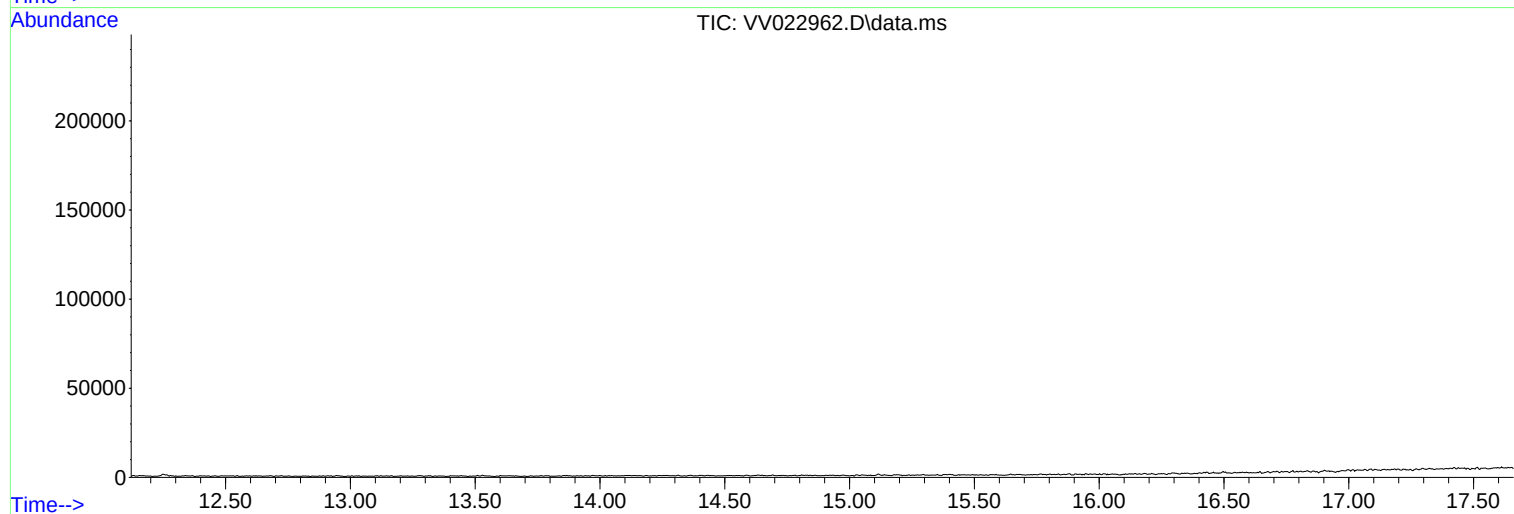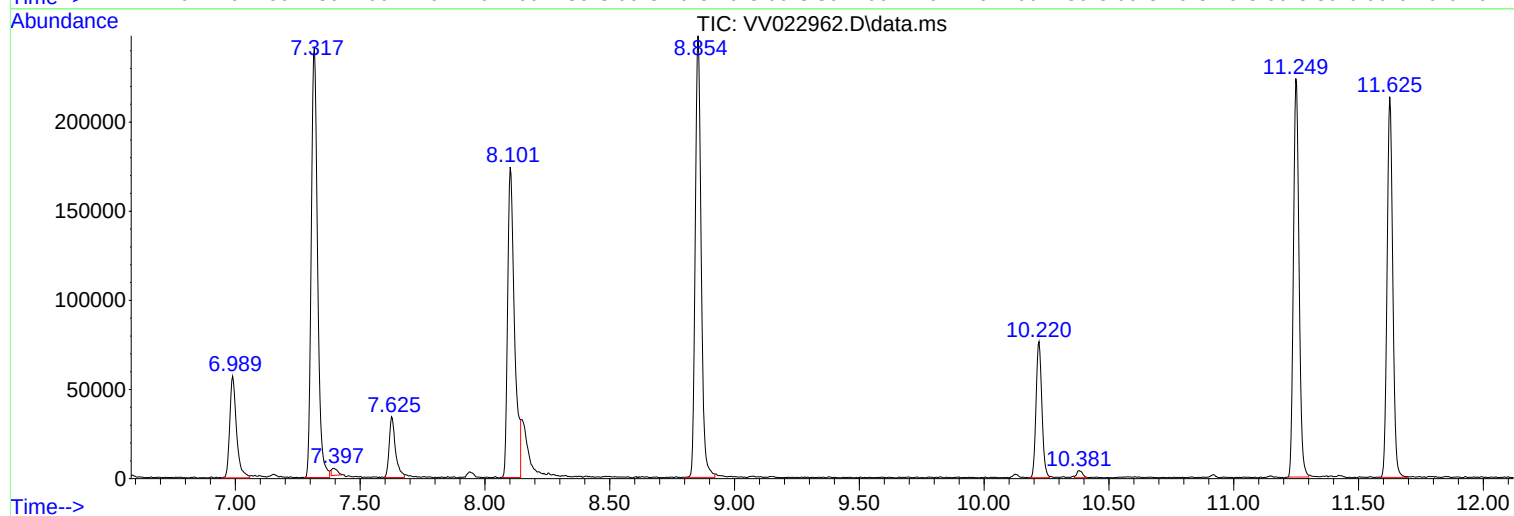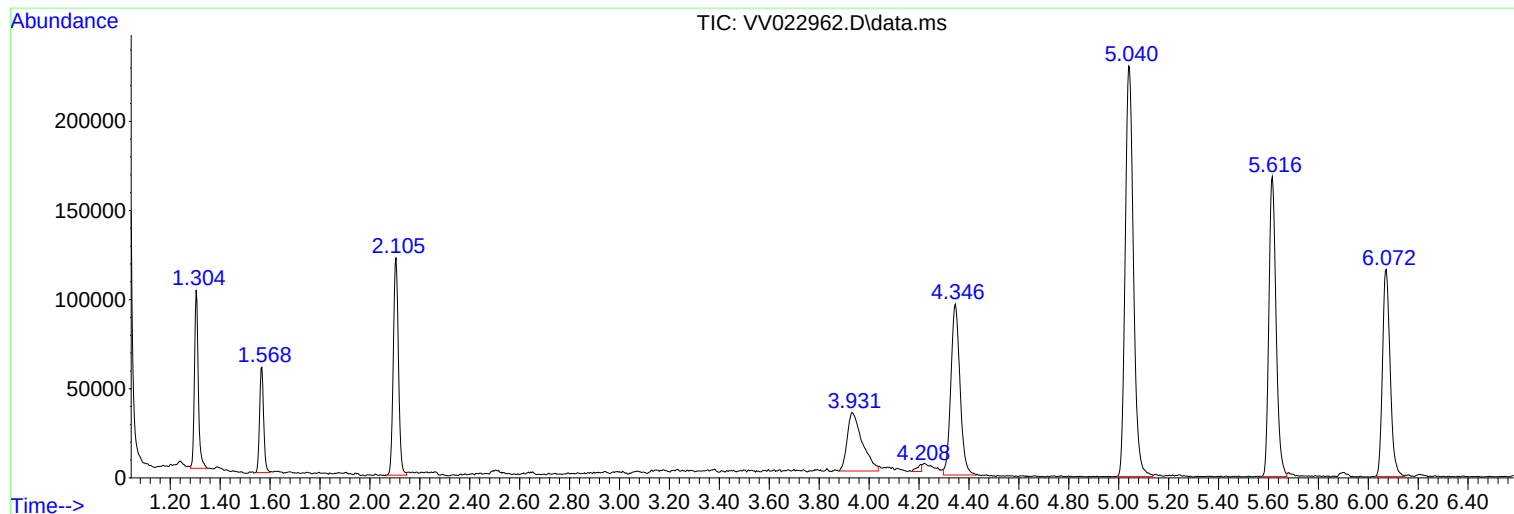

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102221\
Data File : VV022962.D
Acq On : 21 Oct 2021 18:26
Operator : SY/MD
Sample : M4200-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102221\
Data File : VV022962.D
Acq On : 21 Oct 2021 18:26
Operator : SY/MD
Sample : M4200-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc