

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102221\
 Data File : VV022991.D
 Acq On : 22 Oct 2021 16:54
 Operator : SY/MD
 Sample : M4265-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB7H5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV022991.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	74	81	98	rBV	100381	102229	18.83%	2.630%
2	1.400	106	112	122	rVB2	7584	13533	2.49%	0.348%
3	1.561	155	162	172	rVB	57915	65395	12.05%	1.683%
4	2.101	320	330	347	rVB	136665	196593	36.21%	5.058%
5	3.940	882	902	920	rBV2	30278	103963	19.15%	2.675%
6	4.346	1011	1028	1048	rBV	83670	206577	38.05%	5.315%
7	5.037	1228	1243	1269	rBV2	239029	542864	100.00%	13.967%
8	5.616	1407	1423	1450	rBV	163948	330444	60.87%	8.502%
9	5.892	1500	1509	1520	rBV10	2961	6092	1.12%	0.157%
10	6.072	1550	1565	1582	rBV	118771	242711	44.71%	6.245%
11	6.989	1838	1850	1870	rBV	53007	99772	18.38%	2.567%
12	7.313	1939	1951	1967	rBV	219638	386229	71.15%	9.937%
13	7.391	1967	1975	1993	rVB	17097	32188	5.93%	0.828%
14	7.625	2038	2048	2066	rBV	32800	58204	10.72%	1.498%
15	8.104	2186	2197	2232	rBV	176414	374598	69.00%	9.638%
16	8.853	2418	2430	2450	rBV	241209	395069	72.77%	10.165%
17	10.220	2843	2855	2874	rBV	73552	117786	21.70%	3.030%
18	11.249	3165	3175	3194	rBV	199338	306673	56.49%	7.890%
19	11.538	3255	3265	3273	rBV4	10565	17753	3.27%	0.457%
20	11.625	3281	3292	3308	rBV	181271	288015	53.05%	7.410%




Sum of corrected areas: 3886688

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102221\
Data File : VV022991.D
Acq On : 22 Oct 2021 16:54
Operator : SY/MD
Sample : M4265-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB7H5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

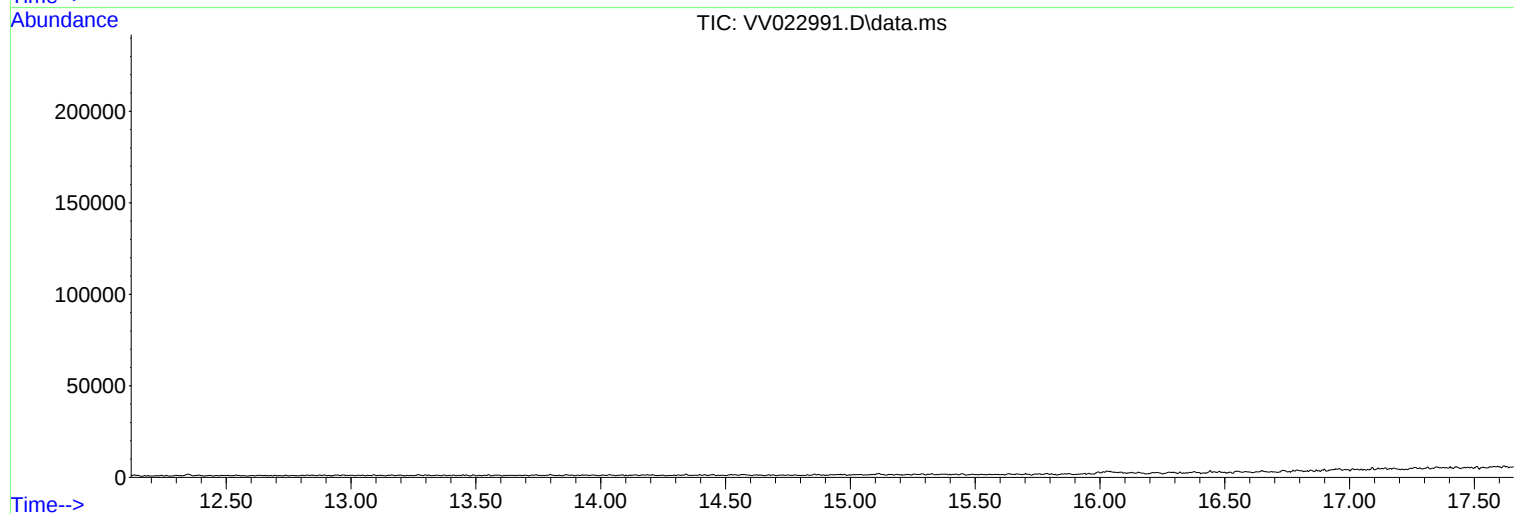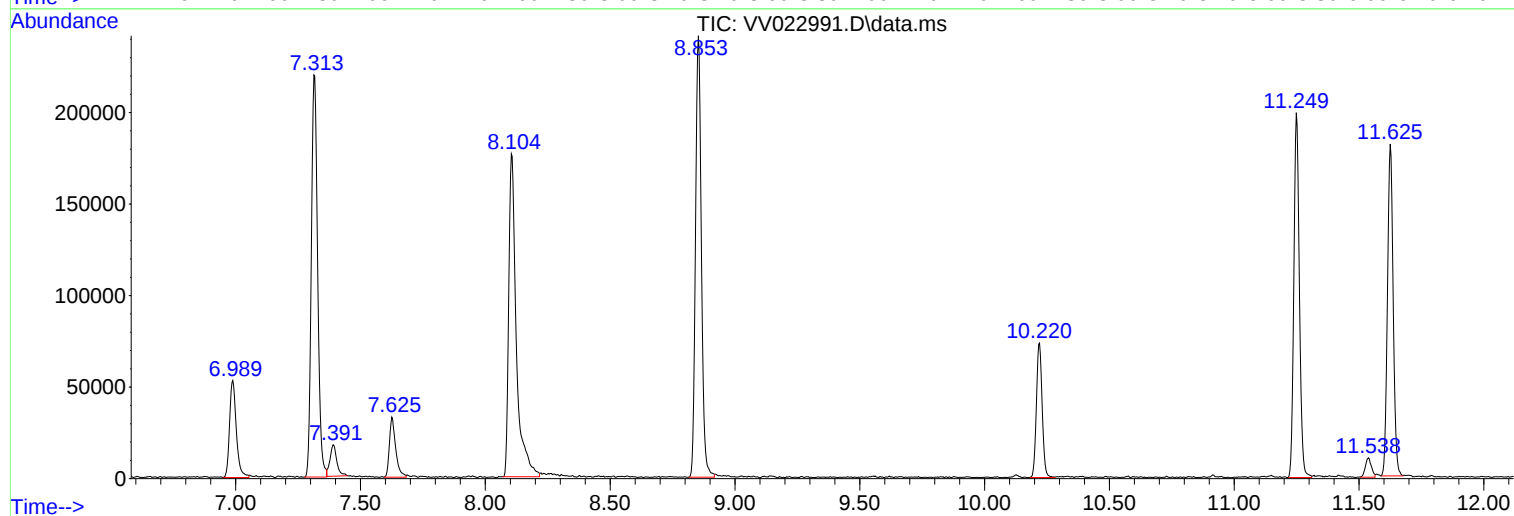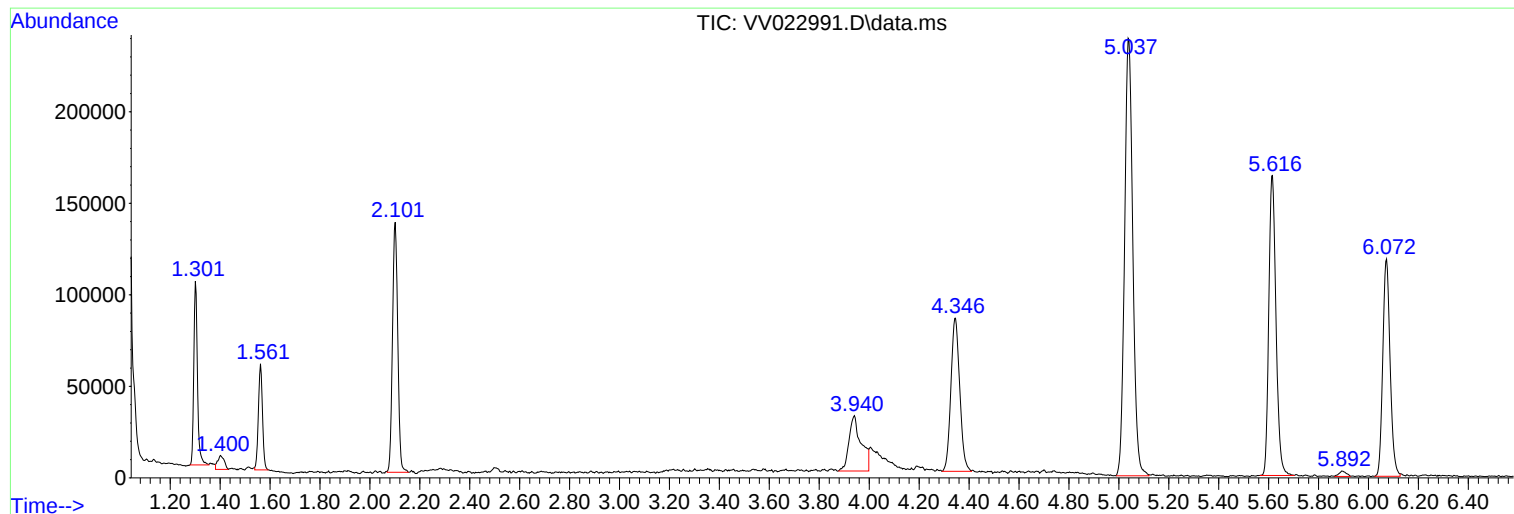

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102221\
Data File : VV022991.D
Acq On : 22 Oct 2021 16:54
Operator : SY/MD
Sample : M4265-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB7H5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102221\
Data File : VV022991.D
Acq On : 22 Oct 2021 16:54
Operator : SY/MD
Sample : M4265-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB7H5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc