

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102221\
 Data File : VV022996.D
 Acq On : 22 Oct 2021 18:53
 Operator : SY/MD
 Sample : M4265-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB7J0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV022996.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.089	10	15	26	rVB	16088	20053	3.60%	0.487%
2	1.304	74	82	93	rBV2	94805	103850	18.65%	2.521%
3	1.410	109	115	123	rVB	12314	13312	2.39%	0.323%
4	1.561	155	162	176	rBV	66674	74926	13.46%	1.819%
5	2.101	320	330	344	rBV	119649	170871	30.69%	4.147%
6	2.233	358	371	380	rBV4	4677	12719	2.28%	0.309%
7	3.957	888	907	926	rBV	38178	162149	29.12%	3.936%
8	4.346	1008	1028	1048	rBV	91508	224713	40.36%	5.454%
9	5.040	1228	1244	1272	rBV2	247866	556808	100.00%	13.515%
10	5.616	1407	1423	1446	rBV	151824	304117	54.62%	7.381%
11	5.895	1503	1510	1522	rVB9	3564	6468	1.16%	0.157%
12	6.072	1551	1565	1587	rBV	126557	260773	46.83%	6.329%
13	6.989	1838	1850	1868	rBV	55627	105158	18.89%	2.552%
14	7.317	1937	1952	1967	rBV	239554	423185	76.00%	10.271%
15	7.391	1968	1975	1990	rVB2	15823	31893	5.73%	0.774%
16	7.628	2039	2049	2065	rBV2	32957	61033	10.96%	1.481%
17	8.104	2186	2197	2234	rBV	206657	429397	77.12%	10.422%
18	8.854	2419	2430	2457	rBV	226001	370414	66.52%	8.991%
19	10.217	2844	2854	2873	rBV2	81921	132736	23.84%	3.222%
20	11.249	3165	3175	3195	rBV	194057	302647	54.35%	7.346%
21	11.535	3253	3264	3276	rBV4	9877	17071	3.07%	0.414%
22	11.625	3279	3292	3310	rVV	212252	335736	60.30%	8.149%


Sum of corrected areas: 4120029

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102221\
Data File : VV022996.D
Acq On : 22 Oct 2021 18:53
Operator : SY/MD
Sample : M4265-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB7J0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

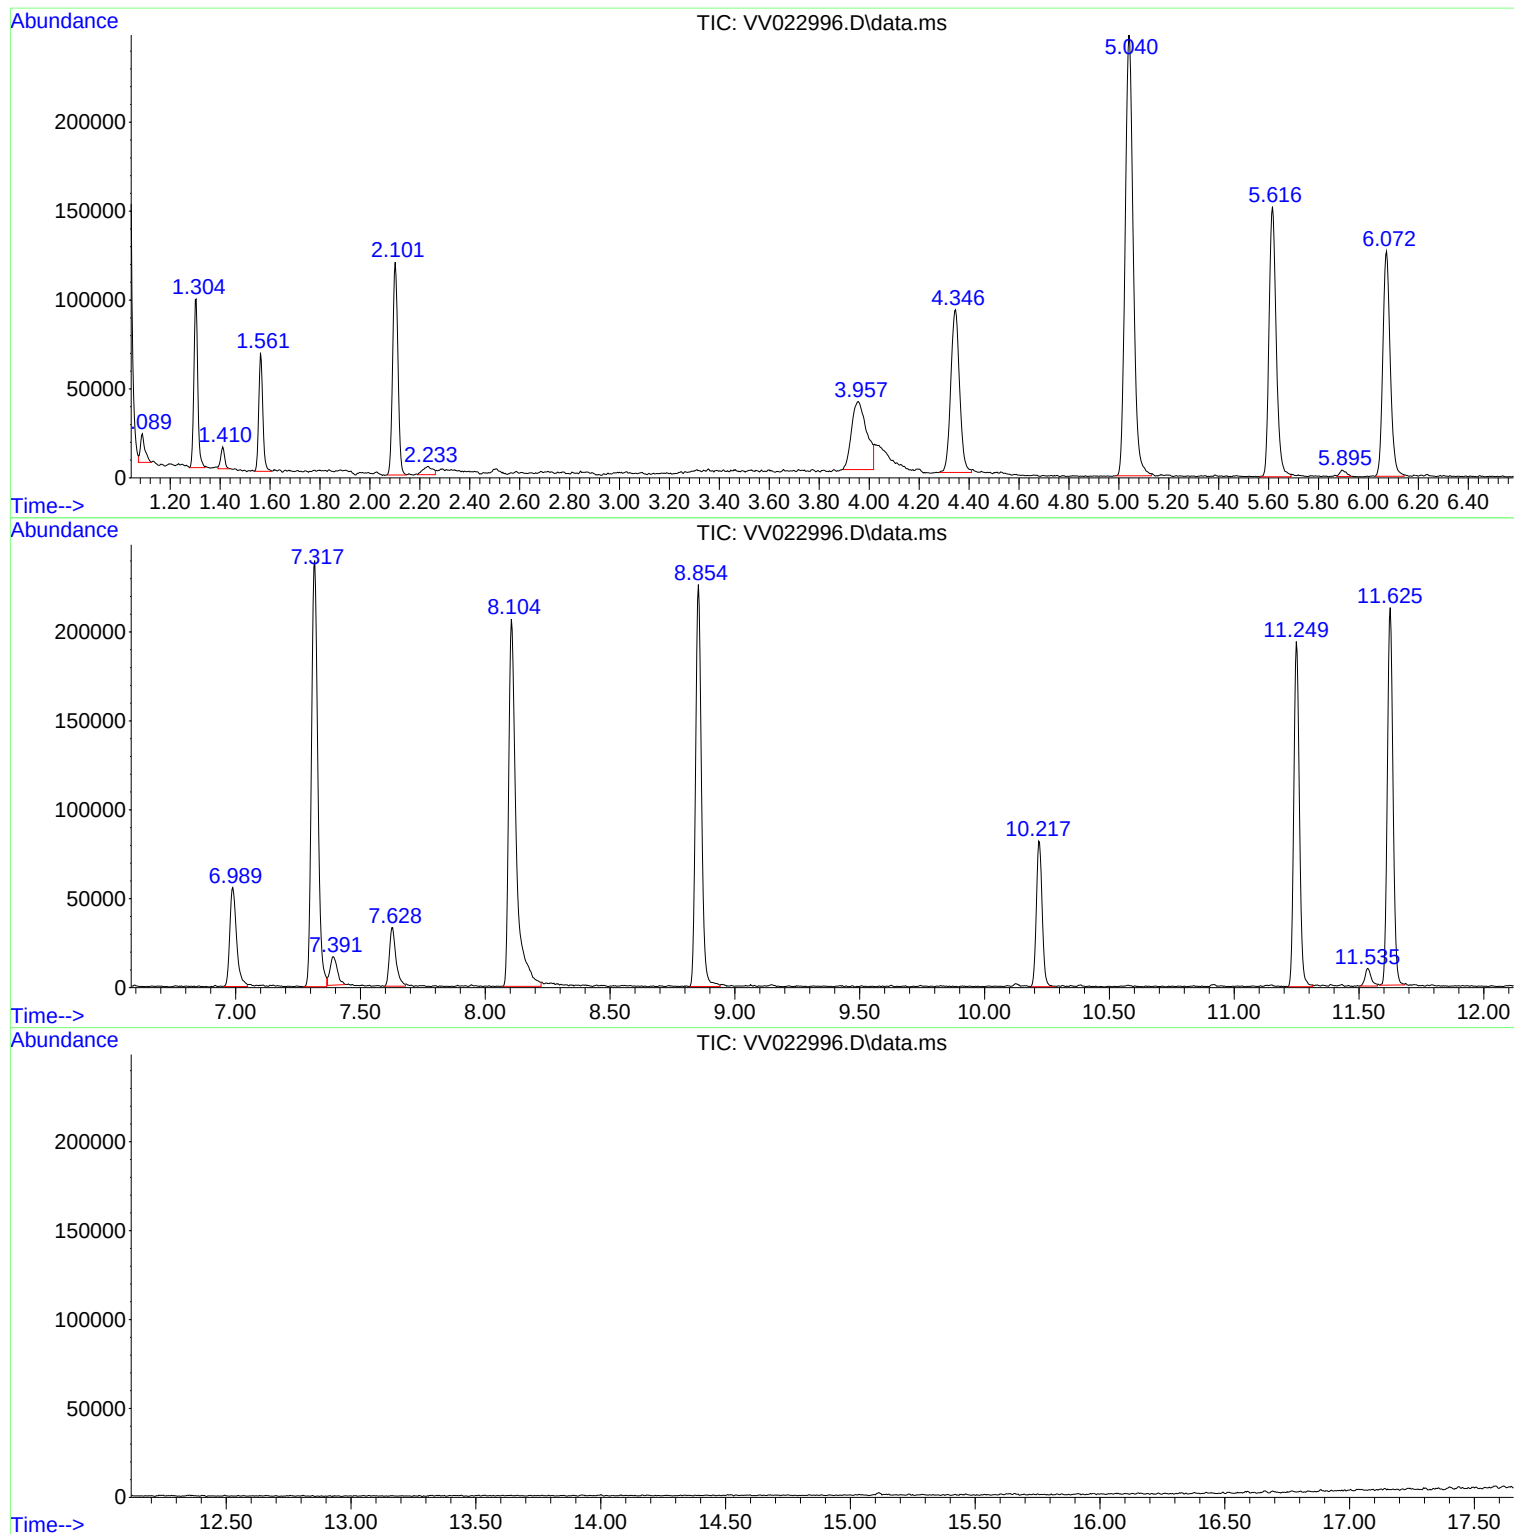

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102221\
Data File : VV022996.D
Acq On : 22 Oct 2021 18:53
Operator : SY/MD
Sample : M4265-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB7J0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102221\
Data File : VV022996.D
Acq On : 22 Oct 2021 18:53
Operator : SY/MD
Sample : M4265-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB7J0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc