

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102221\
 Data File : VV022998.D
 Acq On : 22 Oct 2021 19:41
 Operator : SY/MD
 Sample : M4265-15
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB7J7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV022998.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	74	82	95	rBV	91008	94994	17.51%	2.478%
2	1.561	154	162	179	rBV	66611	76033	14.01%	1.983%
3	2.101	319	330	345	rVB	122350	178314	32.87%	4.651%
4	3.953	885	906	924	rBV2	24472	102072	18.81%	2.663%
5	4.346	1008	1028	1047	rBV2	86391	214664	39.57%	5.600%
6	5.040	1228	1244	1275	rBV2	238653	542535	100.00%	14.152%
7	5.616	1408	1423	1444	rBV	147097	298011	54.93%	7.774%
8	5.895	1501	1510	1520	rBV5	5935	11841	2.18%	0.309%
9	6.072	1550	1565	1582	rBV	121032	246235	45.39%	6.423%
10	6.989	1839	1850	1868	rBV	51726	96546	17.80%	2.518%
11	7.317	1940	1952	1968	rBV	225672	394834	72.78%	10.299%
12	7.394	1969	1976	1987	rVB	9727	17158	3.16%	0.448%
13	7.625	2039	2048	2065	rBV	32105	57817	10.66%	1.508%
14	8.104	2187	2197	2226	rBV2	183660	397645	73.29%	10.373%
15	8.854	2418	2430	2457	rBV	215772	356099	65.64%	9.289%
16	10.217	2842	2854	2870	rBV	71577	114617	21.13%	2.990%
17	11.249	3161	3175	3197	rBV	191711	295251	54.42%	7.702%
18	11.535	3256	3264	3275	rBV2	8784	14618	2.69%	0.381%
19	11.625	3281	3292	3309	rBV	205847	318410	58.69%	8.306%
20	12.349	3509	3517	3525	rBV6	4337	5854	1.08%	0.153%


Sum of corrected areas: 3833548

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102221\
Data File : VV022998.D
Acq On : 22 Oct 2021 19:41
Operator : SY/MD
Sample : M4265-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB7J7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

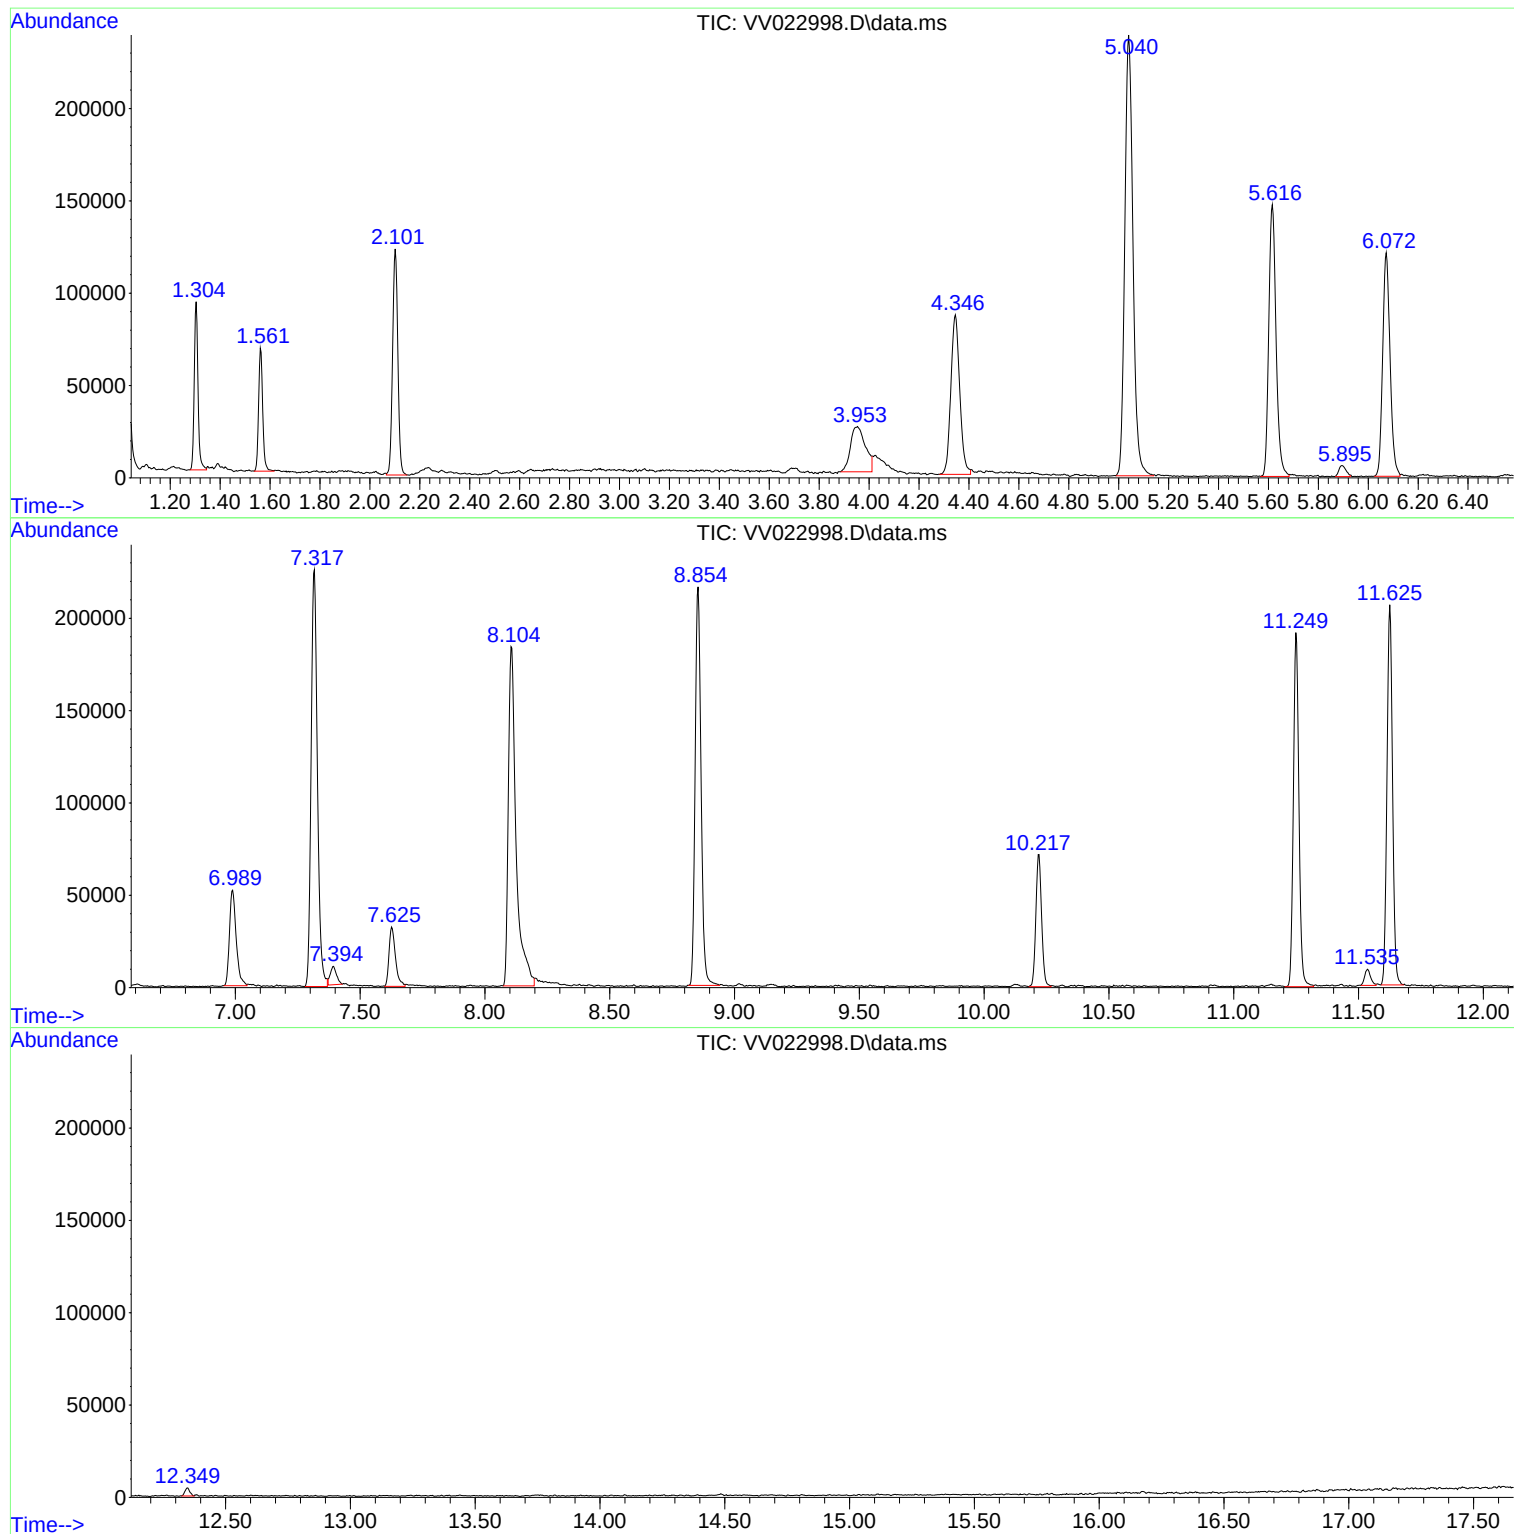

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102221\
Data File : VV022998.D
Acq On : 22 Oct 2021 19:41
Operator : SY/MD
Sample : M4265-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB7J7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102221\
Data File : VV022998.D
Acq On : 22 Oct 2021 19:41
Operator : SY/MD
Sample : M4265-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB7J7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc