


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102221\
 Data File : VV022978.D
 Acq On : 22 Oct 2021 09:32
 Operator : SY/MD
 Sample : BFB220
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB220

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Mon Oct 25 01:03:32 2021

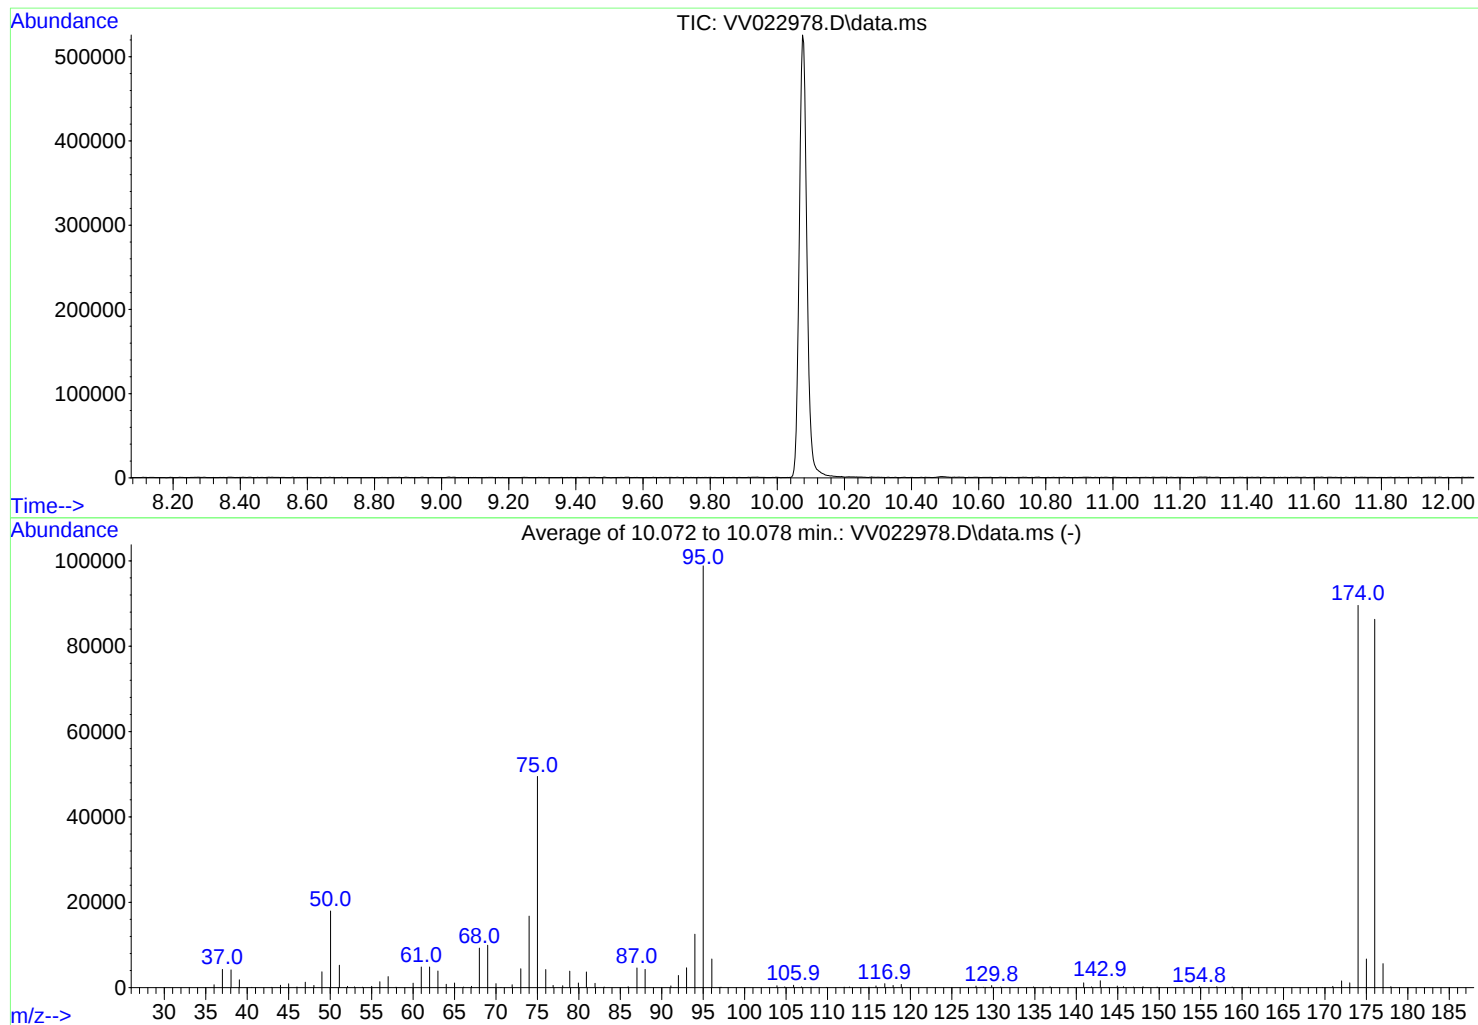

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2797

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.2	17965	PASS
75	95	30	80	50.1	49485	PASS
95	95	100	100	100.0	98829	PASS
96	95	5	9	6.8	6709	PASS
173	174	0.00	2	1.3	1135	PASS
174	95	50	120	90.6	89565	PASS
175	174	5	9	7.5	6727	PASS
176	174	95	105	96.4	86301	PASS
177	176	5	10	6.5	5611	PASS

m/z	Abundance
36.00	654.0
37.00	4228.0
38.10	4170.0
39.10	1893.0
40.10	174.0
40.60	124.0
44.00	845.0
45.00	881.0
46.10	149.0
47.00	1239.0
48.10	498.0
49.00	3700.0
50.00	17464.0
51.10	5152.0
52.10	314.0
53.00	148.0
53.90	106.0
55.00	262.0
56.00	1320.0
57.00	2562.0
58.00	136.0
60.00	1087.0
61.00	4908.0
62.00	4821.0
63.00	3863.0
64.00	806.0
65.00	1023.0
66.10	151.0
67.00	283.0
68.00	9367.0
69.00	9839.0
70.00	906.0
71.90	680.0
73.00	4600.0
74.00	16904.0
75.00	49736.0
76.00	4314.0
76.90	536.0
78.10	473.0
78.90	3843.0
79.90	1099.0
80.90	3589.0
81.90	1001.0
82.90	177.0
86.00	194.0
87.00	4846.0
88.00	4230.0
91.10	491.0
92.00	2765.0
93.00	4570.0
94.00	12566.0
95.00	100144.0
96.00	6569.0
96.90	197.0
103.90	456.0
104.90	261.0
105.90	553.0
106.80	160.0
107.90	104.0
109.90	135.0
112.00	135.0
112.70	138.0
115.00	156.0
115.80	398.0
116.90	835.0
117.90	528.0
118.90	770.0
127.90	342.0
128.80	164.0
129.80	556.0
130.90	170.0
134.80	249.0
136.90	231.0
139.80	117.0
140.90	1099.0
141.90	176.0
142.90	1613.0
143.90	113.0
144.90	400.0
145.70	243.0
146.90	145.0
148.00	253.0
149.70	180.0
154.80	250.0
157.00	232.0
158.80	181.0
160.80	147.0
170.90	286.0
172.00	1716.0
173.00	1160.0
174.00	93528.0
175.00	6860.0

Instrument :
MSVOA_V
ClientSampleId :
BFB220

176.00

177.00

178.00

89088.0

5521.0

227.0

Instrument :

MSVOA_V

ClientSampleId :

BFB220

m/z	Abundance
39.90	215.0
44.00	274.0

Instrument :
MSVOA_V
ClientSampleId :
BFB220

m/z	Abundance
36.00	701.0
37.00	4221.0
38.00	4021.0
39.00	1704.0
40.00	249.0
42.90	120.0
44.10	778.0
45.00	856.0
45.90	141.0
47.00	1230.0
48.00	509.0
49.00	3581.0
50.10	17880.0
51.10	5172.0
52.10	241.0
52.90	204.0
53.90	117.0
55.00	312.0
56.00	1439.0
57.00	2593.0
57.90	136.0
60.00	974.0
61.00	4619.0
62.00	4682.0
63.00	3813.0
64.00	715.0
65.00	1113.0
66.10	171.0
67.10	340.0
68.00	8861.0
69.00	9656.0
70.00	930.0
70.60	102.0
72.00	660.0
73.00	4144.0
74.00	16116.0
75.00	47224.0
76.00	3983.0
76.90	548.0
78.00	413.0
78.90	3744.0
80.00	1020.0
80.90	3659.0
82.00	995.0
83.10	151.0
85.90	239.0
87.00	4197.0
88.00	4189.0
91.10	307.0
92.00	2806.0
93.00	4526.0
94.00	11968.0
95.00	94280.0
96.00	6639.0
97.20	171.0
103.90	408.0
104.80	139.0
105.90	565.0
106.90	178.0
108.10	118.0
112.00	117.0
112.60	138.0
115.90	401.0
116.90	950.0
117.90	495.0
118.90	701.0
127.90	375.0
129.10	149.0
129.80	403.0
130.90	129.0
134.90	172.0
136.80	176.0
140.90	1084.0
141.80	182.0
142.90	1531.0
145.00	357.0
145.70	200.0
146.90	161.0
148.10	222.0
149.80	132.0
154.90	275.0
156.90	180.0
158.80	109.0
160.80	113.0
171.00	271.0
172.00	1396.0
173.00	1074.0
174.00	82856.0
175.00	6381.0
176.00	80384.0
177.00	5504.0
177.90	202.0

Instrument :
MSVOA_V
ClientSampleId :
BFB220

m/z	Abundance
36.00	664.0
37.00	4427.0
38.10	4250.0
39.00	1911.0
40.00	216.0
40.50	129.0
42.90	116.0
44.00	867.0
45.00	928.0
46.00	144.0
47.00	1371.0
48.10	550.0
49.00	3851.0
50.00	18552.0
51.10	5423.0
52.10	307.0
52.90	211.0
53.90	110.0
55.00	297.0
56.00	1433.0
57.00	2653.0
58.00	125.0
60.00	1076.0
61.00	5034.0
62.00	5007.0
63.00	4043.0
64.00	806.0
65.00	1166.0
66.10	174.0
67.00	323.0
68.00	9537.0
69.00	10343.0
70.00	950.0
71.90	727.0
73.00	4492.0
74.00	17280.0
75.00	51496.0
76.00	4448.0
76.90	558.0
78.00	444.0
78.90	4016.0
80.00	1124.0
80.90	3770.0
82.00	1060.0
83.10	163.0
85.90	220.0
87.00	4794.0
88.00	4431.0
91.10	416.0
92.00	2958.0
93.00	4799.0
94.00	13091.0
95.00	102064.0
96.10	6920.0
97.10	171.0
103.90	470.0
104.90	210.0
105.90	584.0
106.90	185.0
108.00	102.0
109.90	125.0
112.00	129.0
112.60	152.0
115.00	135.0
115.90	432.0
116.90	978.0
117.90	547.0
118.90	788.0
127.90	371.0
128.80	157.0
129.80	494.0
130.90	154.0
134.90	199.0
136.90	206.0
140.90	1185.0
141.90	171.0
142.90	1661.0
144.90	386.0
145.70	256.0
146.90	162.0
148.10	252.0
149.70	180.0
154.80	284.0
156.90	213.0
158.80	143.0
160.80	129.0
169.70	105.0
170.90	304.0
172.00	1651.0
173.00	1172.0
174.00	92312.0
175.00	6941.0

Instrument :
MSVOA_V
ClientSampleId :
BFB220

176.00	89432.0
177.00	5808.0
178.00	215.0

Instrument :
MSVOA_V
ClientSampleId :
BFB220