


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV102318\
 Data File : VV008380.D
 Acq On : 23 Oct 2018 17:03
 Operator : SY/MD
 Sample : BFB48
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB48

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102318WMA.M
 Title : VOC Analysis
 Last Update : Wed Oct 24 02:41:57 2018

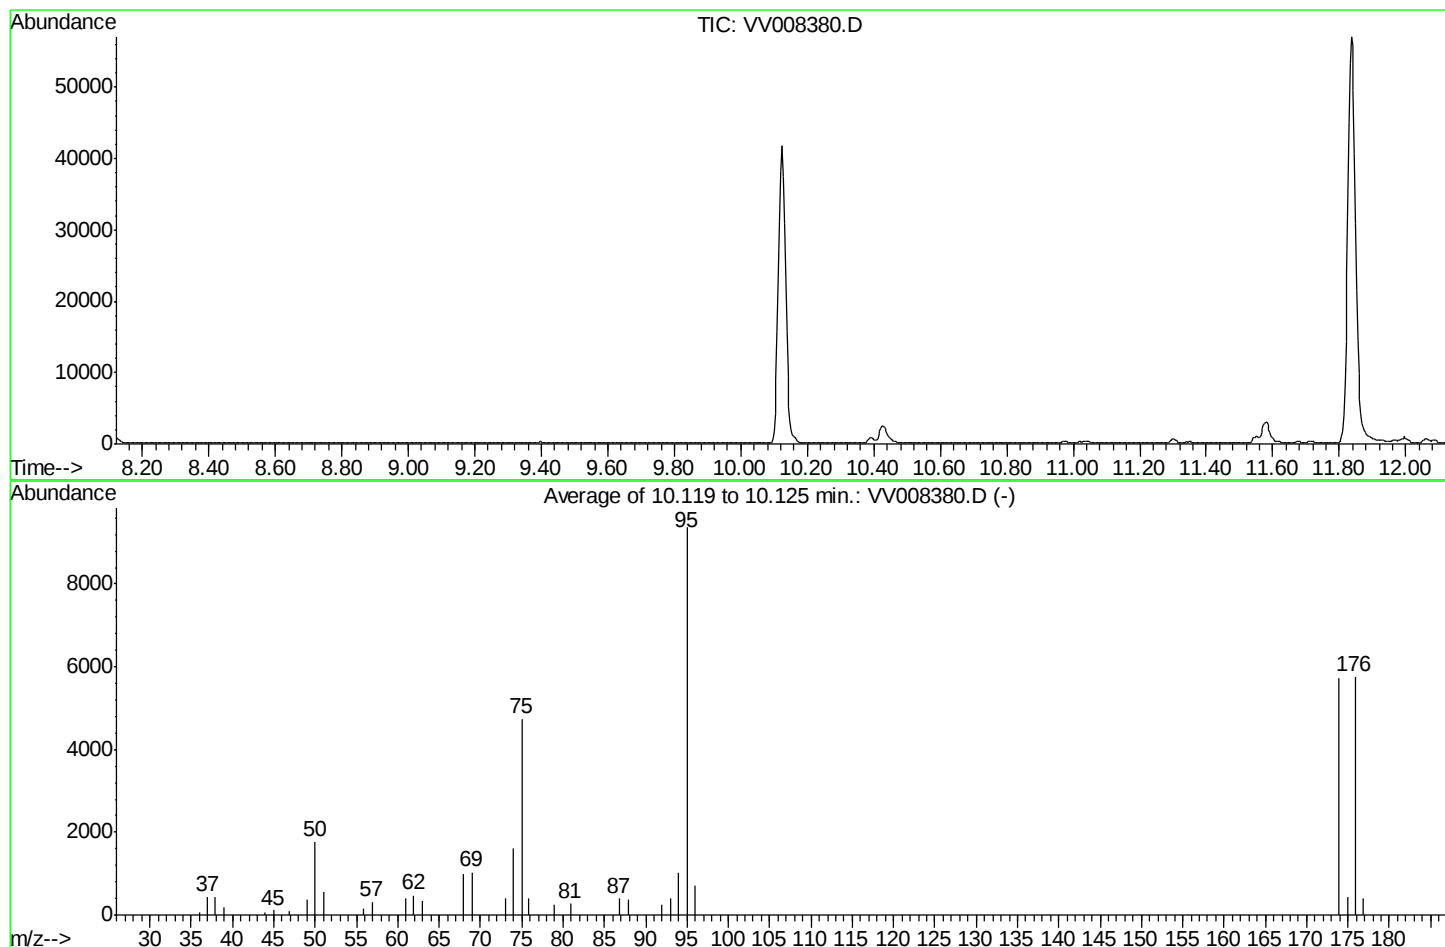

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2799

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.9	1771	PASS
75	95	30	80	50.5	4736	PASS
95	95	100	100	100.0	9370	PASS
96	95	5	9	7.6	710	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	61.0	5720	PASS
175	174	5	9	7.7	440	PASS
176	174	95	101	100.7	5762	PASS
177	176	5	9	6.9	400	PASS

m/z	Abundance
36.00	108.0
37.00	404.0
37.90	409.0
38.90	177.0
43.90	252.0
44.90	112.0
46.90	108.0
48.90	350.0
50.00	1685.0
51.00	553.0
55.90	151.0
56.90	292.0
61.00	368.0
61.90	460.0
63.00	330.0
68.00	911.0
69.00	949.0
73.00	376.0
74.00	1524.0
75.00	4531.0
75.90	371.0
78.90	257.0
80.90	275.0
86.80	350.0
87.90	316.0
91.90	244.0
93.00	376.0
94.00	933.0
95.00	8865.0
96.00	736.0
173.90	5290.0
174.90	429.0
175.90	5296.0
176.90	401.0

Instrument :
MSVOA_V
ClientSampleId :
BFB48

m/z	Abundance
43.90	173.0

Instrument :
MSVOA_V
ClientSampleId :
BFB48

m/z	Abundance
36.90	473.0
37.90	439.0
38.90	184.0
43.90	231.0
45.00	124.0
46.80	105.0
49.00	373.0
50.00	1795.0
51.00	527.0
55.90	155.0
56.90	314.0
60.90	451.0
61.90	475.0
62.90	335.0
68.00	1025.0
69.00	1058.0
73.00	392.0
74.00	1644.0
75.00	4807.0
75.90	420.0
78.90	241.0
80.90	270.0
86.80	426.0
87.90	407.0
91.90	244.0
93.00	411.0
94.00	1057.0
95.00	9560.0
96.00	668.0
173.90	5994.0
174.90	445.0
175.90	6017.0
176.90	378.0

Instrument :
MSVOA_V
ClientSampleId :
BFB48

m/z	Abundance
35.90	112.0
37.00	462.0
37.90	455.0
38.90	192.0
43.90	252.0
44.90	125.0
46.80	108.0
49.00	382.0
50.00	1834.0
51.00	567.0
55.90	163.0
56.90	325.0
61.00	415.0
61.90	499.0
62.90	337.0
68.00	1024.0
69.00	1063.0
73.00	400.0
74.00	1677.0
75.00	4871.0
75.90	407.0
78.90	262.0
80.90	291.0
86.80	395.0
87.90	399.0
91.90	248.0
93.00	412.0
94.00	1039.0
95.00	9686.0
96.00	727.0
173.90	5878.0
174.90	446.0
175.90	5974.0
176.90	421.0

Instrument :
MSVOA_V
ClientSampleId :
BFB48