

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102319\
Quantitation Report (QT Reviewed)


Data File : VV013301.D
Acq On : 23 Oct 2019 14:58
Operator : SY/MD
Sample : K5395-04
Misc : 5.00ML/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0042

Manual Integrations
APPROVED

MMDadoda
10/24/2019 10:45:27 AM

Quant Time: Oct 24 03:59:28 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102319WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Oct 24 02:50:44 2019
Response via : Initial Calibration

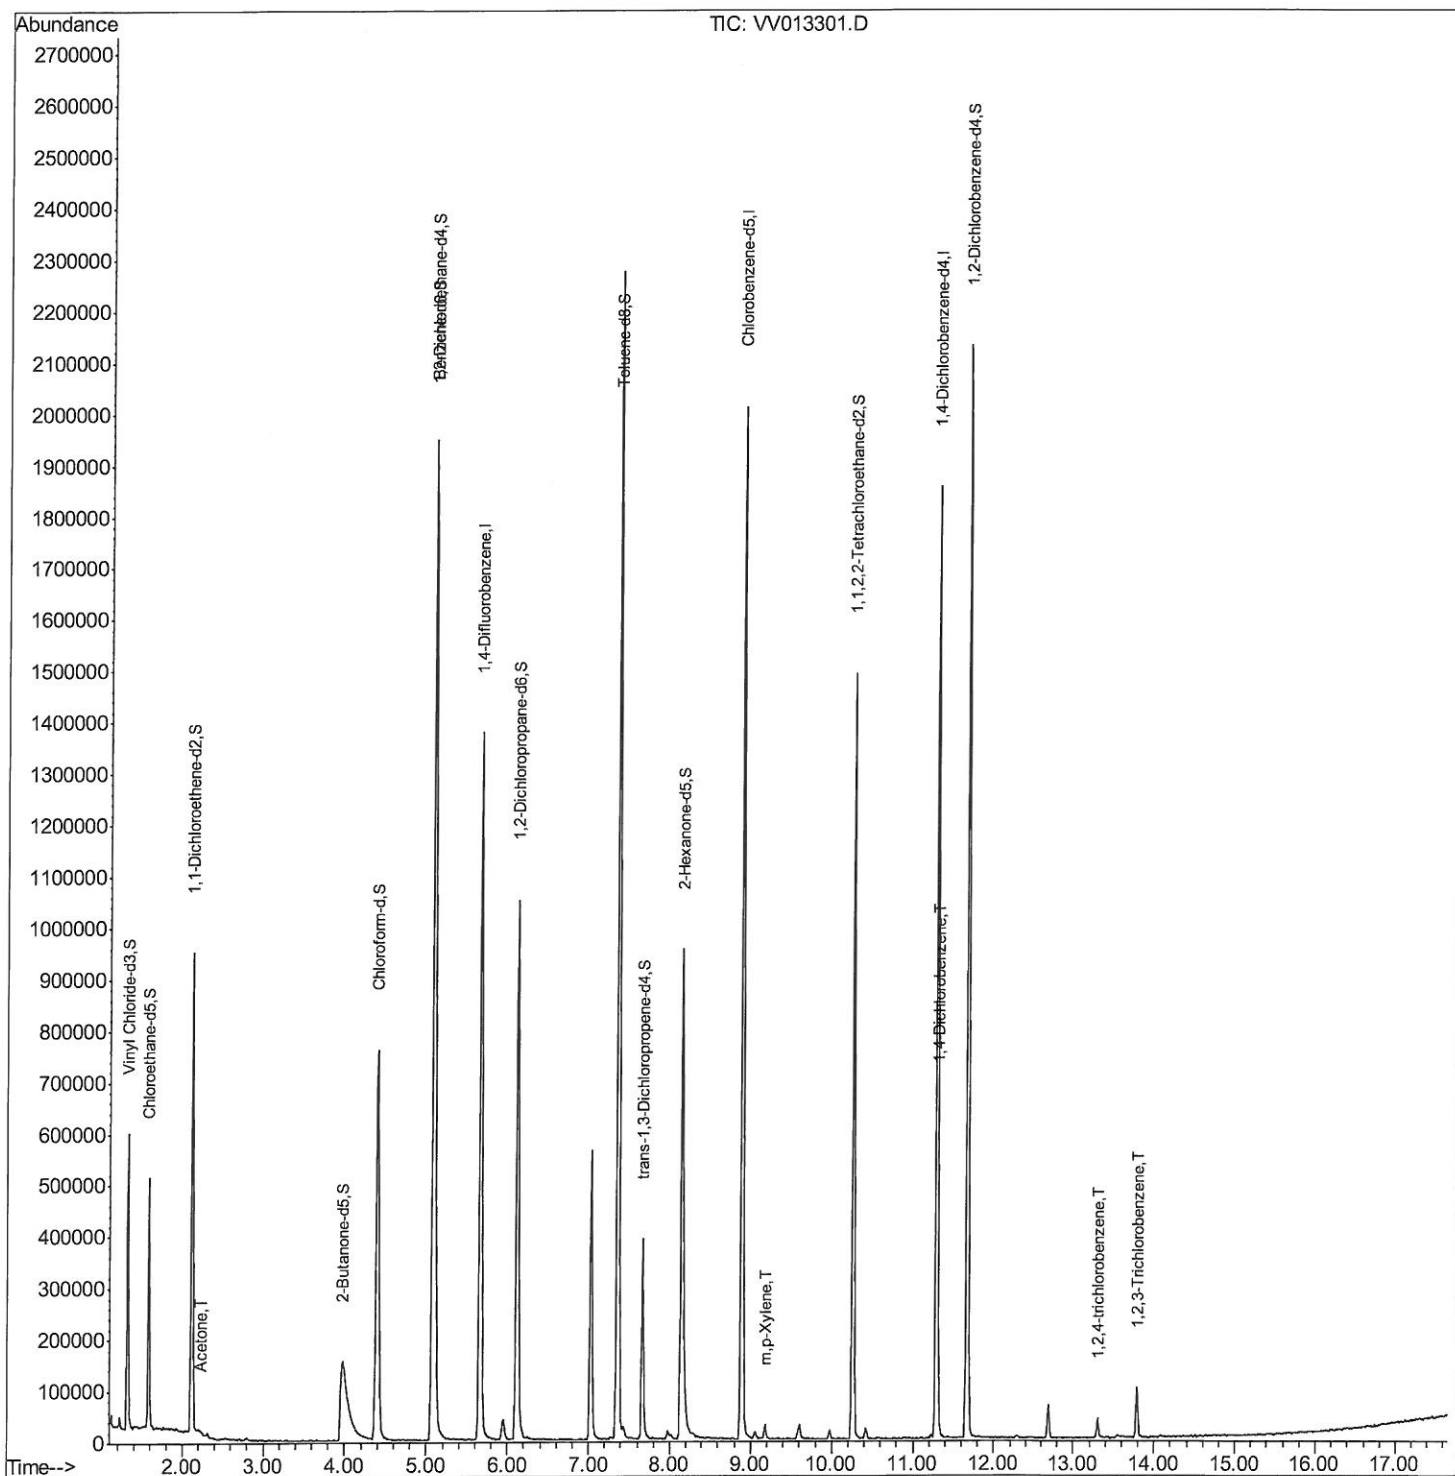

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102319\
Quantitation Report (Qedit)




Data File : VV013301.D
Acq On : 23 Oct 2019 14:58
Operator : SY/MD
Sample : K5395-04
Misc : 5.00ML/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0042

Manual Integrations
APPROVED

MMDadoda
10/24/2019 10:45:27 AM

Quant Time: Oct 24 03:08:50 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102319WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Oct 24 02:50:44 2019
Response via : Initial Calibration

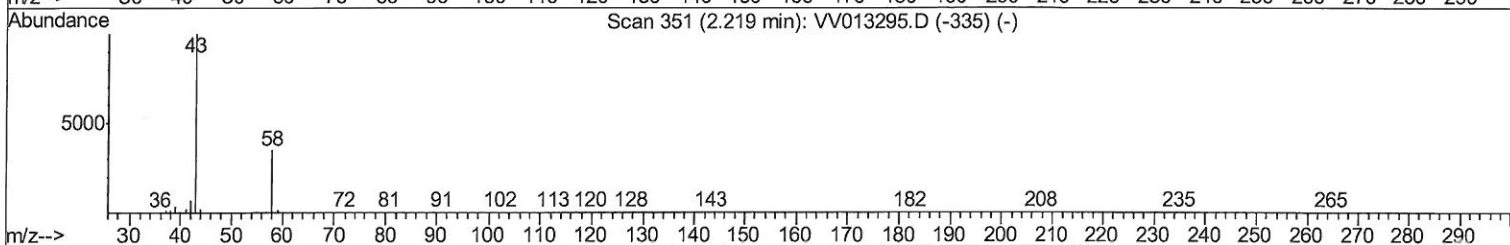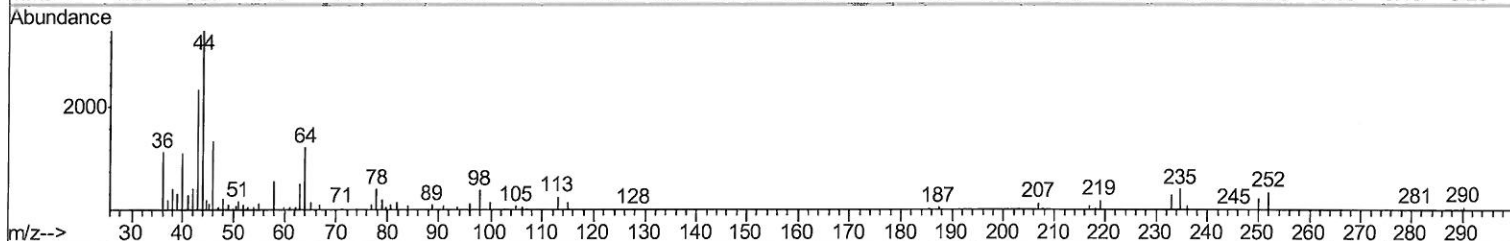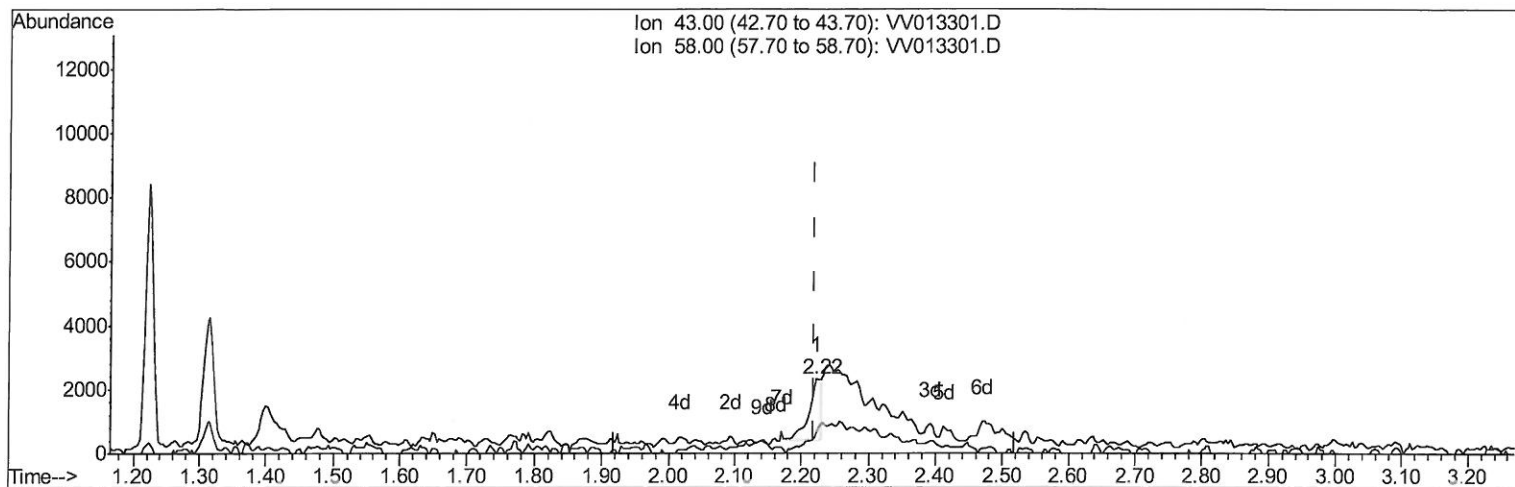

TIC: VV013301.D

(13) Acetone (T)

2.222min (+0.003) 0.60ug/L

response 2426

Ion	Exp%	Act%
43.00	100	100
58.00	32.00	22.92
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102319\
Quantitation Report (Qedit)




Data File : VV013301.D
Acq On : 23 Oct 2019 14:58
Operator : SY/MD
Sample : K5395-04
Misc : 5.00ML/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0042

Manual Integrations
APPROVED

MMDadoda
10/24/2019 10:45:27 AM

Quant Time: Oct 24 03:08:50 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102319WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Oct 24 02:50:44 2019
Response via : Initial Calibration

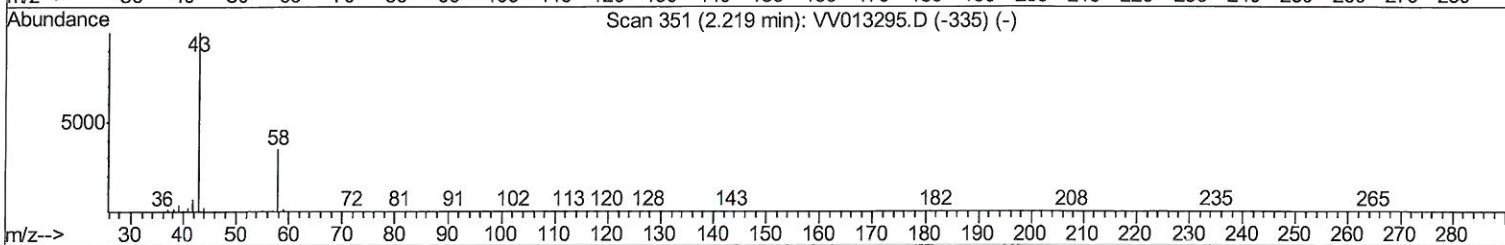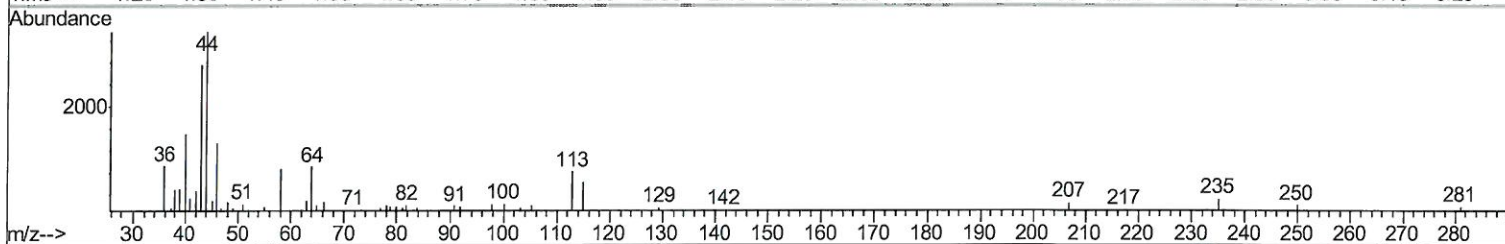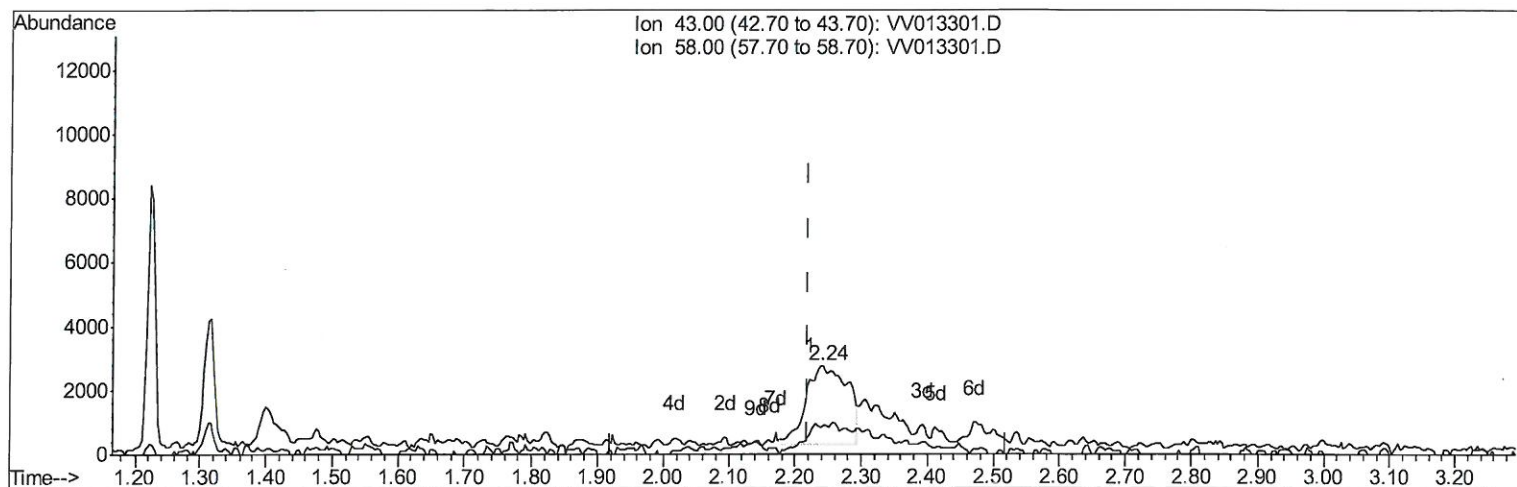

TIC: VV013301.D

(13) Acetone (T)

2.241min (+0.022) 2.60ug/L m

response 10580

Ion	Exp%	Act%
43.00	100	100
58.00	32.00	5.26
0.00	0.00	0.00
0.00	0.00	0.00

7 MD
10/26/19

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102319\
Quantitation Report (QT Reviewed)

Data File : VV013301.D
Acq On : 23 Oct 2019 14:58
Operator : SY/MD
Sample : K5395-04
Misc : 5.00ML/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0042

Manual Integrations
APPROVED

MMDadoda
10/24/2019 10:45:27 AM

Quant Time: Oct 24 03:59:28 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102319WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Oct 24 02:50:44 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Difluorobenzene	5.66	114	1238664	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	1158214	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	508891	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	372308	45.34	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	90.68%
7) Chloroethane-d5	1.58	69	300236	47.37	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	94.74%
11) 1,1-Dichloroethene-d2	2.12	63	450569	37.50	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	75.00%
21) 2-Butanone-d5	3.97	46	550892	100.13	ug/L	0.02
Spiked Amount	100.000	Range	40 - 130	Recovery	=	100.13%
24) Chloroform-d	4.40	84	800015	45.21	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	90.42%
26) 1,2-Dichloroethane-d4	5.08	65	506190	48.18	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.36%
32) Benzene-d6	5.10	84	1709896	47.95	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.90%
36) 1,2-Dichloropropane-d6	6.11	67	526094	47.64	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	95.28%
41) Toluene-d8	7.36	98	1512345	47.04	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	94.08%
43) trans-1,3-Dichloropropene-	7.66	79	227687	46.73	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	93.46%
47) 2-Hexanone-d5	8.13	63	318627	95.28	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	95.28%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	684380	46.89	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	93.78%
64) 1,2-Dichlorobenzene-d4	11.67	152	597441	51.16	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	102.32%

Target Compounds

					Qvalue
13) Acetone	2.24	43	10580m	2.602	ug/L
53) m,p-Xylene	9.18	106	8094	0.547	ug/L
63) 1,4-Dichlorobenzene	11.31	146	12077	0.708	ug/L
68) 1,2,4-trichlorobenzene	13.31	180	12418	1.196	ug/L
70) 1,2,3-Trichlorobenzene	13.79	180	32909	2.958	ug/L

MD
10/28/19

(#) = qualifier out of range (m) = manual integration (+) = signals summed