

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV102319\
Quantitation Report (QT Reviewed)


Data File : VV013309.D
Acq On : 23 Oct 2019 21:22
Operator : SY/MD
Sample : K5395-18
Misc : 5.00ML/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0051

Manual Integrations
APPROVED

MMDadoda
10/24/2019 10:46:09 AM

Quant Time: Oct 24 04:44:11 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102319WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Oct 24 04:17:57 2019
Response via : Initial Calibration

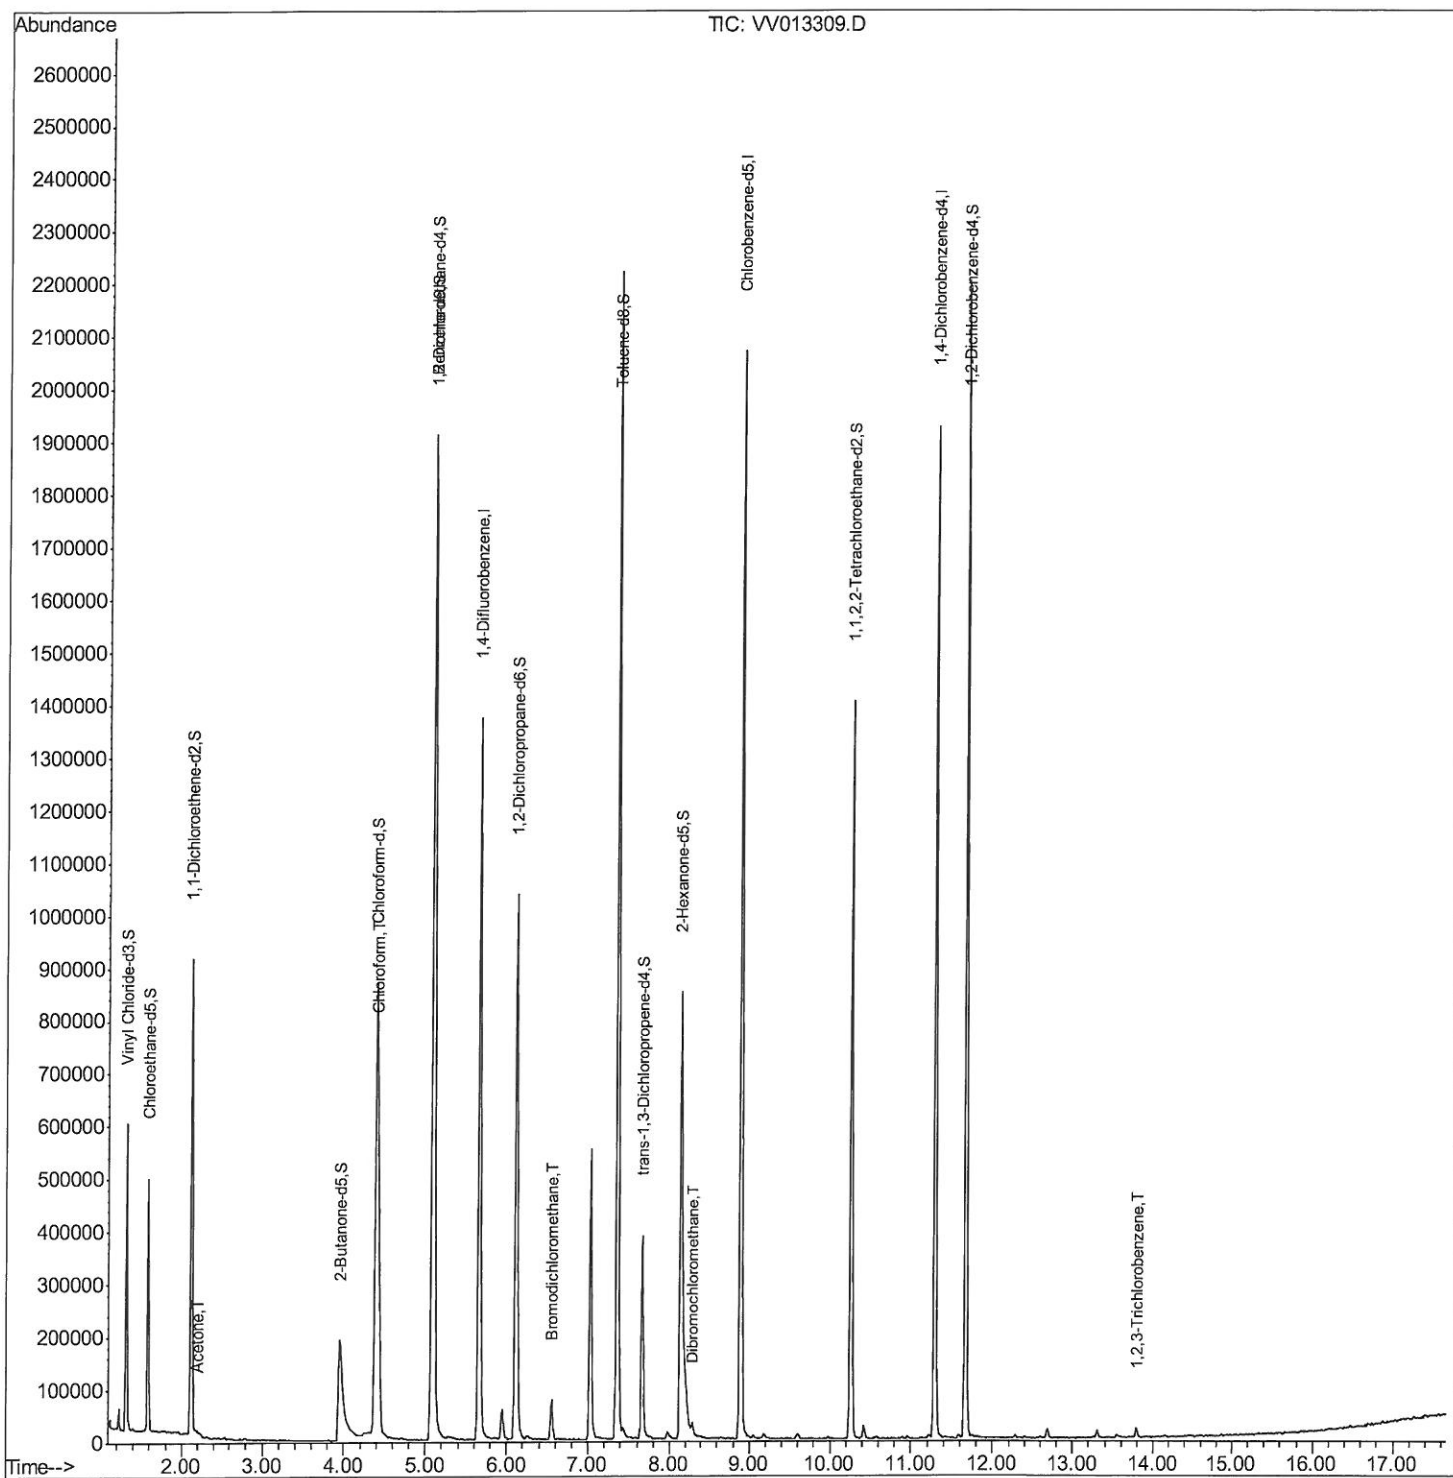

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV102319\
Quantitation Report (Qedit)




Data File : VV013309.D
Acq On : 23 Oct 2019 21:22
Operator : SY/MD
Sample : K5395-18
Misc : 5.00ML/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0051

Manual Integrations
APPROVED

MMDadoda
10/24/2019 10:46:09 AM

Quant Time: Oct 24 04:21:33 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102319WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Oct 24 04:17:57 2019
Response via : Initial Calibration

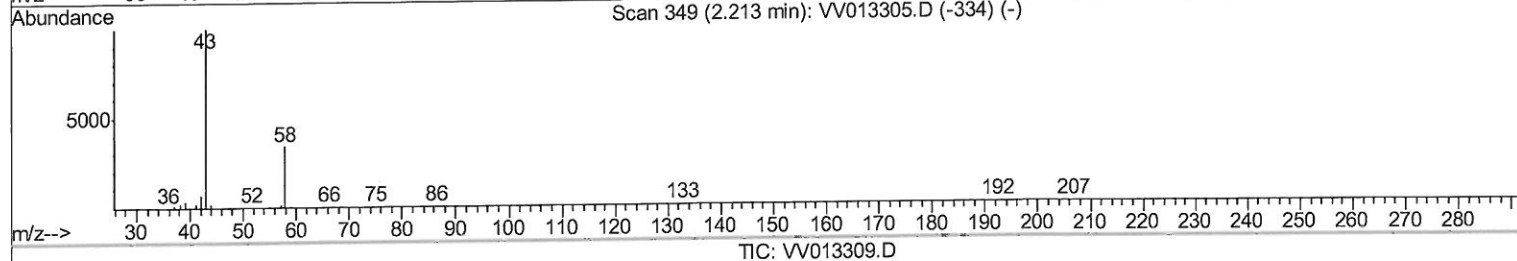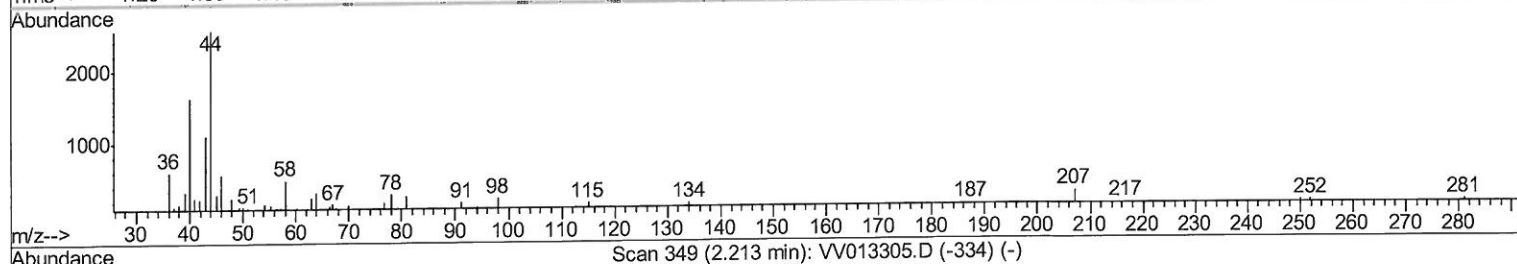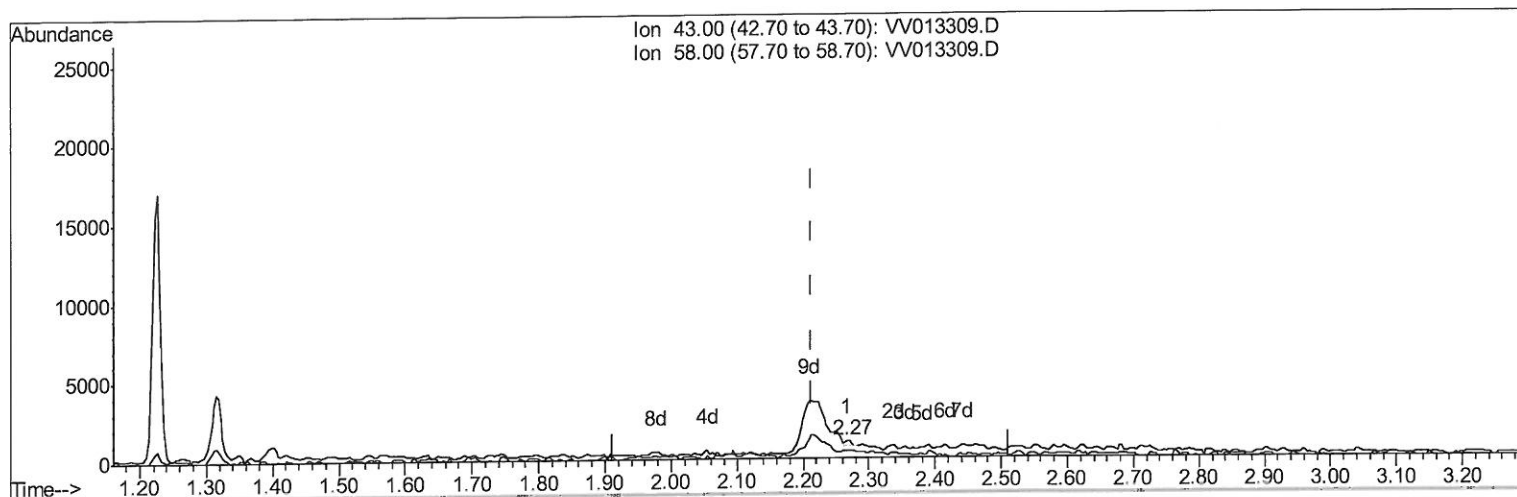

(13) Acetone (T)

2.267min (+0.055) 0.05ug/L

response 201

Ion	Exp%	Act%
43.00	100	100
58.00	32.00	13.43
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV102319\
Quantitation Report (Qedit)




Data File : VV013309.D
Acq On : 23 Oct 2019 21:22
Operator : SY/MD
Sample : K5395-18
Misc : 5.00ML/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0051

Manual Integrations
APPROVED

MMDadoda
10/24/2019 10:46:09 AM

Quant Time: Oct 24 04:21:33 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102319WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Oct 24 04:17:57 2019
Response via : Initial Calibration

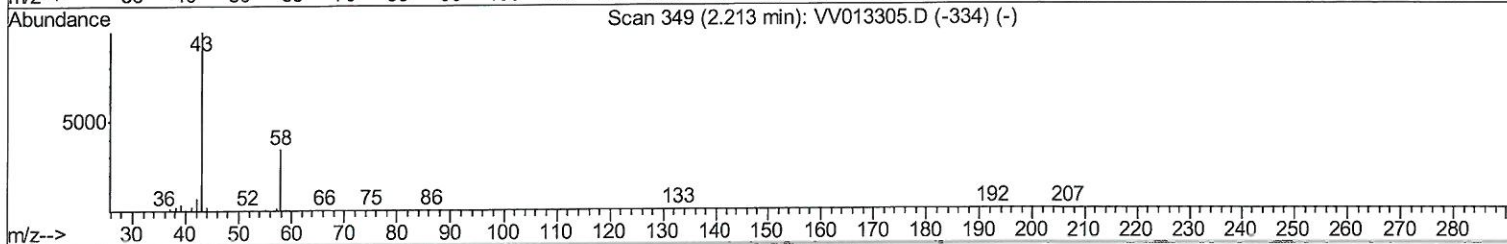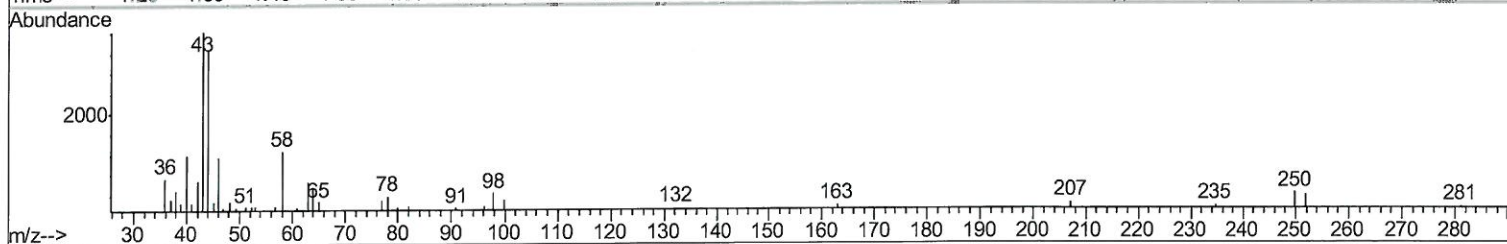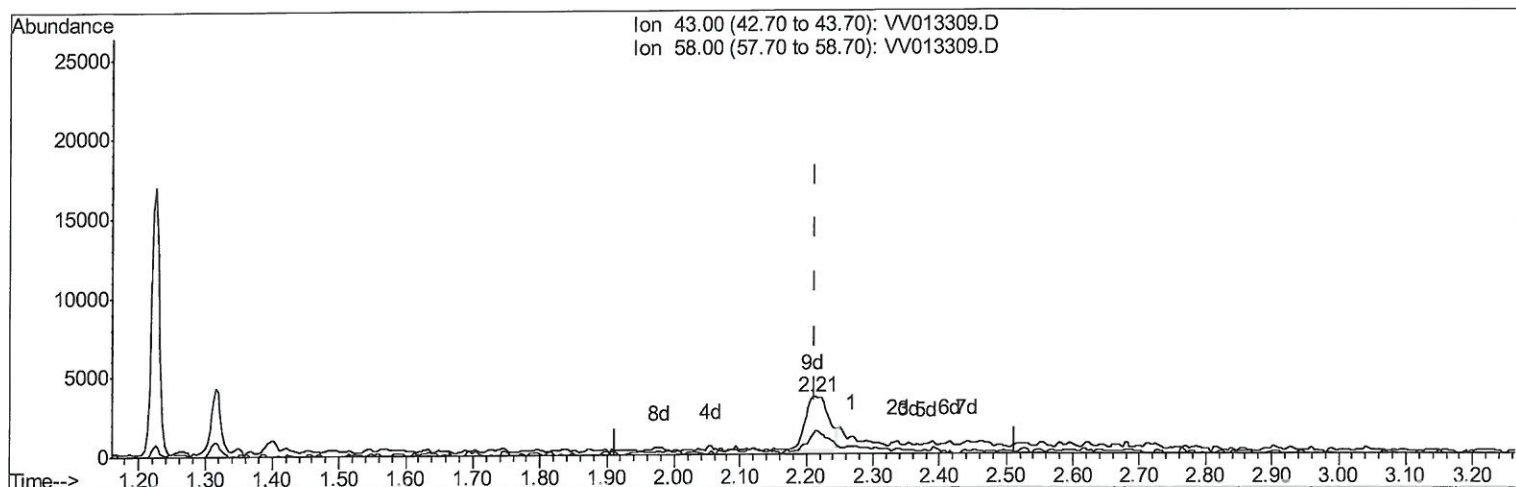

TIC: VV013309.D

(13) Acetone (T)

2.209min (-0.003) 2.06ug/L m

response 8283

Ion Exp% Act%

43.00 100 100

58.00 32.00 0.33

0.00 0.00 0.00

0.00 0.00 0.00

7MD
10/26/19

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV102319\
Quantitation Report (QT Reviewed)

Data File : VV013309.D
Acq On : 23 Oct 2019 21:22
Operator : SY/MD
Sample : K5395-18
Misc : 5.00ML/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0051

Manual Integrations
APPROVED

MMDadoda
10/24/2019 10:46:09 AM

Quant Time: Oct 24 04:44:11 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102319WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Oct 24 04:17:57 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Difluorobenzene	5.66	114	1227878	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	1193581	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	536852	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	364429	44.77	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	89.54%
7) Chloroethane-d5	1.58	69	303070	48.24	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	96.48%
11) 1,1-Dichloroethene-d2	2.13	63	447923	37.61	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	75.22%
21) 2-Butanone-d5	3.95	46	411514	75.46	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	75.46%
24) Chloroform-d	4.40	84	806755	45.99	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.98%
26) 1,2-Dichloroethane-d4	5.08	65	494790	47.51	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.02%
32) Benzene-d6	5.10	84	1676921	45.63	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.26%
36) 1,2-Dichloropropane-d6	6.12	67	520796	45.77	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	91.54%
41) Toluene-d8	7.36	98	1477650	44.60	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	89.20%
43) trans-1,3-Dichloropropene-	7.66	79	223996	44.61	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	89.22%
47) 2-Hexanone-d5	8.13	63	272541	79.08	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	79.08%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	669636	44.52	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	89.04%
64) 1,2-Dichlorobenzene-d4	11.67	152	622889	50.56	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	101.12%

Target Compounds

					Qvalue
13) Acetone	2.21	43	8283m	2.055	ug/L
25) Chloroform	4.42	83	326241	20.566	ug/L
38) Bromodichloromethane	6.55	83	52010	4.325	ug/L
49) Dibromochloromethane	8.29	129	9230	0.906	ug/L
70) 1,2,3-Trichlorobenzene	13.79	180	6289	0.536	ug/L

7 MB
10/26/19

(#) = qualifier out of range (m) = manual integration (+) = signals summed