

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102319\
 Data File : VV013306.D
 Acq On : 23 Oct 2019 20:12
 Operator : SY/MD
 Sample : VV1023WBL02
 Misc : 5.00ML/MSVOA V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK64

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102319WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	89	rVB	595337	619226	12.55%	1.680%
2	1.582	146	153	164	rVB	504613	552338	11.19%	1.498%
3	2.129	313	323	349	rVB	994465	1406347	28.50%	3.814%
4	2.425	411	415	417	rBV5	1611	1306	0.03%	0.004%
5	2.537	441	450	463	rBB6	7426	13166	0.27%	0.036%
6	2.605	468	471	476	rBV6	1316	1189	0.02%	0.003%
7	2.650	482	485	488	rBV5	1294	936	0.02%	0.003%
8	2.775	518	524	525	rBV5	1974	2082	0.04%	0.006%
9	2.843	542	545	548	rBV5	1775	1265	0.03%	0.003%
10	2.945	574	577	583	rVB8	1978	1748	0.04%	0.005%
11	2.984	583	589	591	rBV5	1921	1830	0.04%	0.005%
12	3.032	602	604	610	rVB6	1429	1128	0.02%	0.003%
13	3.135	633	636	641	rBV6	2060	2182	0.04%	0.006%
14	3.299	682	687	688	rBV4	1484	967	0.02%	0.003%
15	3.315	688	692	695	rVV5	1305	1340	0.03%	0.004%
16	3.376	707	711	717	rVB6	1575	1419	0.03%	0.004%
17	3.421	717	725	727	rBV8	1686	1649	0.03%	0.004%
18	3.498	745	749	752	rBV4	1699	1294	0.03%	0.004%
19	3.515	752	754	761	rVB6	1899	1523	0.03%	0.004%
20	3.634	789	791	793	rBV2	1940	964	0.02%	0.003%
21	3.646	793	795	798	rVV2	1780	1056	0.02%	0.003%
22	3.724	815	819	823	rVV6	1740	1882	0.04%	0.005%
23	3.814	845	847	853	rVB6	1118	989	0.02%	0.003%
24	3.949	877	889	930	rBV2	215225	838751	17.00%	2.275%
25	4.399	1014	1029	1055	rVB	792430	1897876	38.46%	5.148%
26	4.814	1154	1158	1161	rBV4	2014	1278	0.03%	0.003%
27	4.900	1183	1185	1191	rVB6	2764	2102	0.04%	0.006%
28	5.093	1226	1245	1275	rBV2	1961052	4934634	100.00%	13.384%
29	5.434	1346	1351	1354	rBV7	2107	2041	0.04%	0.006%
30	5.521	1375	1378	1380	rBV4	1178	927	0.02%	0.003%
31	5.550	1385	1387	1392	rVB4	1818	1157	0.02%	0.003%
32	5.662	1402	1422	1448	rBV	1481605	2927990	59.34%	7.942%
33	5.945	1499	1510	1526	rVB4	47217	101247	2.05%	0.275%
34	6.019	1530	1533	1539	rVB7	3436	2912	0.06%	0.008%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102319\
 Data File : VV013306.D
 Acq On : 23 Oct 2019 20:12
 Operator : SY/MD
 Sample : VV1023WBL02
 Misc : 5.00ML/MSVOA V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK64

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102319WMA.M
 Title : VOC Analysis

35	6.058	1541	1545	1548	rBV4	2102	1716	0.03%	0.005%
36	6.116	1548	1563	1594	rBV	1091931	2227216	45.13%	6.041%
37	6.373	1641	1643	1647	rVB5	2017	1435	0.03%	0.004%
38	6.559	1696	1701	1705	rVB7	2656	2594	0.05%	0.007%
39	6.617	1715	1719	1720	rBV4	1568	972	0.02%	0.003%
40	6.662	1730	1733	1735	rVV4	1793	1210	0.02%	0.003%
41	6.727	1748	1753	1756	rVB5	1538	1137	0.02%	0.003%
42	6.868	1794	1797	1799	rBV3	1479	1091	0.02%	0.003%
43	7.026	1833	1846	1870	rBV	590942	1059274	21.47%	2.873%
44	7.170	1889	1891	1894	rBV4	1562	1194	0.02%	0.003%
45	7.357	1934	1949	1969	rBV	2355390	3990231	80.86%	10.823%
46	7.662	2033	2044	2061	rVV	405665	690603	14.00%	1.873%
47	8.013	2146	2153	2160	rVB	6749	10165	0.21%	0.028%
48	8.067	2165	2170	2174	rBV6	1255	1260	0.03%	0.003%
49	8.090	2174	2177	2179	rBV4	1562	1055	0.02%	0.003%
50	8.135	2179	2191	2253	rBV3	902577	2348239	47.59%	6.369%
51	8.450	2285	2289	2295	rBV8	2173	2548	0.05%	0.007%
52	8.527	2311	2313	2317	rVB4	2210	992	0.02%	0.003%
53	8.791	2392	2395	2399	rVV4	1301	1065	0.02%	0.003%
54	8.891	2413	2426	2455	rVV	2217849	3608250	73.12%	9.787%
55	9.055	2469	2477	2485	rVB8	6605	10202	0.21%	0.028%
56	9.180	2510	2516	2526	rVB3	8894	12417	0.25%	0.034%
57	9.460	2598	2603	2606	rVV7	1167	1180	0.02%	0.003%
58	9.521	2620	2622	2629	rVB8	1520	1364	0.03%	0.004%
59	9.601	2636	2647	2659	rVB9	8615	19241	0.39%	0.052%
60	9.672	2665	2669	2673	rBV6	1759	1520	0.03%	0.004%
61	9.694	2673	2676	2678	rVV4	1609	1040	0.02%	0.003%
62	9.884	2733	2735	2739	rVB4	1600	1000	0.02%	0.003%
63	9.971	2753	2762	2770	rBV7	5955	9417	0.19%	0.026%
64	10.257	2838	2851	2871	rBV	1445555	2340898	47.44%	6.349%
65	10.530	2933	2936	2938	rBV3	1616	1026	0.02%	0.003%
66	10.579	2945	2951	2960	rVV7	5585	8538	0.17%	0.023%
67	10.665	2975	2978	2981	rVB3	1401	958	0.02%	0.003%
68	10.768	3006	3010	3012	rBV4	1523	1226	0.02%	0.003%
69	10.797	3015	3019	3023	rBV6	1206	1293	0.03%	0.004%
70	10.820	3023	3026	3030	rBV5	1369	1070	0.02%	0.003%
71	10.894	3043	3049	3050	rBV5	2846	2622	0.05%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102319\
 Data File : VV013306.D
 Acq On : 23 Oct 2019 20:12
 Operator : SY/MD
 Sample : VV1023WBL02
 Misc : 5.00ML/MSVOA V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK64

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102319WMA.M
 Title : VOC Analysis

72	10.932	3057	3061	3063	rBV3	1278	1027	0.02%	0.003%
73	10.952	3063	3067	3068	rBV3	4985	3076	0.06%	0.008%
74	11.222	3140	3151	3160	rBV5	10970	21178	0.43%	0.057%
75	11.289	3160	3172	3193	rBV	2124311	3267603	66.22%	8.863%
76	11.572	3257	3260	3264	rBV5	2335	1840	0.04%	0.005%
77	11.665	3276	3289	3310	rBV	2369408	3691463	74.81%	10.012%
78	11.984	3384	3388	3394	rVV7	2434	2215	0.04%	0.006%
79	12.083	3415	3419	3421	rBV3	2013	1438	0.03%	0.004%
80	12.141	3433	3437	3439	rBV4	2129	1896	0.04%	0.005%
81	12.164	3440	3444	3447	rVB4	2185	2102	0.04%	0.006%
82	12.186	3447	3451	3454	rBV4	1771	1512	0.03%	0.004%
83	12.289	3477	3483	3485	rBV6	2046	2147	0.04%	0.006%
84	12.347	3499	3501	3505	rVV3	1957	1239	0.03%	0.003%
85	12.431	3523	3527	3528	rBV4	1371	953	0.02%	0.003%
86	12.472	3536	3540	3547	rVV8	2487	3174	0.06%	0.009%
87	12.501	3547	3549	3551	rVB2	2227	1091	0.02%	0.003%
88	12.530	3556	3558	3565	rVB8	2163	1779	0.04%	0.005%
89	12.591	3574	3577	3582	rVV5	2158	2052	0.04%	0.006%
90	12.617	3582	3585	3589	rVB4	1574	1335	0.03%	0.004%
91	12.691	3598	3608	3620	rBV3	24227	42615	0.86%	0.116%
92	12.929	3679	3682	3685	rBV5	2068	1639	0.03%	0.004%
93	13.263	3784	3786	3789	rVB4	1867	1070	0.02%	0.003%
94	13.308	3789	3800	3812	rBV3	23421	44329	0.90%	0.120%
95	13.553	3869	3876	3886	rBV	10227	17478	0.35%	0.047%
96	13.694	3918	3920	3923	rBV3	1926	1111	0.02%	0.003%
97	13.714	3923	3926	3929	rVB4	2071	1430	0.03%	0.004%
98	13.791	3939	3950	3962	rBV3	28250	51418	1.04%	0.139%
99	14.312	4109	4112	4115	rBV4	2297	1588	0.03%	0.004%
100	14.948	4308	4310	4312	rBV3	2838	1583	0.03%	0.004%


Sum of corrected areas: 36869381

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV102319\
Data File : VV013306.D
Acq On : 23 Oct 2019 20:12
Operator : SY/MD
Sample : VV1023WBL02
Misc : 5.00ML/MSVOA V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK64

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

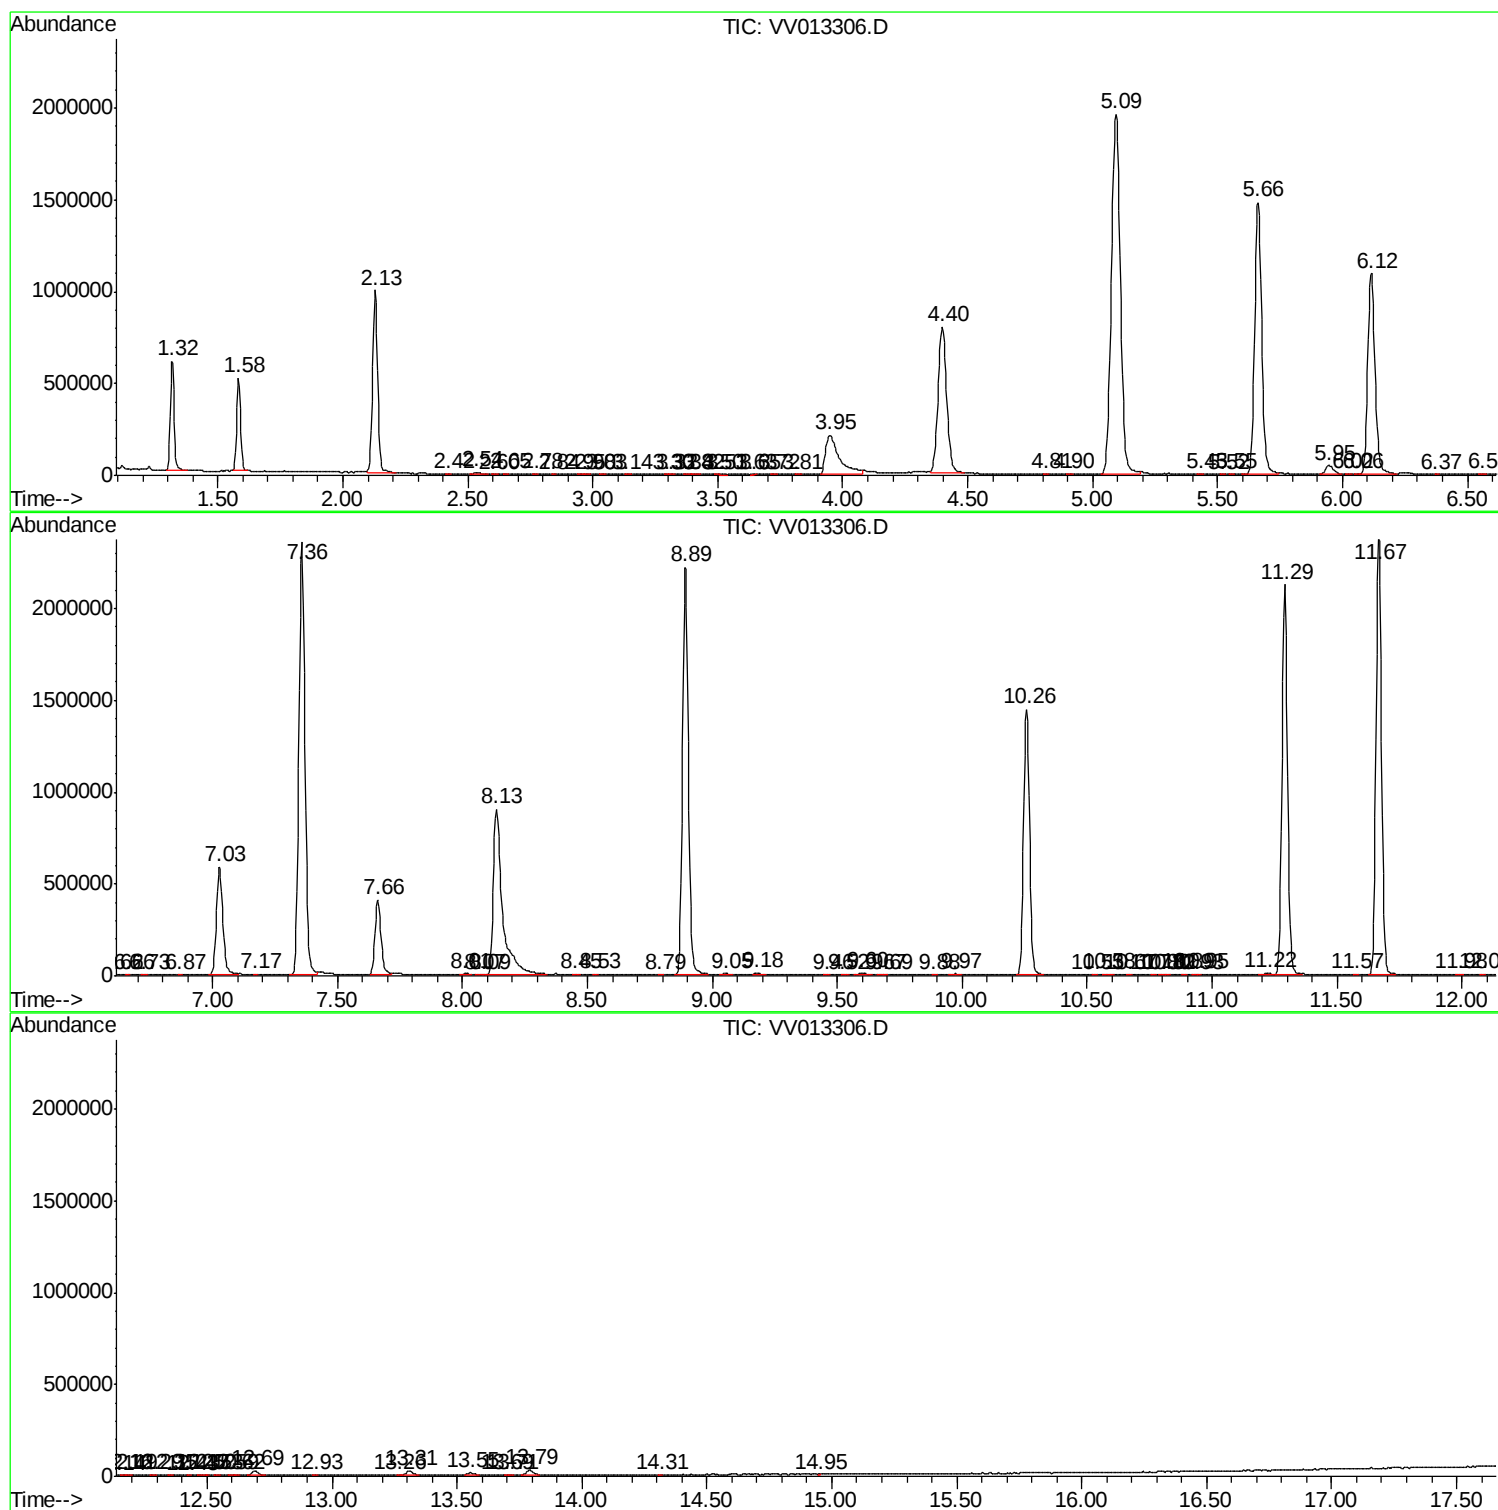

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV102319\
Data File : VV013306.D
Acq On : 23 Oct 2019 20:12
Operator : SY/MD
Sample : VV1023WBL02
Misc : 5.00ML/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK64

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV102319\
Data File : VV013306.D
Acq On : 23 Oct 2019 20:12
Operator : SY/MD
Sample : VV1023WBL02
Misc : 5.00ML/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK64

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc