

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102319\
 Data File : VV013308.D
 Acq On : 23 Oct 2019 20:59
 Operator : SY/MD
 Sample : K5395-17
 Misc : 5.00ML/MSVOA V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0050

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102319WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.225	37	42	47	rVB	92992	75457	1.56%	0.207%
2	1.315	63	70	84	rVB	574660	587500	12.17%	1.613%
3	1.582	146	153	164	rVB	490740	540897	11.21%	1.485%
4	2.129	312	323	335	rBV	947264	1332344	27.60%	3.658%
5	2.653	481	486	491	rBV8	3012	3679	0.08%	0.010%
6	2.714	502	505	507	rVB2	2060	1055	0.02%	0.003%
7	2.727	507	509	516	rVB8	1936	1578	0.03%	0.004%
8	2.917	563	568	569	rBV3	1410	1161	0.02%	0.003%
9	3.032	600	604	605	rBV2	1706	1291	0.03%	0.004%
10	3.077	614	618	620	rBV3	1368	1083	0.02%	0.003%
11	3.167	643	646	650	rBV4	1869	1426	0.03%	0.004%
12	3.460	731	737	740	rBV6	1606	1786	0.04%	0.005%
13	3.524	751	757	761	rVB7	2160	2211	0.05%	0.006%
14	3.547	761	764	769	rVB6	1767	1413	0.03%	0.004%
15	3.878	862	867	870	rBV7	1589	1293	0.03%	0.004%
16	3.952	877	890	940	rBV	205639	873545	18.10%	2.399%
17	4.402	1014	1030	1069	rVB3	881220	2799009	57.99%	7.686%
18	4.717	1123	1128	1129	rBV4	2847	2443	0.05%	0.007%
19	4.820	1158	1160	1165	rVB4	1890	1559	0.03%	0.004%
20	4.842	1165	1167	1169	rBV3	2043	1071	0.02%	0.003%
21	4.904	1184	1186	1189	rBV3	1951	1102	0.02%	0.003%
22	5.029	1219	1225	1226	rBV5	1826	1254	0.03%	0.003%
23	5.093	1226	1245	1289	rBV2	1942763	4826852	100.00%	13.254%
24	5.437	1349	1352	1354	rVV3	1650	992	0.02%	0.003%
25	5.505	1369	1373	1377	rBV5	1661	1626	0.03%	0.004%
26	5.543	1382	1385	1388	rBV4	1524	975	0.02%	0.003%
27	5.662	1405	1422	1451	rBV	1356432	2712859	56.20%	7.449%
28	5.910	1496	1499	1500	rBV3	1747	1031	0.02%	0.003%
29	5.945	1500	1510	1525	rVV	60134	120937	2.51%	0.332%
30	6.116	1548	1563	1594	rVV	1067273	2171582	44.99%	5.963%
31	6.325	1625	1628	1630	rVB4	1816	1012	0.02%	0.003%
32	6.344	1630	1634	1637	rBV5	1794	1548	0.03%	0.004%
33	6.402	1650	1652	1655	rVB5	1958	947	0.02%	0.003%
34	6.553	1686	1699	1720	rVV	83519	161535	3.35%	0.444%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102319\
 Data File : VV013308.D
 Acq On : 23 Oct 2019 20:59
 Operator : SY/MD
 Sample : K5395-17
 Misc : 5.00ML/MSVOA V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0050

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102319WMA.M
 Title : VOC Analysis

35	6.672	1732	1736	1738	rBV5	1777	1250	0.03%	0.003%
36	6.791	1770	1773	1775	rBV3	1392	960	0.02%	0.003%
37	6.903	1803	1808	1810	rBV4	1114	1210	0.03%	0.003%
38	6.920	1810	1813	1818	rVB7	2022	1512	0.03%	0.004%
39	7.029	1834	1847	1869	rBV	561701	1016382	21.06%	2.791%
40	7.270	1918	1922	1923	rBV3	2147	1547	0.03%	0.004%
41	7.357	1935	1949	1968	rBV	2258023	3857238	79.91%	10.591%
42	7.662	2032	2044	2062	rBV	392142	675725	14.00%	1.855%
43	7.936	2126	2129	2133	rBV6	1739	1464	0.03%	0.004%
44	7.974	2135	2141	2149	rVV3	5904	9610	0.20%	0.026%
45	8.083	2170	2175	2178	rBV5	2396	1637	0.03%	0.004%
46	8.138	2179	2192	2231	rBV4	889275	2269211	47.01%	6.231%
47	8.579	2326	2329	2332	rBV4	1587	1083	0.02%	0.003%
48	8.710	2366	2370	2374	rBV6	1481	1080	0.02%	0.003%
49	8.739	2376	2379	2383	rVB4	1560	1155	0.02%	0.003%
50	8.768	2383	2388	2389	rBV4	1745	1153	0.02%	0.003%
51	8.781	2389	2392	2396	rVB5	1696	1238	0.03%	0.003%
52	8.894	2413	2427	2455	rBV	2057602	3334494	69.08%	9.156%
53	9.093	2486	2489	2494	rBV6	1910	2023	0.04%	0.006%
54	9.138	2499	2503	2507	rVV6	2185	2277	0.05%	0.006%
55	9.183	2508	2517	2526	rVB3	11874	19947	0.41%	0.055%
56	9.222	2527	2529	2532	rVB4	2338	1353	0.03%	0.004%
57	9.254	2532	2539	2541	rBV8	2098	2579	0.05%	0.007%
58	9.382	2575	2579	2581	rVB4	2020	1333	0.03%	0.004%
59	9.399	2581	2584	2590	rBV6	1523	1715	0.04%	0.005%
60	9.550	2628	2631	2633	rBV3	2568	1486	0.03%	0.004%
61	9.595	2636	2645	2646	rBV4	9485	10894	0.23%	0.030%
62	9.665	2664	2667	2672	rVV5	1974	1574	0.03%	0.004%
63	9.781	2700	2703	2708	rVV5	1935	1504	0.03%	0.004%
64	9.881	2730	2734	2740	rVB8	1598	1676	0.03%	0.005%
65	9.974	2757	2763	2765	rVV6	3987	3829	0.08%	0.011%
66	10.045	2781	2785	2787	rBV3	1600	1430	0.03%	0.004%
67	10.138	2812	2814	2818	rVB4	1650	1033	0.02%	0.003%
68	10.257	2837	2851	2871	rBV	1423483	2268767	47.00%	6.230%
69	10.418	2892	2901	2912	rVB3	14261	22973	0.48%	0.063%
70	10.566	2944	2947	2948	rBV3	2362	1263	0.03%	0.003%
71	10.714	2989	2993	2996	rVB4	1444	1316	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102319\
 Data File : VV013308.D
 Acq On : 23 Oct 2019 20:59
 Operator : SY/MD
 Sample : K5395-17
 Misc : 5.00ML/MSVOA V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0050

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102319WMA.M
 Title : VOC Analysis

72	10.736	2996	3000	3001	rBV4	1813	1105	0.02%	0.003%
73	10.820	3020	3026	3027	rBV3	1747	1799	0.04%	0.005%
74	10.868	3038	3041	3044	rBV4	1231	1015	0.02%	0.003%
75	10.894	3044	3049	3052	rBV6	2224	1828	0.04%	0.005%
76	10.955	3064	3068	3071	rVV4	3159	2912	0.06%	0.008%
77	11.225	3141	3152	3160	rBV10	8625	15106	0.31%	0.041%
78	11.289	3160	3172	3192	rBV	1912555	2954302	61.21%	8.112%
79	11.591	3263	3266	3268	rVV3	1709	1142	0.02%	0.003%
80	11.669	3277	3290	3317	rVV	2213609	3531727	73.17%	9.697%
81	11.865	3348	3351	3356	rVB6	1594	1315	0.03%	0.004%
82	12.006	3393	3395	3398	rBV4	1311	1020	0.02%	0.003%
83	12.064	3410	3413	3416	rBV6	1496	1242	0.03%	0.003%
84	12.215	3456	3460	3461	rBV3	1544	1176	0.02%	0.003%
85	12.283	3478	3481	3483	rBV4	2769	1893	0.04%	0.005%
86	12.508	3546	3551	3553	rBV4	1466	1176	0.02%	0.003%
87	12.627	3586	3588	3596	rVB8	1920	1198	0.02%	0.003%
88	12.691	3598	3608	3619	rBV4	20803	36965	0.77%	0.101%
89	12.781	3632	3636	3640	rBV7	2293	1988	0.04%	0.005%
90	12.900	3670	3673	3678	rBV7	2236	1711	0.04%	0.005%
91	12.923	3678	3680	3682	rBV3	2102	1096	0.02%	0.003%
92	13.086	3728	3731	3734	rVB4	1740	1428	0.03%	0.004%
93	13.115	3738	3740	3743	rVB3	1739	1144	0.02%	0.003%
94	13.228	3772	3775	3780	rVB7	2648	2151	0.04%	0.006%
95	13.254	3780	3783	3786	rBV5	2006	1473	0.03%	0.004%
96	13.308	3791	3800	3808	rBV5	17323	29222	0.61%	0.080%
97	13.376	3819	3821	3825	rBV4	1720	1172	0.02%	0.003%
98	13.559	3870	3878	3891	rBV5	8160	14920	0.31%	0.041%
99	13.791	3941	3950	3961	rVB3	23769	41333	0.86%	0.113%
100	14.906	4295	4297	4299	rBV4	2777	1454	0.03%	0.004%


Sum of corrected areas: 36418987

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV102319\
Data File : VV013308.D
Acq On : 23 Oct 2019 20:59
Operator : SY/MD
Sample : K5395-17
Misc : 5.00ML/MSVOA V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0050

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

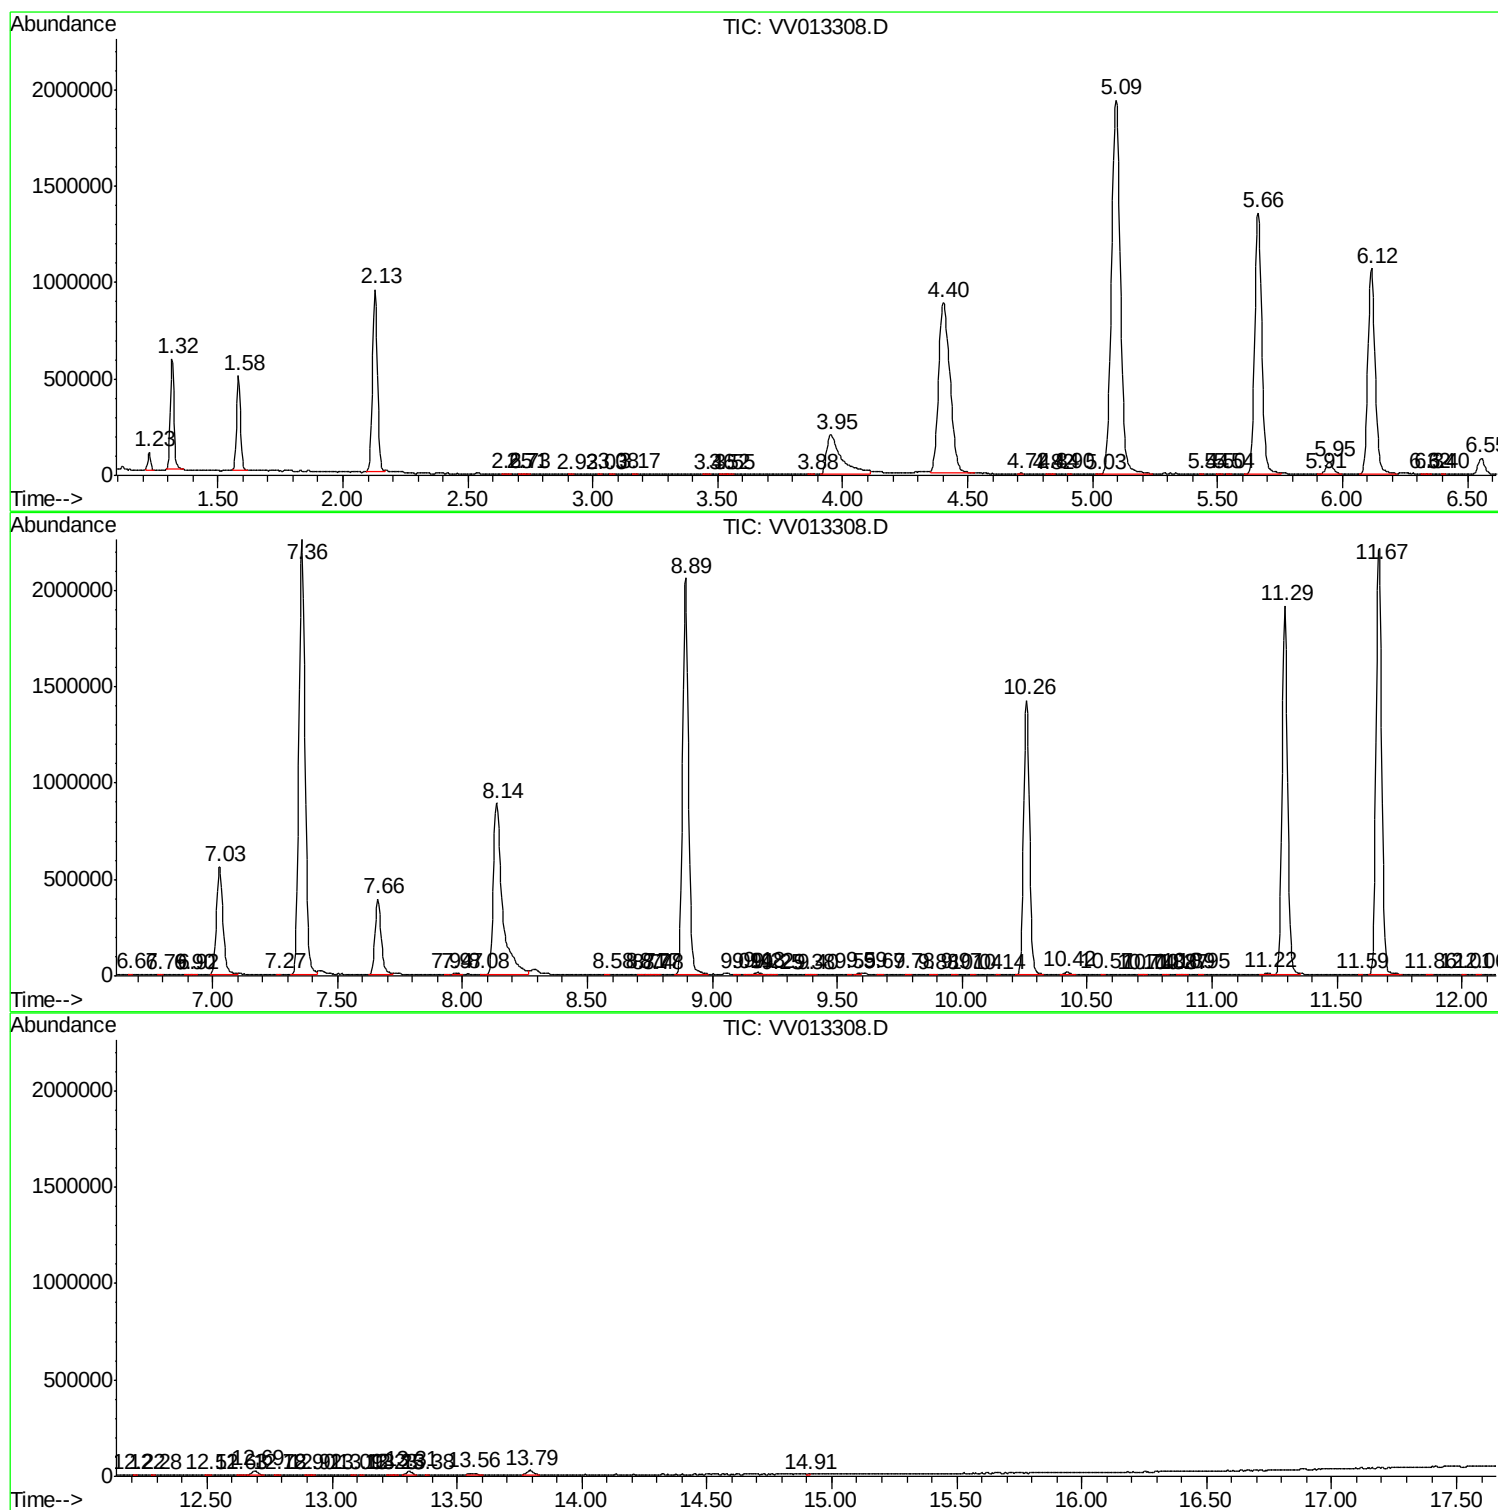

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV102319\
Data File : VV013308.D
Acq On : 23 Oct 2019 20:59
Operator : SY/MD
Sample : K5395-17
Misc : 5.00ML/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0050

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV102319\
Data File : VV013308.D
Acq On : 23 Oct 2019 20:59
Operator : SY/MD
Sample : K5395-17
Misc : 5.00ML/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0050

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc