

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102319\
 Data File : VV013309.D
 Acq On : 23 Oct 2019 21:22
 Operator : SY/MD
 Sample : K5395-18
 Misc : 5.00ML/MSVOA V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0051

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102319WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.226	38	42	52	rVB2	40595	36083	0.76%	0.101%
2	1.316	63	70	84	rBV	579997	584526	12.31%	1.640%
3	1.582	145	153	164	rBV	478627	527533	11.11%	1.480%
4	2.126	313	322	336	rBV	895271	1261126	26.56%	3.539%
5	2.933	571	573	576	rBV3	1468	972	0.02%	0.003%
6	2.997	588	593	598	rBV7	1667	1930	0.04%	0.005%
7	3.065	609	614	616	rBV5	1553	1400	0.03%	0.004%
8	3.264	672	676	678	rBV3	1283	908	0.02%	0.003%
9	3.450	728	734	738	rBV7	1560	1472	0.03%	0.004%
10	3.486	743	745	751	rVB7	1287	1014	0.02%	0.003%
11	3.518	753	755	760	rVB4	1663	1154	0.02%	0.003%
12	3.602	777	781	785	rBV6	1123	1078	0.02%	0.003%
13	3.717	813	817	821	rBV6	1333	970	0.02%	0.003%
14	3.791	837	840	845	rVV6	1419	1435	0.03%	0.004%
15	3.817	845	848	852	rVB3	2244	1750	0.04%	0.005%
16	3.865	860	863	866	rBV4	1399	867	0.02%	0.002%
17	3.885	866	869	873	rBV5	1458	1187	0.02%	0.003%
18	3.952	878	890	917	rBV2	189711	701300	14.77%	1.968%
19	4.402	1014	1030	1062	rVB2	857242	2598810	54.73%	7.293%
20	4.663	1108	1111	1115	rBV6	2429	1728	0.04%	0.005%
21	4.868	1173	1175	1180	rVB5	1448	1202	0.03%	0.003%
22	5.020	1219	1222	1225	rVB3	1709	1203	0.03%	0.003%
23	5.094	1225	1245	1287	rBV2	1910615	4748573	100.00%	13.327%
24	5.434	1348	1351	1354	rBV4	1719	1354	0.03%	0.004%
25	5.505	1369	1373	1378	rVV7	1851	1570	0.03%	0.004%
26	5.576	1392	1395	1398	rVB5	1989	1388	0.03%	0.004%
27	5.663	1405	1422	1450	rBV	1370567	2725881	57.40%	7.650%
28	5.946	1500	1510	1528	rVB2	55932	111994	2.36%	0.314%
29	6.116	1548	1563	1596	rVV	1034672	2125863	44.77%	5.966%
30	6.229	1596	1598	1600	rBV3	2863	1950	0.04%	0.005%
31	6.396	1645	1650	1657	rVB8	1744	2195	0.05%	0.006%
32	6.428	1657	1660	1664	rBV4	1871	1245	0.03%	0.003%
33	6.489	1677	1679	1684	rVB6	1394	1163	0.02%	0.003%
34	6.553	1686	1699	1717	rBV2	76457	145562	3.07%	0.409%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102319\
 Data File : VV013309.D
 Acq On : 23 Oct 2019 21:22
 Operator : SY/MD
 Sample : K5395-18
 Misc : 5.00ML/MSVOA V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0051

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102319WMA.M
 Title : VOC Analysis

35	6.621	1717	1720	1722	rBV3	1711	962	0.02%	0.003%
36	6.679	1734	1738	1741	rBV5	1854	1331	0.03%	0.004%
37	6.695	1741	1743	1748	rVB4	1432	941	0.02%	0.003%
38	6.827	1781	1784	1788	rVV5	2147	1402	0.03%	0.004%
39	6.894	1802	1805	1807	rBV3	2015	1255	0.03%	0.004%
40	7.026	1833	1846	1871	rBV	552092	1003728	21.14%	2.817%
41	7.357	1935	1949	1967	rBV	2217544	3785027	79.71%	10.623%
42	7.663	2033	2044	2065	rBV	384900	666567	14.04%	1.871%
43	7.978	2130	2142	2151	rBV3	12457	26645	0.56%	0.075%
44	8.135	2179	2191	2232	rBV3	848882	2233767	47.04%	6.269%
45	8.730	2373	2376	2377	rBV2	1732	971	0.02%	0.003%
46	8.801	2395	2398	2401	rVB4	1319	858	0.02%	0.002%
47	8.830	2405	2407	2411	rVB5	1558	941	0.02%	0.003%
48	8.891	2411	2426	2454	rBV	2068021	3370902	70.99%	9.460%
49	9.052	2471	2476	2479	rBV6	5392	6101	0.13%	0.017%
50	9.177	2509	2515	2522	rBV5	7587	11432	0.24%	0.032%
51	9.312	2554	2557	2561	rVB5	1703	1261	0.03%	0.004%
52	9.347	2562	2568	2571	rBV7	1909	1921	0.04%	0.005%
53	9.412	2586	2588	2593	rVB6	1913	1469	0.03%	0.004%
54	9.463	2599	2604	2607	rBV6	1783	1392	0.03%	0.004%
55	9.482	2607	2610	2613	rVB5	1977	1209	0.03%	0.003%
56	9.518	2619	2621	2625	rVB4	1623	961	0.02%	0.003%
57	9.537	2625	2627	2630	rBV4	1366	910	0.02%	0.003%
58	9.601	2634	2647	2653	rBV4	8468	19973	0.42%	0.056%
59	9.688	2670	2674	2675	rBV3	1670	1133	0.02%	0.003%
60	9.736	2685	2689	2692	rBV6	2455	2062	0.04%	0.006%
61	9.929	2744	2749	2751	rBV5	1656	1099	0.02%	0.003%
62	9.971	2757	2762	2763	rBV3	2924	2521	0.05%	0.007%
63	10.029	2775	2780	2783	rVB7	2080	1633	0.03%	0.005%
64	10.190	2827	2830	2833	rBV3	1876	1210	0.03%	0.003%
65	10.257	2836	2851	2877	rBV	1402087	2231288	46.99%	6.262%
66	10.421	2892	2902	2918	rVB	25930	45665	0.96%	0.128%
67	10.717	2991	2994	2996	rBV3	2050	1386	0.03%	0.004%
68	10.765	3004	3009	3012	rVB6	2165	1504	0.03%	0.004%
69	10.781	3012	3014	3018	rVB3	1859	1242	0.03%	0.003%
70	10.900	3042	3051	3054	rBV9	3857	6216	0.13%	0.017%
71	10.949	3062	3066	3068	rBV2	3624	2961	0.06%	0.008%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102319\
 Data File : VV013309.D
 Acq On : 23 Oct 2019 21:22
 Operator : SY/MD
 Sample : K5395-18
 Misc : 5.00ML/MSVOA V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0051

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102319WMA.M
 Title : VOC Analysis

72	11.061	3097	3101	3108	rBV8	1553	1986	0.04%	0.006%
73	11.132	3120	3123	3124	rBV3	1487	876	0.02%	0.002%
74	11.174	3134	3136	3140	rBV3	1507	1168	0.02%	0.003%
75	11.219	3140	3150	3158	rVV9	6048	11178	0.24%	0.031%
76	11.289	3161	3172	3194	rVV	1921104	2968656	62.52%	8.331%
77	11.582	3255	3263	3267	rBV9	5703	8444	0.18%	0.024%
78	11.666	3276	3289	3308	rBV	2198191	3472387	73.12%	9.745%
79	11.788	3324	3327	3331	rBV5	2037	1547	0.03%	0.004%
80	11.884	3354	3357	3360	rBV5	1830	1307	0.03%	0.004%
81	12.071	3412	3415	3417	rBV4	1759	1089	0.02%	0.003%
82	12.116	3427	3429	3436	rVB7	1776	1559	0.03%	0.004%
83	12.209	3456	3458	3461	rBV3	1447	966	0.02%	0.003%
84	12.289	3477	3483	3489	rVB7	5992	8261	0.17%	0.023%
85	12.322	3489	3493	3496	rBV5	1107	1150	0.02%	0.003%
86	12.399	3509	3517	3525	rBV5	4328	8202	0.17%	0.023%
87	12.479	3539	3542	3547	rVB6	3055	2939	0.06%	0.008%
88	12.505	3547	3550	3553	rBV5	1413	1422	0.03%	0.004%
89	12.559	3562	3567	3572	rBV9	1932	2079	0.04%	0.006%
90	12.595	3576	3578	3581	rVV4	1638	1017	0.02%	0.003%
91	12.691	3600	3608	3620	rVB4	17669	29351	0.62%	0.082%
92	12.842	3649	3655	3656	rBV4	2218	1955	0.04%	0.005%
93	12.929	3678	3682	3686	rBV6	1898	1810	0.04%	0.005%
94	13.013	3705	3708	3711	rBV5	1857	1552	0.03%	0.004%
95	13.158	3751	3753	3757	rVB4	2567	1649	0.03%	0.005%
96	13.180	3757	3760	3762	rBV3	1560	1087	0.02%	0.003%
97	13.309	3794	3800	3811	rVB4	14055	21841	0.46%	0.061%
98	13.717	3923	3927	3930	rBV6	2421	2173	0.05%	0.006%
99	13.791	3941	3950	3959	rBV3	19356	32776	0.69%	0.092%
100	14.093	4041	4044	4046	rBV4	1963	1429	0.03%	0.004%


Sum of corrected areas: 35632088

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV102319\
Data File : VV013309.D
Acq On : 23 Oct 2019 21:22
Operator : SY/MD
Sample : K5395-18
Misc : 5.00ML/MSVOA V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0051

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

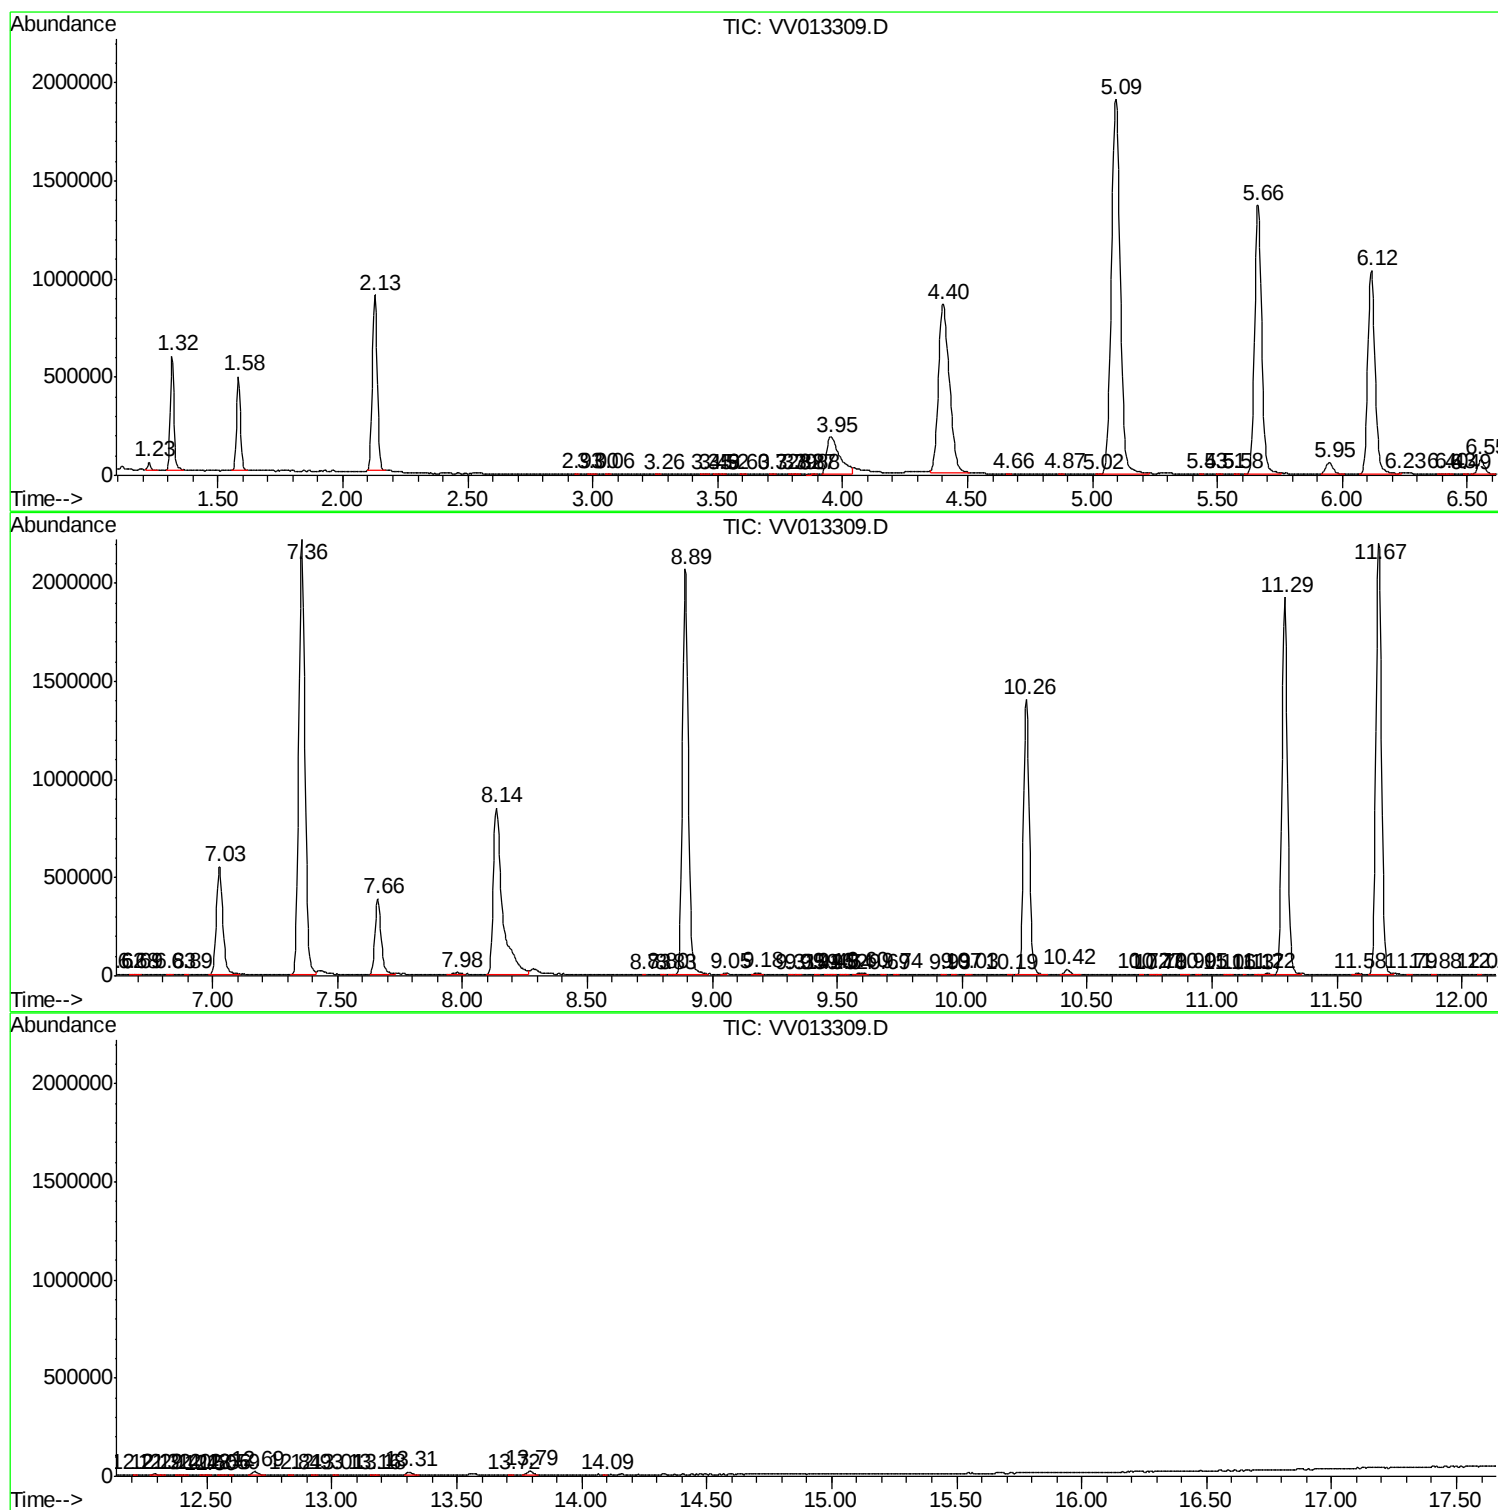

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV102319\
Data File : VV013309.D
Acq On : 23 Oct 2019 21:22
Operator : SY/MD
Sample : K5395-18
Misc : 5.00ML/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0051

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV102319\
Data File : VV013309.D
Acq On : 23 Oct 2019 21:22
Operator : SY/MD
Sample : K5395-18
Misc : 5.00ML/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0051

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc