


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV102319\
 Data File : VV013291.D
 Acq On : 23 Oct 2019 09:13
 Operator : SY/MD
 Sample : BFB74
 Misc : 5.00ML/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB74

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102319WMA.M
 Title : VOC Analysis
 Last Update : Thu Oct 24 04:17:57 2019

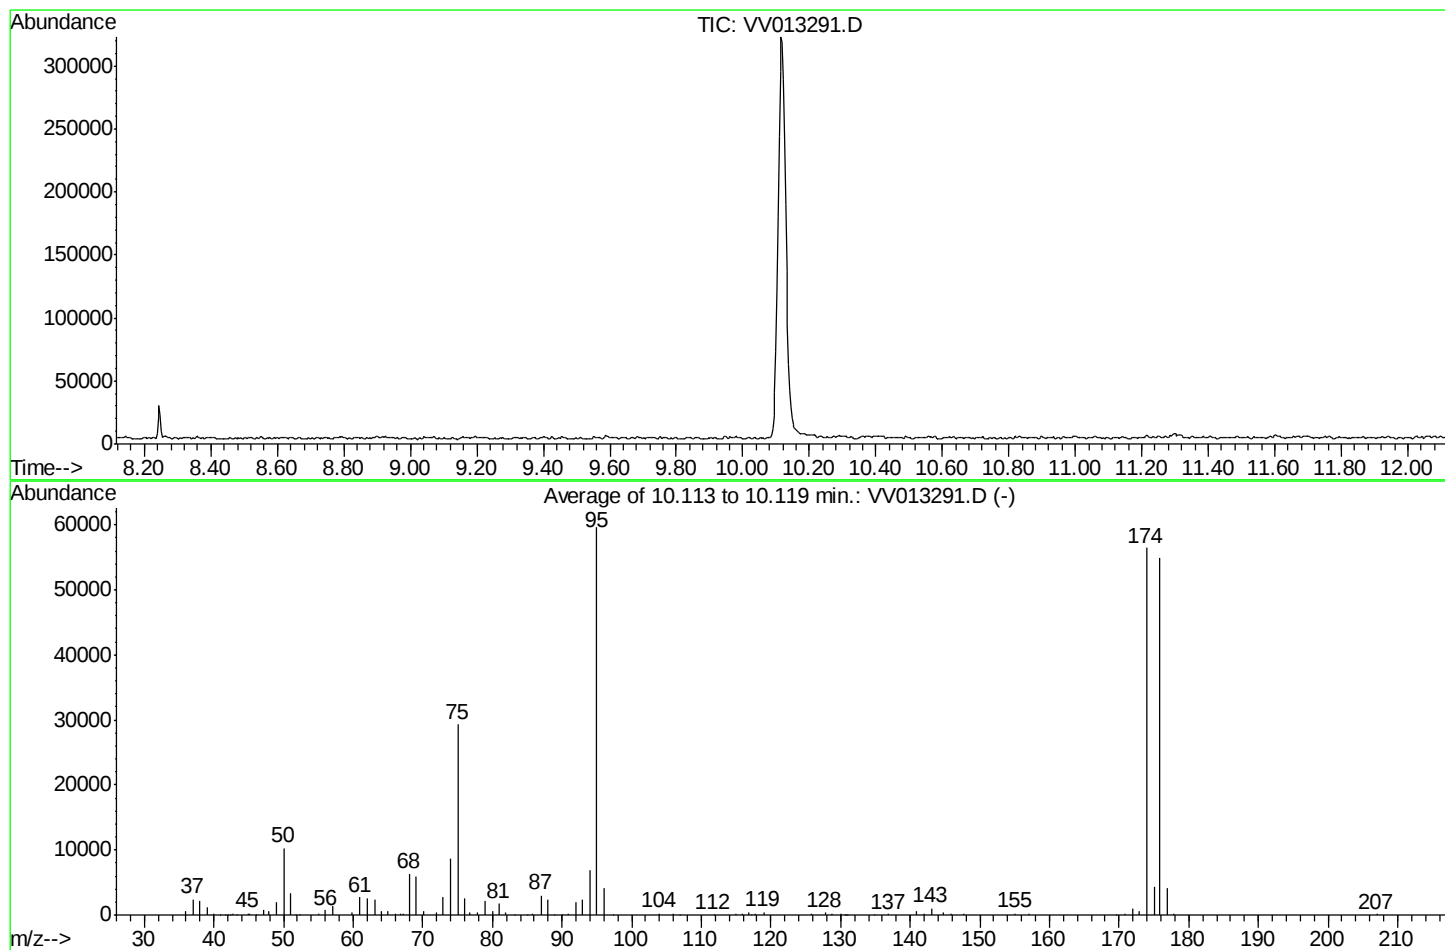

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.3	10283	PASS
75	95	30	80	49.1	29285	PASS
95	95	100	100	100.0	59608	PASS
96	95	5	9	6.9	4124	PASS
173	174	0.00	2	1.1	634	PASS
174	95	50	120	94.7	56461	PASS
175	174	5	9	7.5	4260	PASS
176	174	95	101	97.4	54970	PASS
177	176	5	9	7.5	4115	PASS

m/z	Abundance
36.10	688.0
37.00	2329.0
38.00	2472.0
39.00	974.0
39.90	1281.0
40.80	110.0
41.60	109.0
42.70	123.0
43.20	148.0
44.00	1511.0
44.90	344.0
45.10	335.0
46.20	126.0
47.10	757.0
47.80	693.0
49.00	2183.0
50.00	10169.0
51.00	3232.0
53.10	145.0
55.00	179.0
56.00	782.0
57.00	1653.0
59.80	435.0
61.00	2705.0
62.00	2719.0
63.10	2320.0
64.10	726.0
65.00	439.0
66.00	131.0
66.70	248.0
67.10	202.0
68.00	6342.0
69.00	5408.0
70.00	562.0
71.90	282.0
73.00	2662.0
74.00	8398.0
75.00	27880.0
76.00	2252.0
76.80	514.0
77.80	265.0
78.90	2051.0
79.90	542.0
80.90	1664.0
81.90	382.0
85.00	109.0
85.80	204.0
86.90	2703.0
87.90	2140.0
88.90	109.0
90.90	190.0
92.00	2096.0
92.90	2575.0
94.00	6324.0
95.00	56912.0
96.00	3885.0
97.30	107.0
104.00	255.0
105.90	185.0
111.80	115.0
114.90	157.0
115.90	256.0
116.80	278.0
117.10	301.0
117.80	244.0
119.00	421.0
125.80	128.0
127.80	301.0
130.00	191.0
130.50	158.0
131.10	177.0
136.90	230.0
141.00	644.0
142.00	136.0
143.00	1001.0
144.70	396.0
155.10	212.0
156.90	116.0
170.80	262.0
172.00	949.0
173.90	51672.0
175.00	4001.0
175.90	51496.0
176.90	4038.0
177.90	142.0
207.00	104.0

Instrument :
MSVOA_V
ClientSampleId :
BFB74

m/z	Abundance
36.00	759.0
37.00	2507.0
38.00	2455.0
39.00	1121.0
39.90	1355.0
40.80	108.0
41.70	101.0
42.30	125.0
42.70	134.0
43.30	130.0
44.00	1358.0
44.90	374.0
45.20	364.0
46.20	141.0
47.10	931.0
47.80	549.0
49.10	2152.0
50.00	10524.0
51.00	3603.0
52.30	120.0
53.10	183.0
55.00	236.0
56.00	733.0
57.00	1494.0
59.90	437.0
61.00	2783.0
62.00	2617.0
63.00	2512.0
64.10	840.0
65.10	485.0
66.10	138.0
66.80	244.0
67.10	174.0
68.00	6615.0
69.00	6128.0
70.10	579.0
71.90	294.0
72.90	2750.0
74.00	8700.0
75.00	30296.0
76.10	2583.0
76.80	567.0
77.80	345.0
78.90	2185.0
79.90	555.0
80.90	1803.0
81.90	344.0
83.30	109.0
85.00	116.0
85.80	194.0
86.90	3137.0
87.90	2391.0
88.80	150.0
90.80	264.0
92.00	2136.0
93.00	2396.0
94.00	7154.0
95.00	61936.0
96.00	4236.0
104.00	274.0
106.00	228.0
106.80	143.0
114.90	173.0
115.90	256.0
116.80	417.0
117.80	304.0
119.00	458.0
125.80	156.0
127.80	338.0
128.70	150.0
130.00	262.0
130.60	133.0
131.00	115.0
134.90	120.0
136.90	177.0
141.00	675.0
142.00	189.0
143.00	1122.0
144.80	436.0
145.80	267.0
147.70	161.0
155.10	309.0
157.00	122.0
170.80	252.0
172.00	1000.0
173.00	1003.0
173.90	58264.0
175.00	4456.0
175.90	56784.0
177.00	4257.0
177.90	179.0
207.00	105.0

Instrument :
MSVOA_V
ClientSampleId :
BFB74

m/z	Abundance
35.90	665.0
37.00	2490.0
38.00	2351.0
39.00	1246.0
39.90	1458.0
42.00	152.0
42.70	108.0
44.00	1248.0
44.90	420.0
46.00	162.0
47.10	962.0
47.90	375.0
49.10	1886.0
50.00	10156.0
51.00	3448.0
51.80	213.0
52.20	124.0
53.10	131.0
55.00	268.0
56.00	639.0
57.00	1302.0
59.90	446.0
61.00	2711.0
62.00	2550.0
63.00	2355.0
64.10	759.0
65.10	592.0
66.10	106.0
66.80	232.0
68.00	6151.0
69.00	6098.0
70.20	574.0
71.90	375.0
73.00	2902.0
74.00	8892.0
75.00	29680.0
76.10	2577.0
76.80	546.0
77.80	387.0
78.90	2225.0
80.00	605.0
80.90	1799.0
81.80	313.0
83.20	121.0
85.70	168.0
87.00	3121.0
87.90	2540.0
90.00	146.0
90.90	294.0
92.00	1792.0
93.10	2310.0
94.00	7163.0
95.00	59976.0
96.00	4251.0
104.00	269.0
106.00	271.0
106.80	171.0
114.90	138.0
115.80	200.0
116.80	508.0
117.70	313.0
118.90	382.0
125.80	106.0
127.80	325.0
128.80	179.0
130.00	302.0
130.80	133.0
134.70	144.0
136.90	133.0
140.90	691.0
142.00	183.0
143.10	1075.0
144.80	498.0
145.80	377.0
147.70	187.0
155.10	288.0
157.10	123.0
169.60	129.0
170.80	254.0
171.90	960.0
172.90	901.0
173.90	59448.0
175.00	4325.0
175.90	56632.0
177.00	4052.0
177.90	182.0
207.00	121.0

Instrument :
MSVOA_V
ClientSampleId :
BFB74

Scan 2795 (10.077 min): VV013291.D
BFB74

m/z	Abundance
36.20	164.0
37.80	179.0
40.00	1236.0
41.40	126.0
43.00	106.0
43.90	1414.0
44.90	165.0
46.00	140.0
52.50	165.0
53.10	190.0
64.00	193.0
76.70	144.0
78.50	168.0
104.40	116.0
146.90	124.0
208.00	107.0

Instrument :
MSVOA_V
ClientSampleId :
BFB74